

Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP092519\
 Data File : BP000410.D
 Acq On : 25 Sep 2019 15:17
 Operator : JU
 Sample : PB123346TB
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :

Quant Time: Sep 25 23:28:51 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA P\METHODS\8270-BP091619.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Sep 19 14:44:51 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.79	152	245730	20.00	ng	0.00
21) Naphthalene-d8	8.07	136	909359	20.00	ng	0.00
39) Acenaphthene-d10	9.83	164	498933	20.00	ng	0.00
64) Phenanthrene-d10	11.33	188	943592	20.00	ng	0.00
76) Chrysene-d12	14.00	240	862548	20.00	ng	0.00
87) Perylene-d12	15.48	264	923686	20.00	ng	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
5) 2-Fluorophenol	5.41	112	1541044	108.26	ng	0.00
7) Phenol-d6	6.42	99	2014895	115.48	ng	0.00
23) Nitrobenzene-d5	7.35	82	1099159	77.99	ng	0.00
42) 2,4,6-Tribromophenol	10.63	330	620292	125.34	ng	0.00
45) 2-Fluorobiphenyl	9.15	172	2429445	87.64	ng	0.00
79) Terphenyl-d14	12.93	244	3215130	78.20	ng	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
9) Benzaldehyde	6.42	77	2949	Below Cal		# 1
19) n-Nitroso-di-n-propylamine	7.35	70	133733	14.497	ng	# 75
25) Isophorone	7.35	82	1098646	39.366	ng	# 63
50) Dimethylphthalate	9.55	163	144609	4.254	ng	# 98
51) 2,6-Dinitrotoluene	9.83	165	65117	8.712	ng	# 30
57) 2,4-Dinitrotoluene	9.83	165	65319	6.685	ng	# 35
67) 4-Bromophenyl-phenylether	10.62	248	43286	4.057	ng	# 1
69) Atrazine	11.14	200	35	Below Cal		73

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP092519\
Data File : BP000410.D
Acq On : 25 Sep 2019 15:17
Operator : JU
Sample : PB123346TB
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :

Quant Time: Sep 25 23:28:51 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA P\METHODS\8270-BP091619.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Sep 19 14:44:51 2019
Response via : Initial Calibration

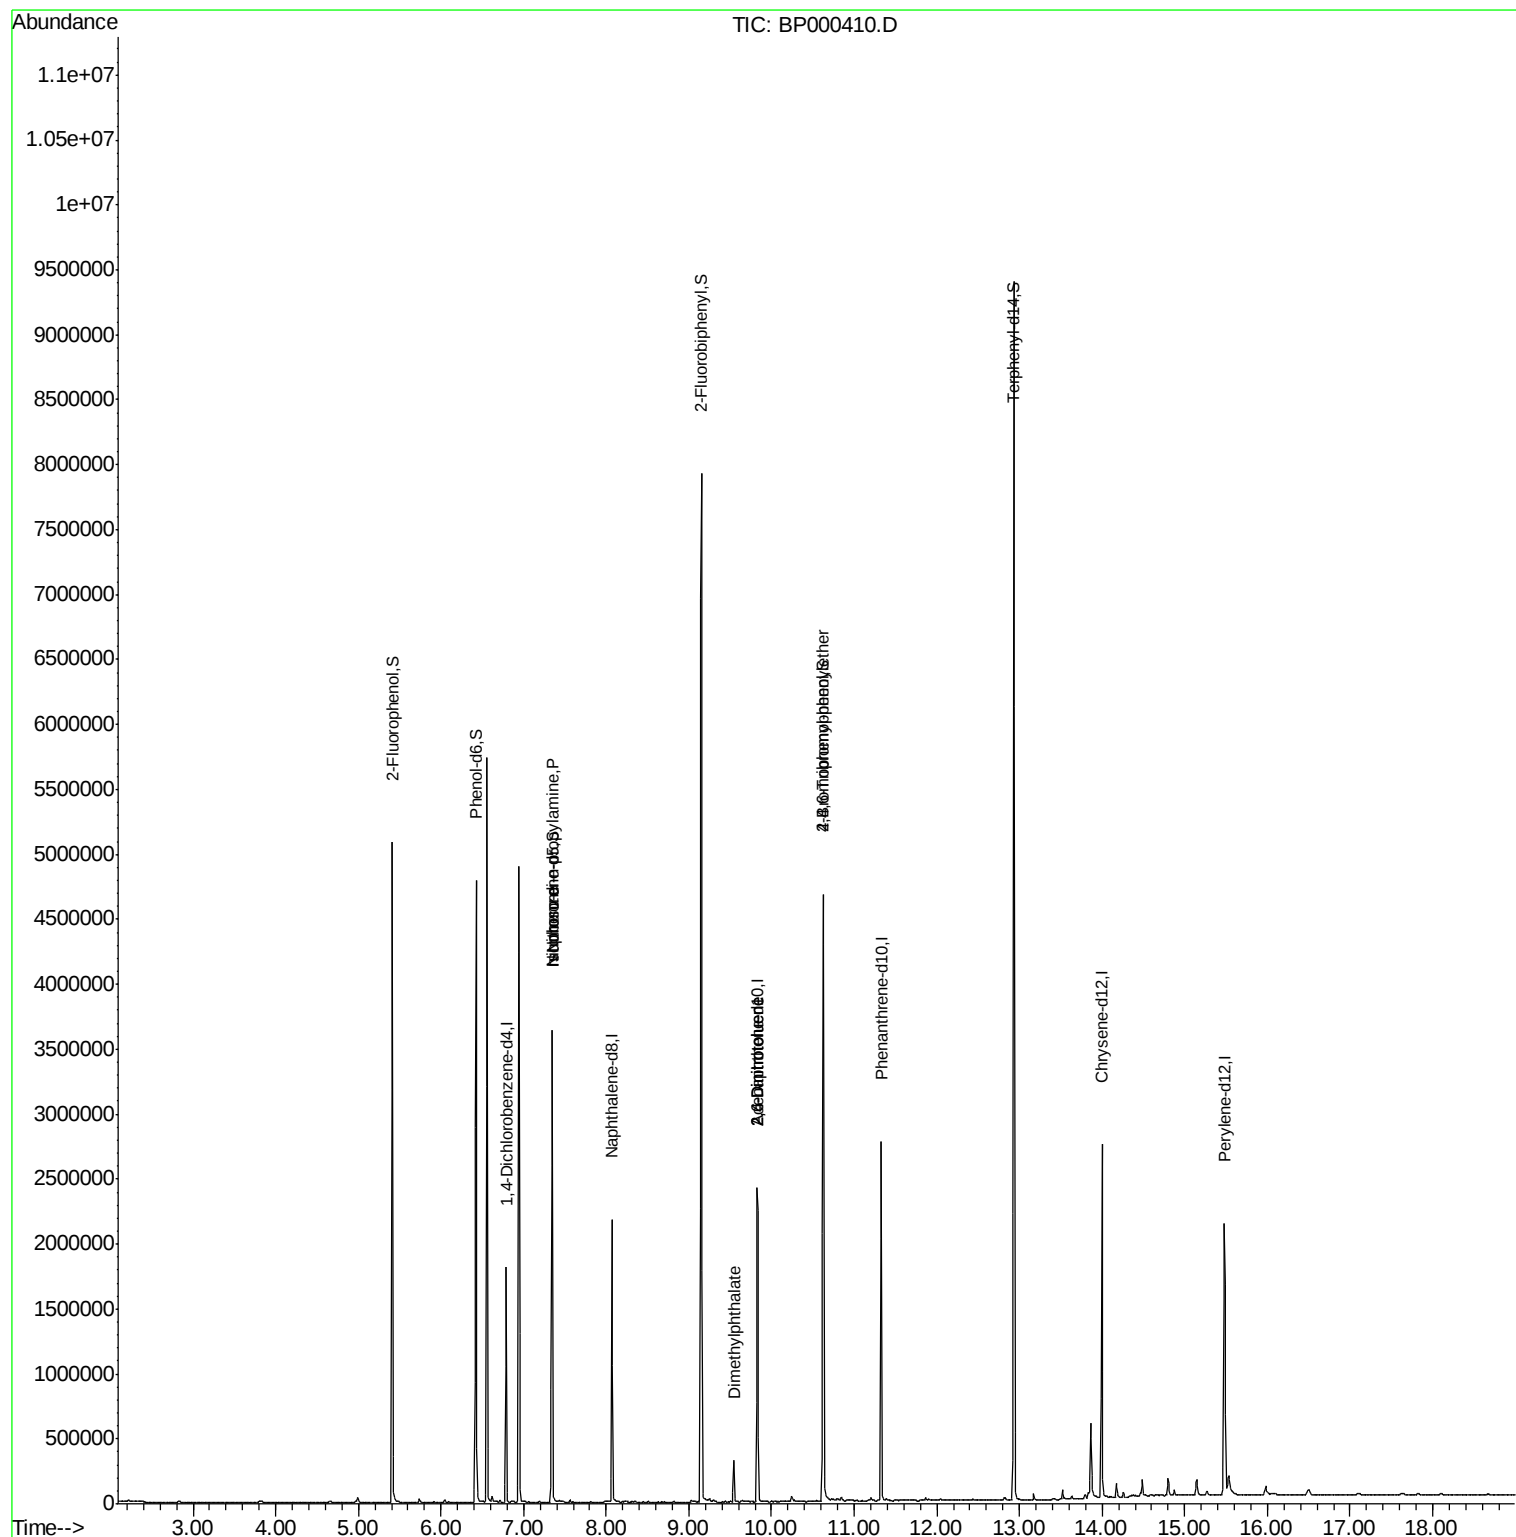




#1




1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 6.79 min Scan# 799
Delta R.T. -0.00 min
Lab File: BP000410.D
Acq: 25 Sep 2019 15:17

Instrument :
BNA_P
ClientSampleId :

Tot Ion	Ratio	Lower	Upper
152	100		
150	155.5	125.2	187.8
115	58.4	49.7	74.5

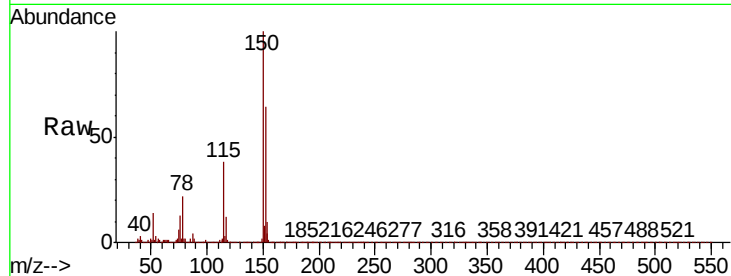


Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

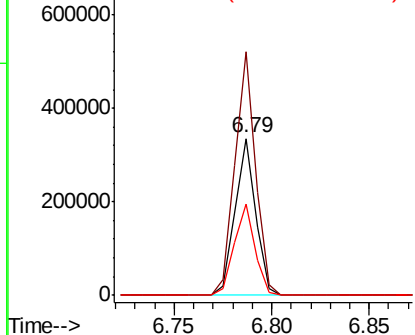



#5


2-Fluorophenol
Concen: 108.264 ng
RT: 5.41 min Scan# 565
Delta R.T. 0.01 min
Lab File: BP000410.D
Acq: 25 Sep 2019 15:17

Tgt Ion	Ratio	Lower	Upper
112	100		
64	44.4	36.2	54.4
63	22.9	18.3	27.5

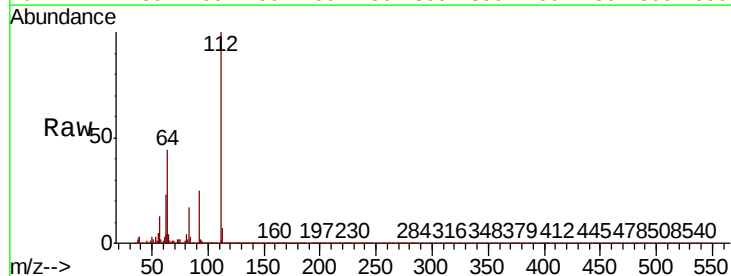

Abundance Ion 112.00 (111.70 to 112.70): E
Ion 64.00 (63.70 to 64.70): BP0
Ion 63.00 (62.70 to 63.70): BP0

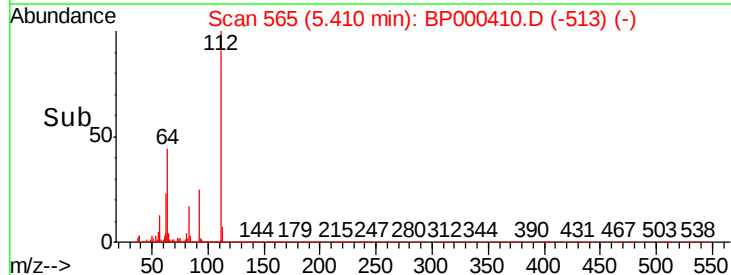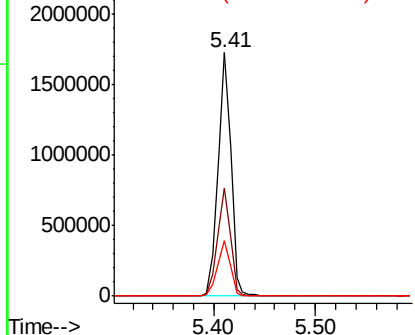

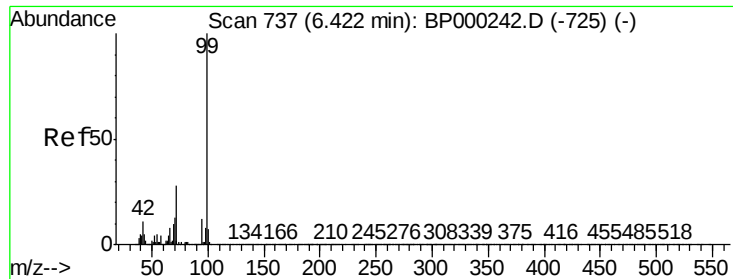

#7

Phenol-d6

Concen: 115.480 ng

RT: 6.42 min Scan# 737

Delta R.T. -0.00 min

Lab File: BP000410.D

Acq: 25 Sep 2019 15:17

Instrument :

BNA_P

ClientSampled :


Tot Ion: 99 Resp: 2014895

Ion Ratio Lower Upper

99 100

42 11.2 8.5 12.7




71 29.3 22.6 34.0

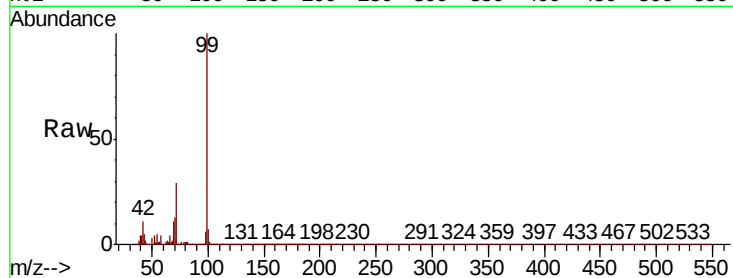

Abundance Ion 99.00 (98.70 to 99.70): BP0

Ion 42.00 (41.70 to 42.70): BP0

Ion 71.00 (70.70 to 71.70): BP0

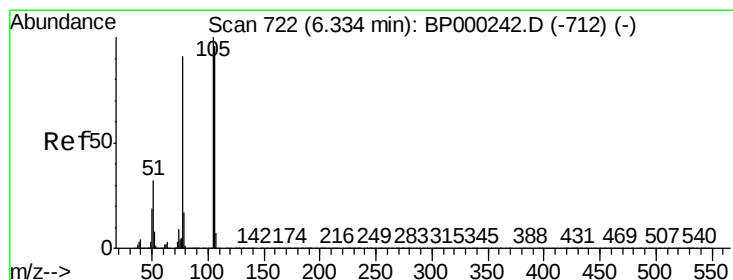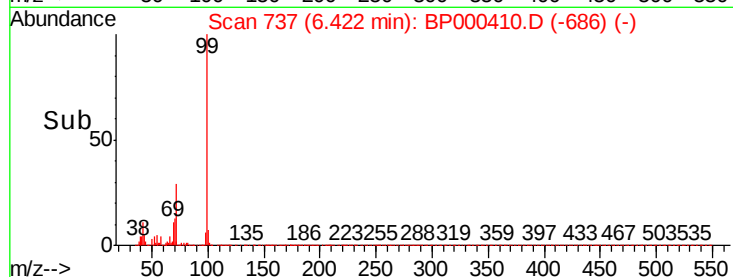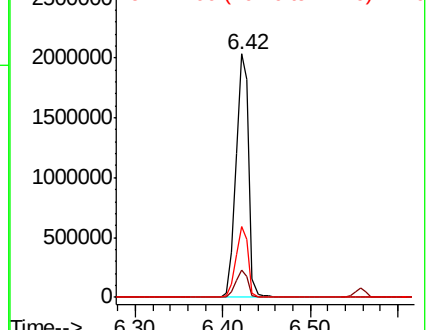

#9

Benzaldehyde

Concen: Below Cal

RT: 6.42 min Scan# 737

Delta R.T. 0.09 min

Lab File: BP000410.D

Acq: 25 Sep 2019 15:17


Tgt Ion: 77 Resp: 2949

Ion Ratio Lower Upper

77 100

105 3.5 89.6 129.6#



106 0.5 84.6 124.6#

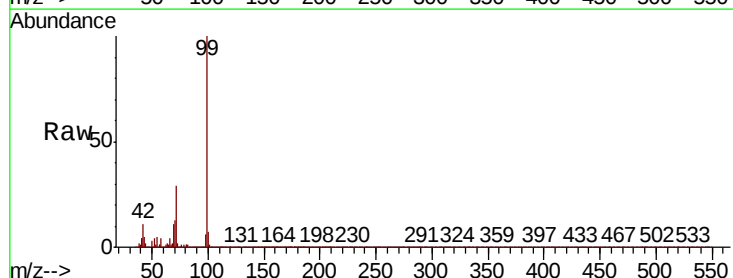


Abundance Ion 77.00 (76.70 to 77.70): BP0

Ion 105.00 (104.70 to 105.70): E

Ion 106.00 (105.70 to 106.70): E



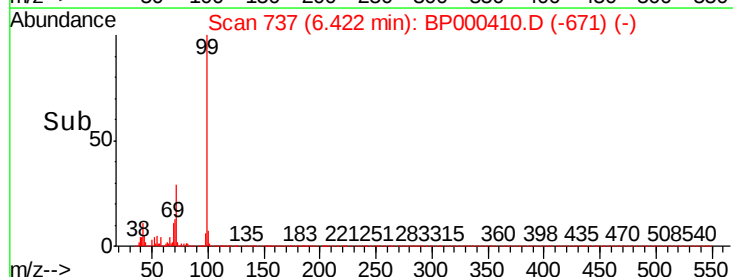
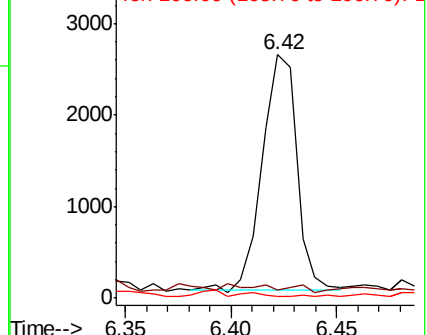


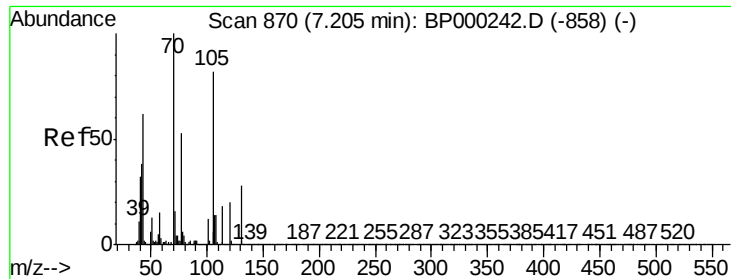

#19
n-Nitroso-di-n-propylamine
Concen: 14.497 ng
RT: 7.35 min Scan# 894
Delta R.T. 0.14 min
Lab File: BP000410.D
Acq: 25 Sep 2019 15:17




Instrument :
BNA_P
ClientSampled :


Tot Ion	Ratio	Lower	Upper
70	100		
42	33.9	30.7	46.1
101	0.0	9.6	14.4#
130	2.6	22.0	33.0#

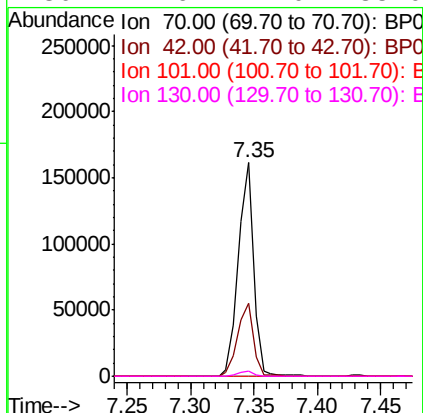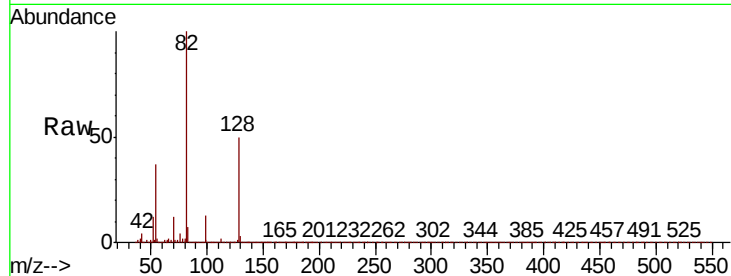

#21
Naphthalene-d8
Concen: 20.000 ng
RT: 8.07 min Scan# 1017
Delta R.T. -0.01 min
Lab File: BP000410.D
Acq: 25 Sep 2019 15:17

Tgt Ion	Ratio	Lower	Upper
136	100		
137	11.1	8.6	13.0
54	5.6	4.5	6.7
68	5.6	4.5	6.7


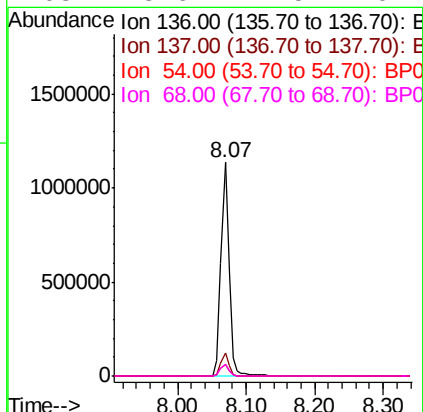




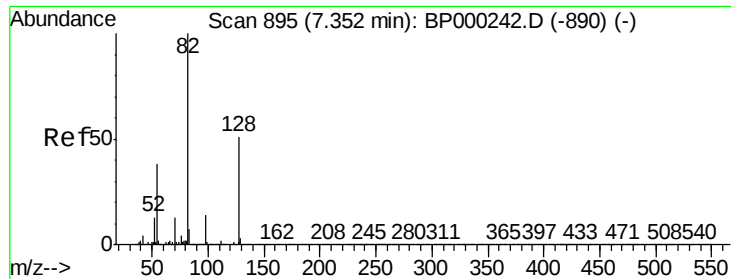

#23
Nitrobenzene-d5
Concen: 77.986 ng
RT: 7.35 min Scan# 894
Delta R.T. -0.01 min
Lab File: BP000410.D
Acq: 25 Sep 2019 15:17




Instrument :
BNA_P
ClientSampleId :


Tot Ion: 82 Resp: 1099159
Ion Ratio Lower Upper
82 100
128 50.3 40.7 61.1
54 37.0 30.1 45.1

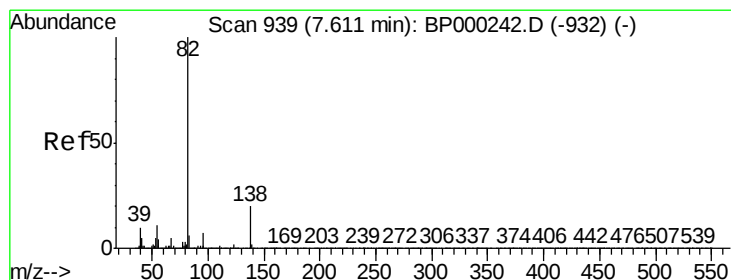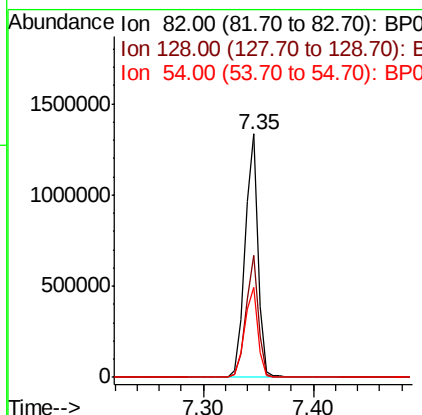

#25
Isophorone
Concen: 39.366 ng
RT: 7.35 min Scan# 894
Delta R.T. -0.26 min
Lab File: BP000410.D
Acq: 25 Sep 2019 15:17

Tgt Ion: 82 Resp: 1098646
Ion Ratio Lower Upper
82 100
95 0.0 5.9 8.9#
138 0.0 15.9 23.9#


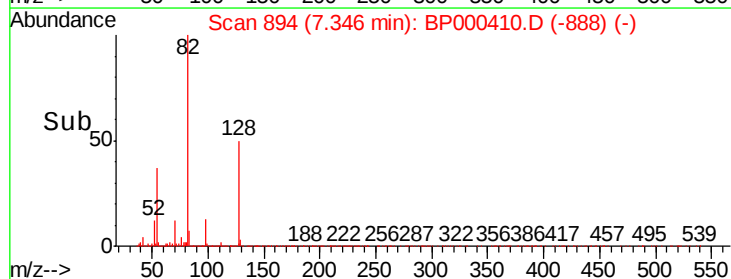
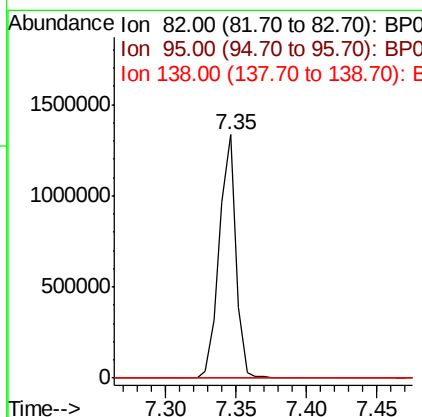
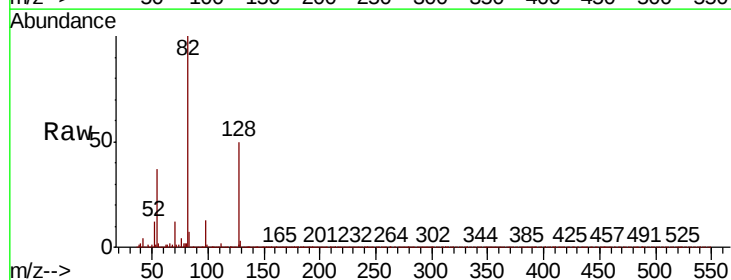


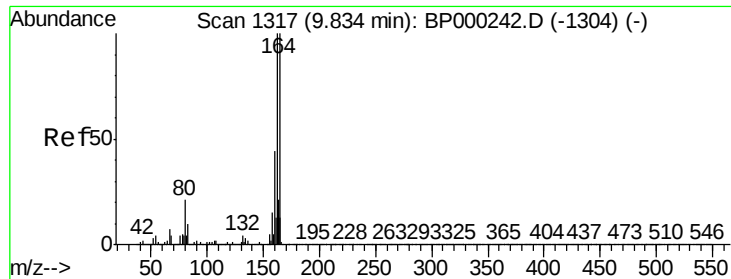

#39
 Acenaphthene-d10
 Concen: 20.000 ng
 RT: 9.83 min Scan# 1316
 Delta R.T. -0.01 min
 Lab File: BP000410.D
 Acq: 25 Sep 2019 15:17




Instrument :
 BNA_P
 ClientSampleId :


Tot Ion	Ratio	Lower	Upper
164	100		
162	100.1	79.9	119.9
160	44.6	35.6	53.4

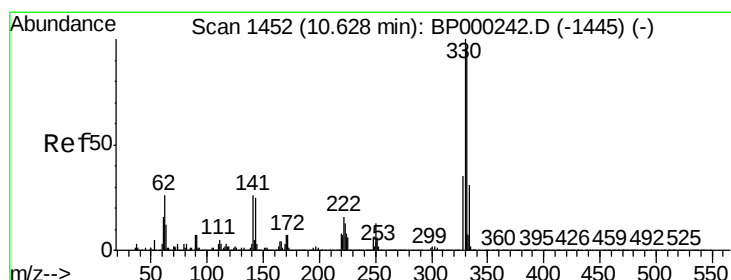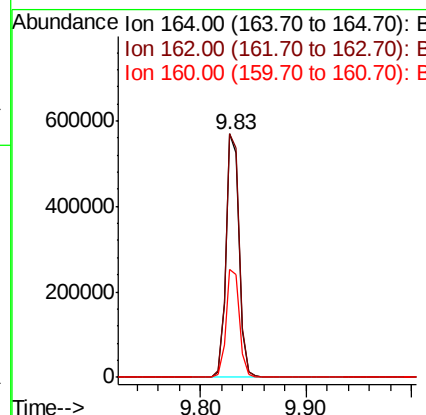

#42
 2,4,6-Tribromophenol
 Concen: 125.343 ng
 RT: 10.63 min Scan# 1452
 Delta R.T. -0.00 min
 Lab File: BP000410.D
 Acq: 25 Sep 2019 15:17

Tgt Ion	Ratio	Lower	Upper
330	100		
332	96.0	76.6	115.0
141	33.5	26.5	39.7



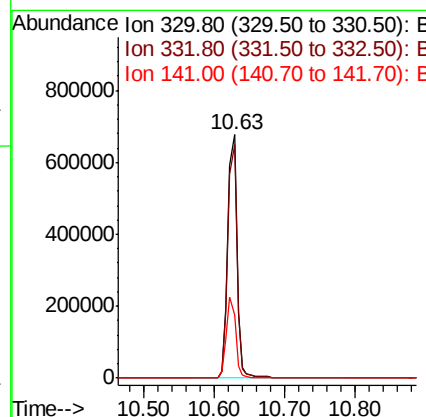
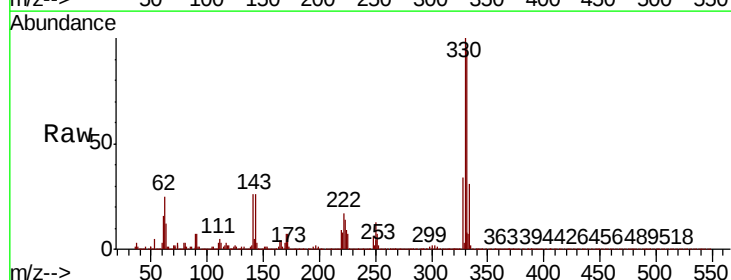


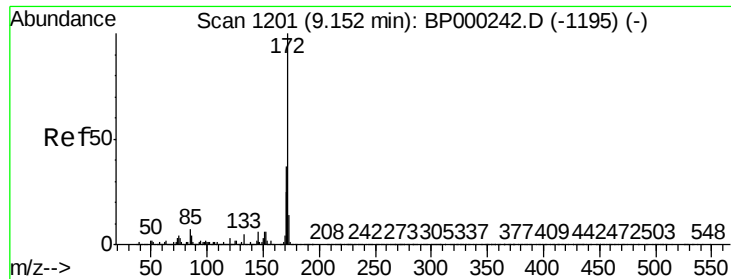

#45
2-Fluorobiphenyl
Concen: 87.638 ng
RT: 9.15 min Scan# 1201
Delta R.T. -0.00 min
Lab File: BP000410.D
Acq: 25 Sep 2019 15:17




Instrument :
BNA_P
ClientSampleId :


Tot Ion:172 Resp: 2429445
Ion Ratio Lower Upper
172 100
171 36.2 29.8 44.6
170 24.2 19.8 29.6

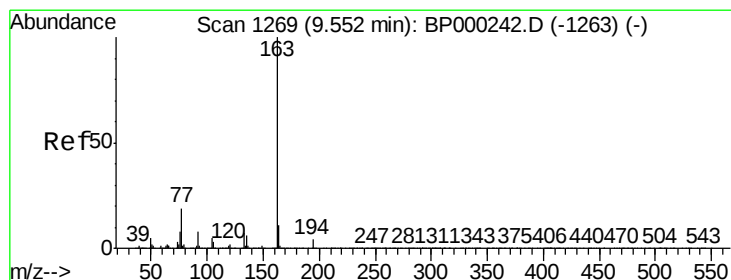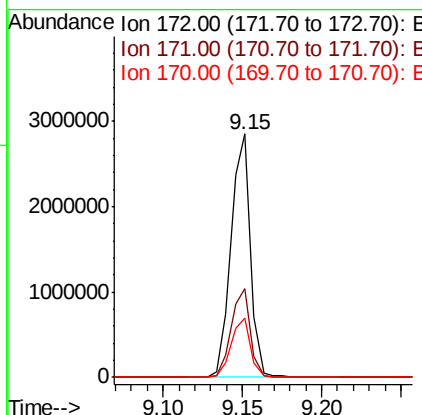

#50
Dimethylphthalate
Concen: 4.254 ng
RT: 9.55 min Scan# 1268
Delta R.T. -0.01 min
Lab File: BP000410.D
Acq: 25 Sep 2019 15:17

Tgt Ion:163 Resp: 144609
Ion Ratio Lower Upper
163 100
194 4.8 3.4 5.0
164 9.8 8.5 12.7

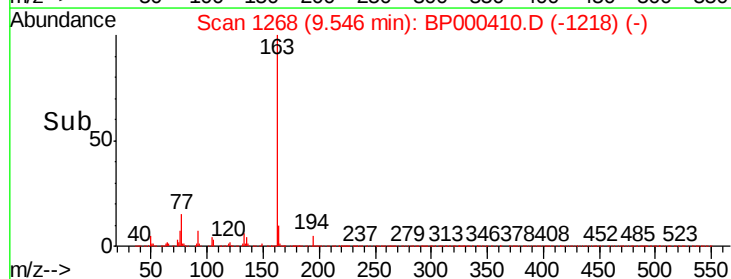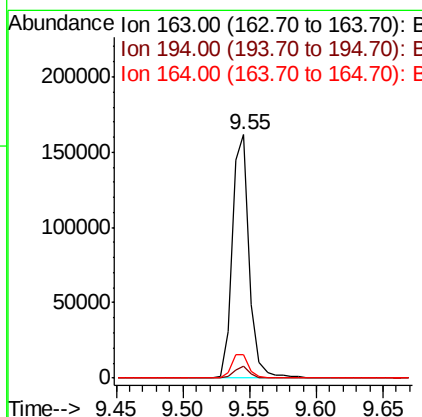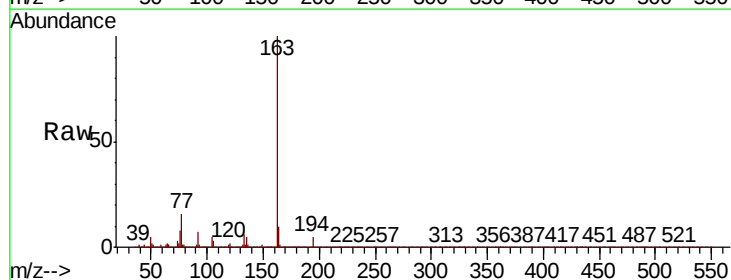



#51

2,6-Dinitrotoluene

Concen: 8.712 ng

RT: 9.83 min Scan# 1316

Delta R.T. 0.22 min

Lab File: BP000410.D

Acq: 25 Sep 2019 15:17

Instrument :

BNA_P

ClientSampleId :


Tot Ion:165 Resp: 65117

Ion Ratio Lower Upper

165 100

63 1.0 35.8 53.8#




89 1.2 42.6 63.8#

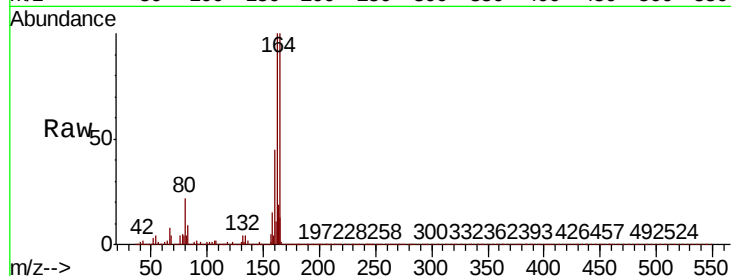

Abundance Ion 165.00 (164.70 to 165.70): E

Ion 63.00 (62.70 to 63.70): BP0

Ion 89.00 (88.70 to 89.70): BP0

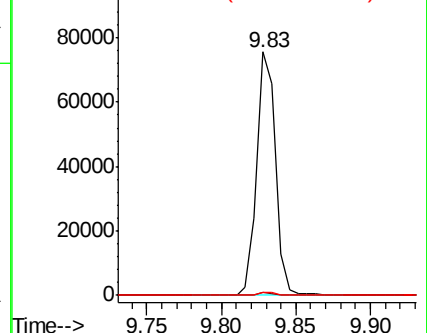

#57

2,4-Dinitrotoluene

Concen: 6.685 ng

RT: 9.83 min Scan# 1316

Delta R.T. -0.19 min

Lab File: BP000410.D

Acq: 25 Sep 2019 15:17

Tgt Ion:165 Resp: 65319


Ion Ratio Lower Upper

165 100

63 1.0 21.7 32.5#

89 1.2 45.0 67.6#

182 0.0 2.4 3.6#






Abundance Ion 165.00 (164.70 to 165.70): E

Ion 63.00 (62.70 to 63.70): BP0

Ion 89.00 (88.70 to 89.70): BP0

Ion 182.00 (181.70 to 182.70): E

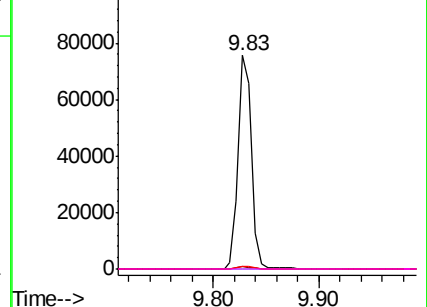



#64

Phenanthrene-d10

Concen: 20.000 ng

RT: 11.33 min Scan# 1571

Delta R.T. -0.00 min

Lab File: BP000410.D

Acq: 25 Sep 2019 15:17

Instrument :

BNA_P

ClientSampleId :


Tot Ion:188 Resp: 943592

Ion Ratio Lower Upper

188 100

94 9.6 8.5 12.7

80 9.7 8.6 13.0



Abundance Ion 188.00 (187.70 to 188.70): E

Ion 94.00 (93.70 to 94.70): BPO

Ion 80.00 (79.70 to 80.70): BPO

1500000



11.33

1000000

500000

0

Time-->



#67

4-Bromophenyl-phenylether

Concen: 4.057 ng

RT: 10.62 min Scan# 1451

Delta R.T. -0.25 min

Lab File: BP000410.D

Acq: 25 Sep 2019 15:17


Tgt Ion:248 Resp: 43286

Ion Ratio Lower Upper

248 100

250 201.3 77.0 115.4#

141 500.6 58.5 87.7#



Abundance Ion 248.00 (247.70 to 248.70): E

Ion 250.00 (249.70 to 250.70): E

Ion 141.00 (140.70 to 141.70): E

300000

250000

200000


150000


100000

50000

0

Time-->







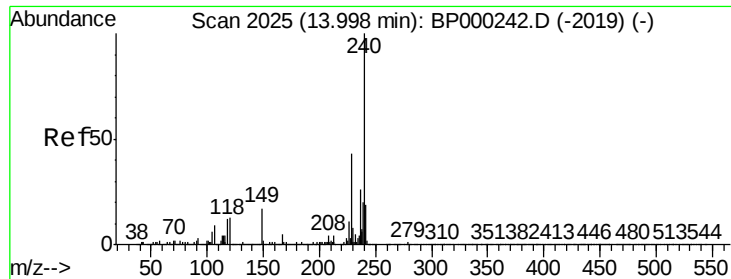

#76
 Chrysene-d12
 Concen: 20.000 ng
 RT: 14.00 min Scan# 2025
 Delta R.T. -0.00 min
 Lab File: BP000410.D
 Acq: 25 Sep 2019 15:17




Instrument :
 BNA_P
 ClientSampleId :


Tot Ion:240 Resp: 862548
 Ion Ratio Lower Upper
 240 100
 120 11.0 10.4 15.6
 236 26.4 21.0 31.6

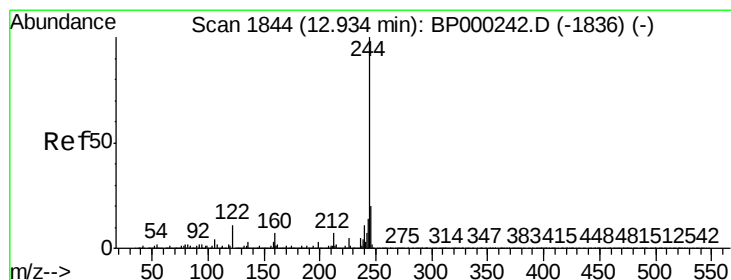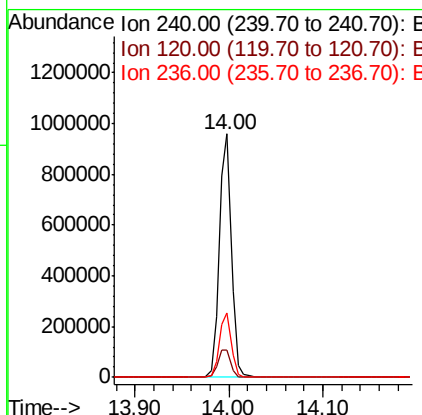

#79
 Terphenyl-d14
 Concen: 78.197 ng
 RT: 12.93 min Scan# 1844
 Delta R.T. -0.00 min
 Lab File: BP000410.D
 Acq: 25 Sep 2019 15:17

Tgt Ion:244 Resp: 3215130
 Ion Ratio Lower Upper
 244 100
 212 7.7 5.9 8.9
 122 11.9 9.0 13.4

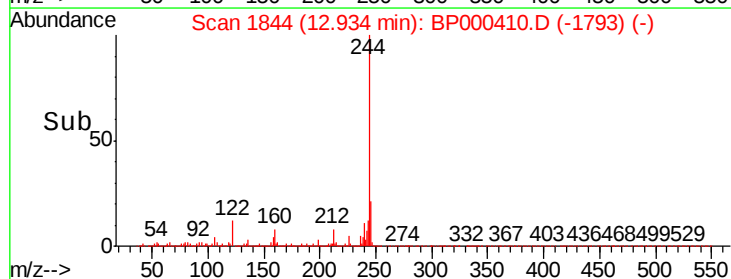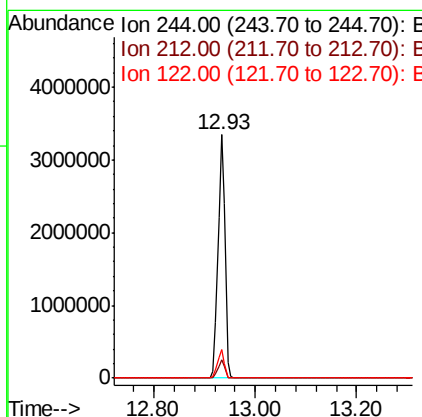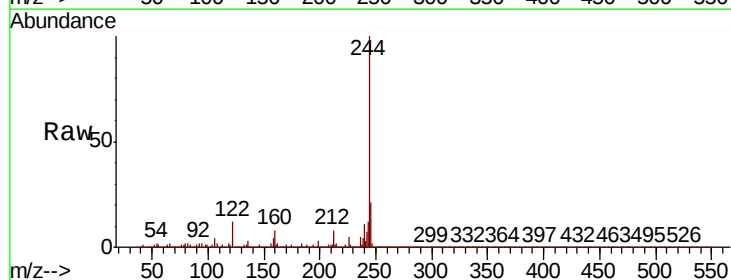




#87
Pervlene-d12
Concen: 20.000 ng
RT: 15.48 min Scan# 2277
Delta R.T. -0.00 min
Lab File: BP000410.D
Acq: 25 Sep 2019 15:17

Instrument :
BNA_P
ClientSampleId :

Tot Ion:	264	Resp:	923686
Ion	Ratio	Lower	Upper
264	100		
260	24.1	18.9	28.3
265	21.5	17.2	25.8



Abundance

Ion 264.00 (263.70 to 264.70): E

Ion 260.00 (259.70 to 260.70): E

Ion 265.00 (264.70 to 265.70): E

