


Data Path : Z:\SVOASRV\HPCHEM1\BNA_P\DATA\BP092519\
 Data File : BP000404.D
 Acq On : 25 Sep 2019 12:24
 Operator : JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP091619.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Sep 19 14:44:51 2019

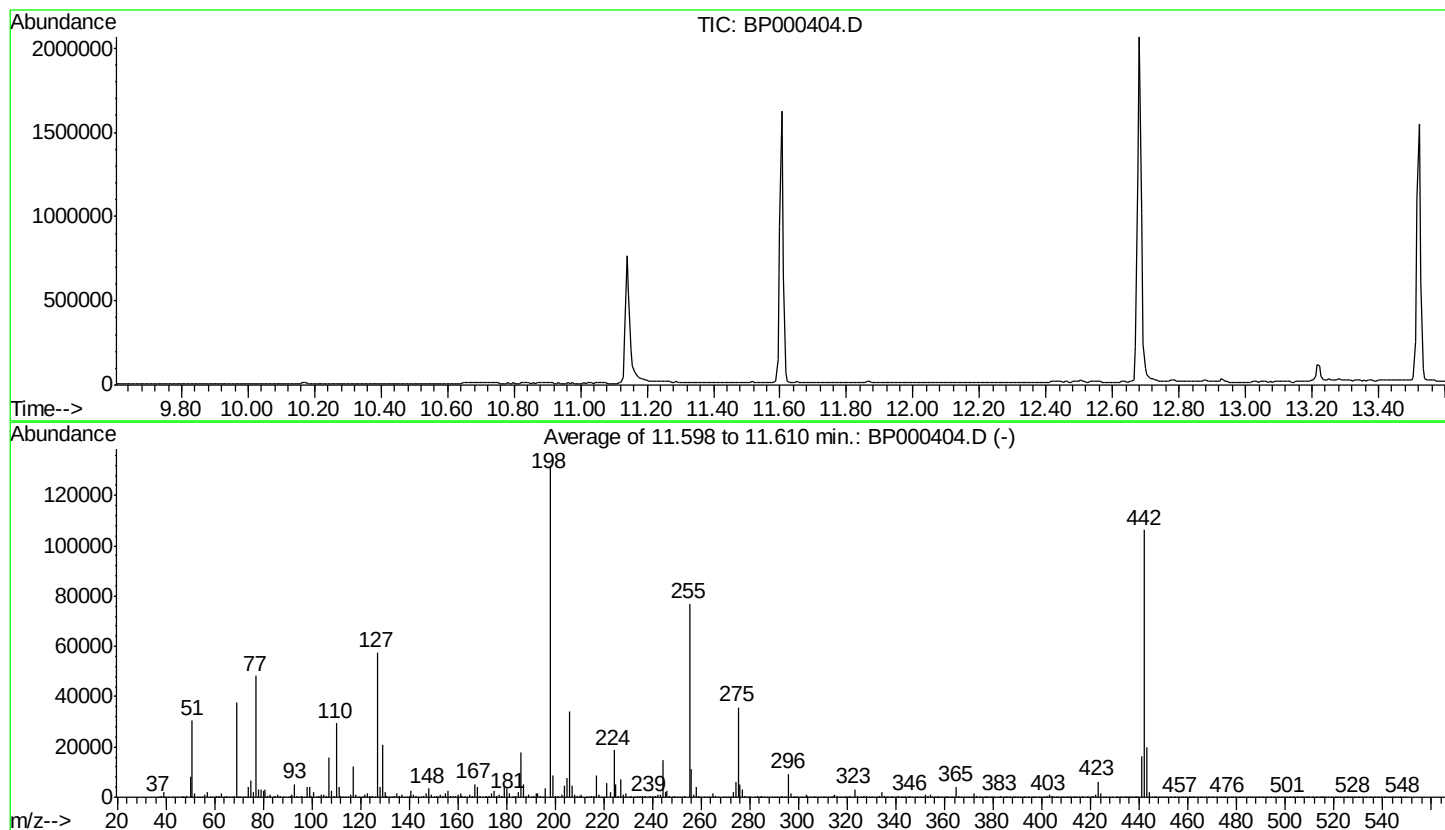

AutoFind: Scans 1617, 1618, 1619; Background Corrected with Scan 1611

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	23.0	30320	PASS
68	69	0.00	2	1.9	697	PASS
69	198	0.00	100	28.6	37642	PASS
70	69	0.00	2	0.3	104	PASS
127	198	10	80	43.5	57375	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	131840	PASS
199	198	5	9	6.7	8859	PASS
275	198	10	60	27.0	35656	PASS
365	198	1	100	3.2	4266	PASS
441	198	0.01	100	12.3	16256	PASS
442	198	50	100	80.6	106277	PASS
443	442	15	24	18.7	19879	PASS