

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP092521\
 Data File : BP007194.D
 Acq On : 25 Sep 2021 19:33
 Operator : CG/JU
 Sample : M3927-17
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :

Quant Time: Sep 26 02:16:03 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP092121.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Sep 23 11:17:25 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.881	152	203271	20.000	ng	-0.01
21) Naphthalene-d8	10.681	136	814441	20.000	ng	#-0.01
39) Acenaphthene-d10	14.510	164	517475	20.000	ng	-0.02
64) Phenanthrene-d10	17.263	188	1093926	20.000	ng	-0.01
76) Chrysene-d12	21.345	240	1088392	20.000	ng	#-0.01
86) Perylene-d12	23.751	264	1179523	20.000	ng	-0.02
System Monitoring Compounds						
5) 2-Fluorophenol	5.458	112	1249735	102.916	ng	0.00
7) Phenol-d6	7.052	99	1568903	94.530	ng	-0.01
23) Nitrobenzene-d5	9.040	82	909779	65.053	ng	-0.02
42) 2,4,6-Tribromophenol	16.004	330	732654	109.208	ng	-0.01
45) 2-Fluorobiphenyl	13.140	172	2369321	65.594	ng	-0.01
79) Terphenyl-d14	19.822	244	3697403	65.098	ng	-0.01


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP092521\
Data File : BP007194.D
Acq On : 25 Sep 2021 19:33
Operator : CG/JU
Sample : M3927-17
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :

Quant Time: Sep 26 02:16:03 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP092121.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Sep 23 11:17:25 2021
Response via : Initial Calibration



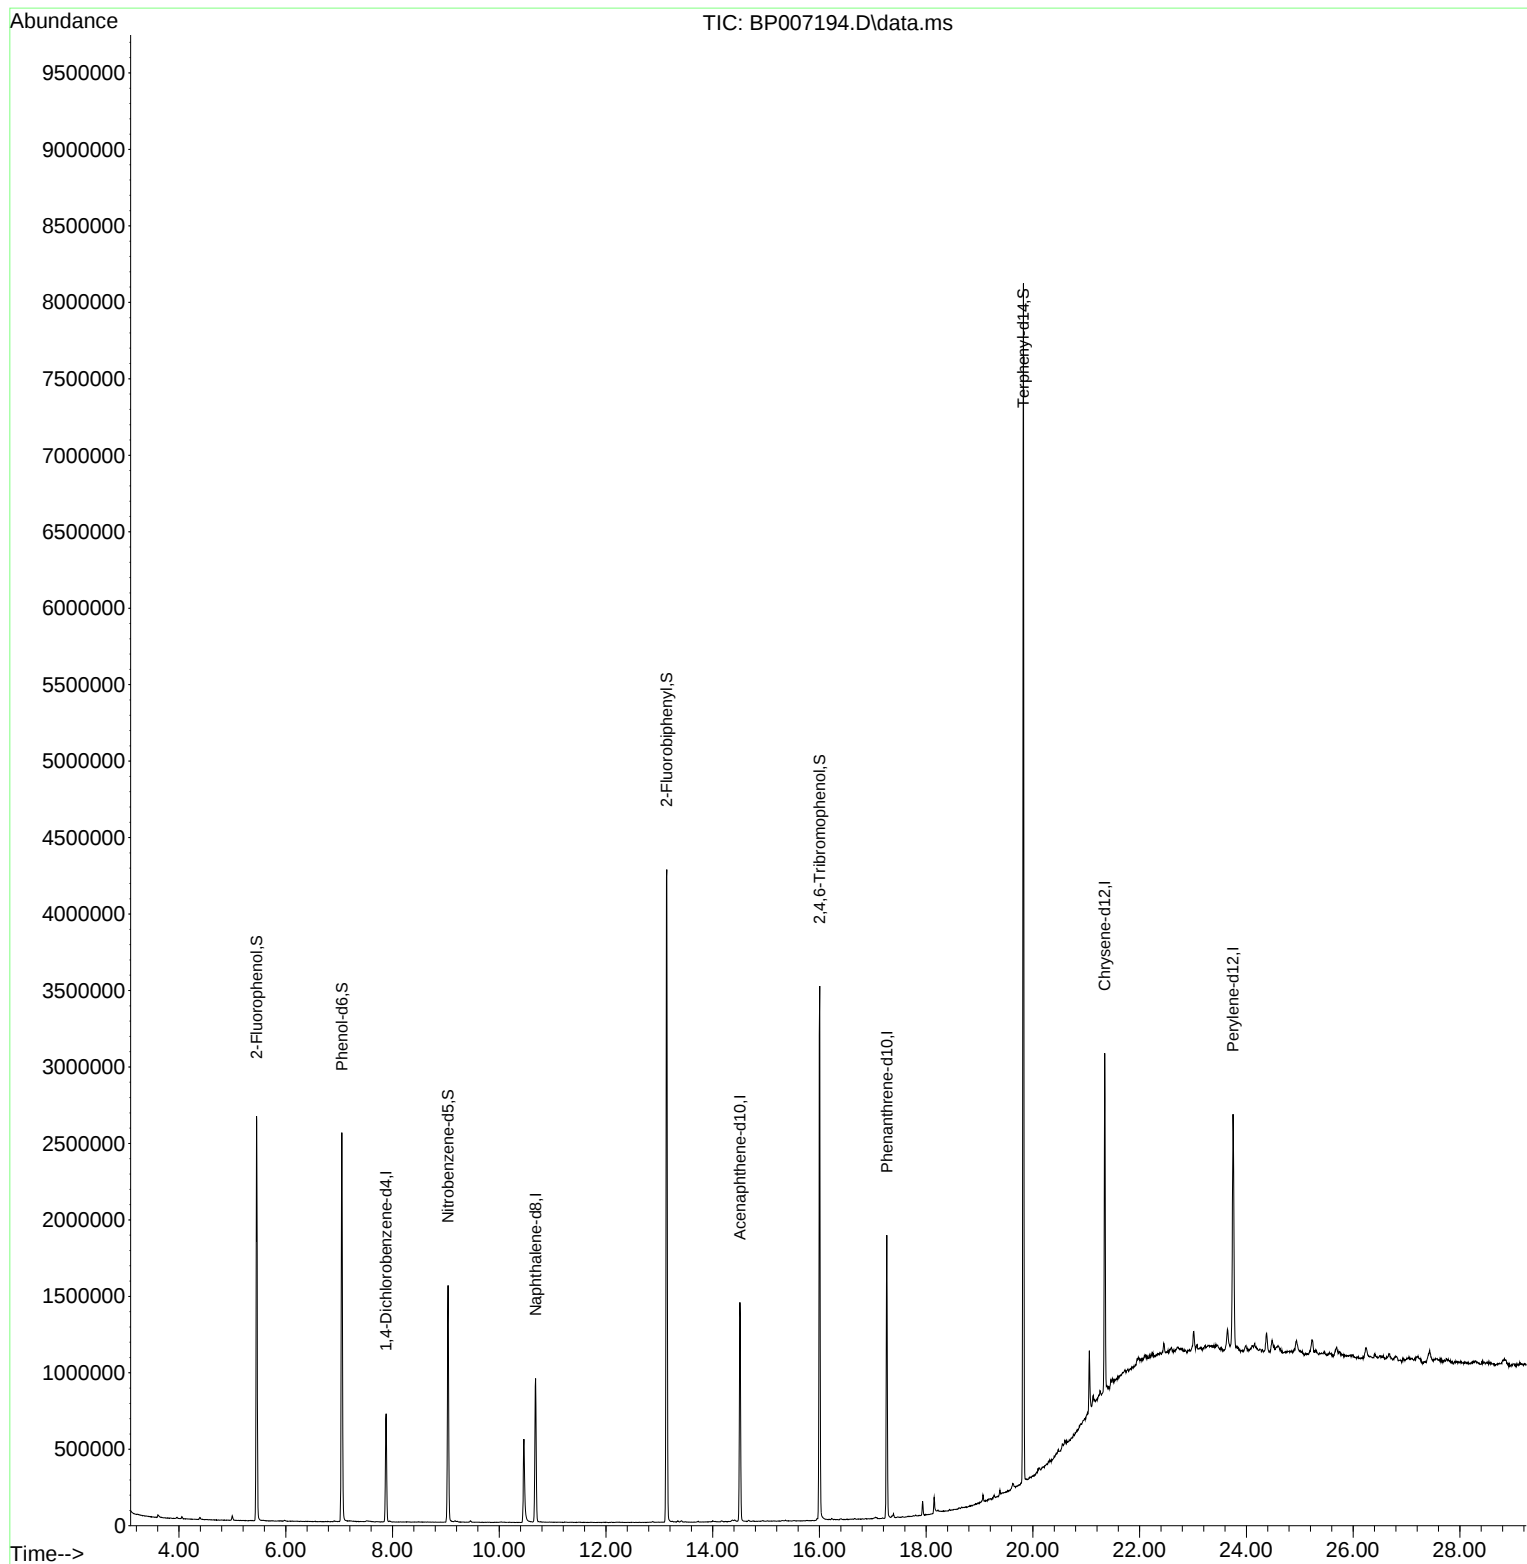




#1
1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 7.881 min Scan# 815
Delta R.T. -0.012 min
Lab File: BP007194.D
Acq: 25 Sep 2021 19:33




Instrument :
BNA_P
ClientSampleId :


Tgt Ion:152 Resp: 203271
Ion Ratio Lower Upper
152 100
150 151.7 125.6 188.4
115 54.9 48.5 72.7

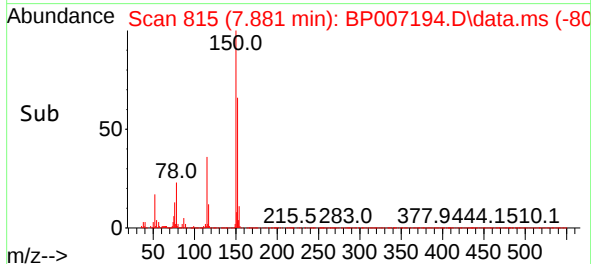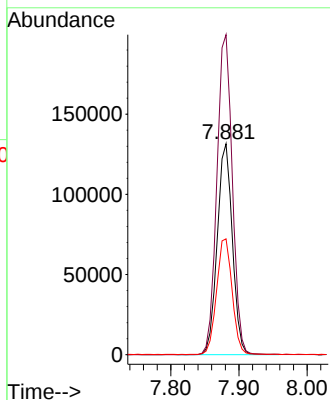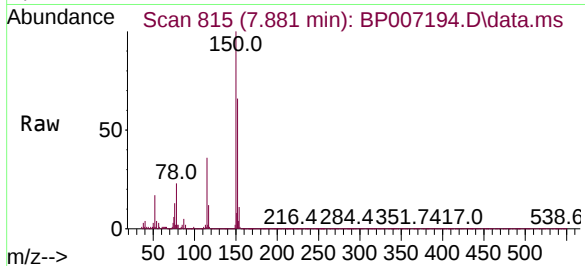

#5
2-Fluorophenol
Concen: 102.916 ng
RT: 5.458 min Scan# 403
Delta R.T. -0.006 min
Lab File: BP007194.D
Acq: 25 Sep 2021 19:33

Tgt Ion:112 Resp: 1249735
Ion Ratio Lower Upper
112 100
64 50.9 41.4 62.2
63 26.3 23.8 35.8

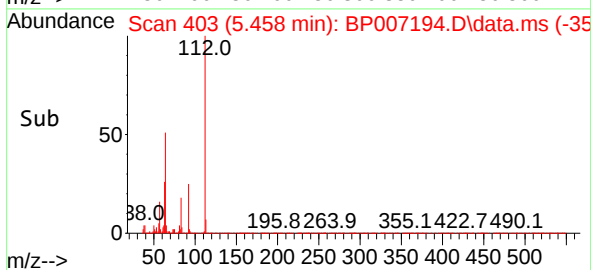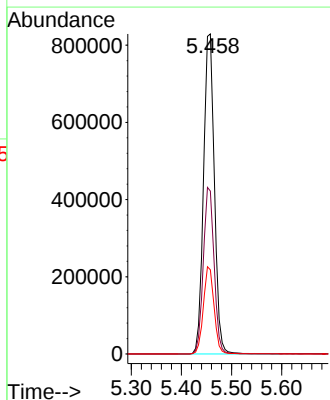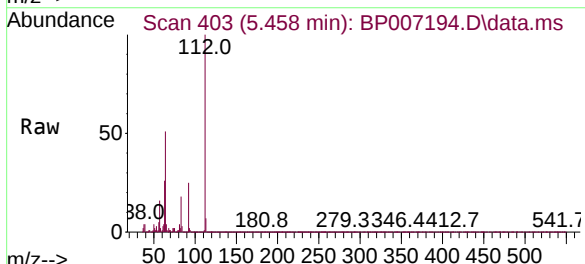







#7
Phenol-d6
Concen: 94.530 ng
RT: 7.052 min Scan# 674
Delta R.T. -0.012 min
Lab File: BP007194.D
Acq: 25 Sep 2021 19:33

Instrument :
BNA_P
ClientSampleId :

Tgt Ion: 99 Resp: 1568903




Ion	Ratio	Lower	Upper
99	100		
42	13.5	13.4	20.0
71	31.0	30.6	46.0

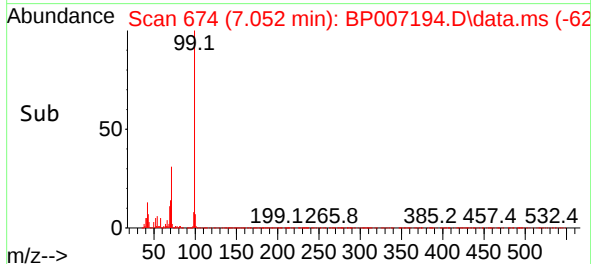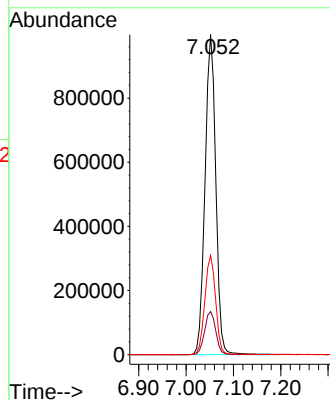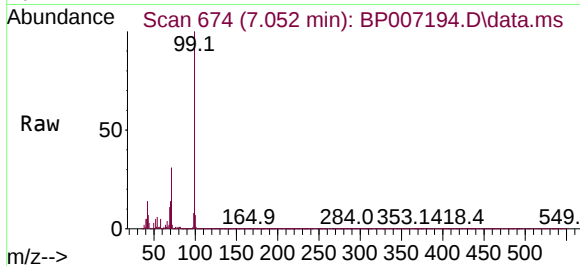


#21
Naphthalene-d8
Concen: 20.000 ng
RT: 10.681 min Scan# 1291
Delta R.T. -0.012 min
Lab File: BP007194.D
Acq: 25 Sep 2021 19:33

Tgt Ion: 136 Resp: 814441

Ion	Ratio	Lower	Upper
136	100		
137	10.6	8.6	12.8
54	7.0	4.6	6.8#
68	5.6	3.6	5.4#


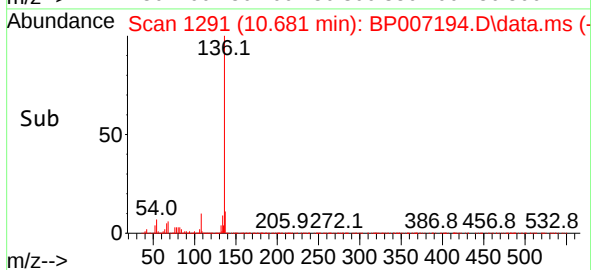
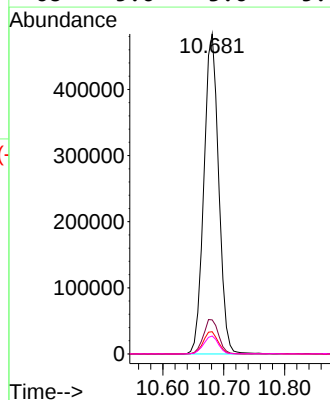
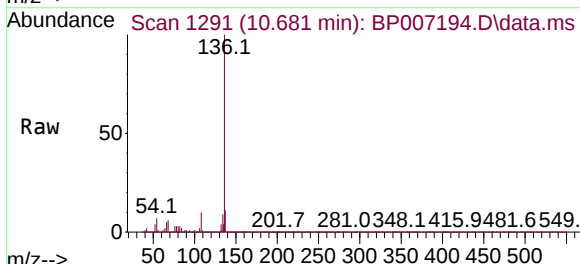


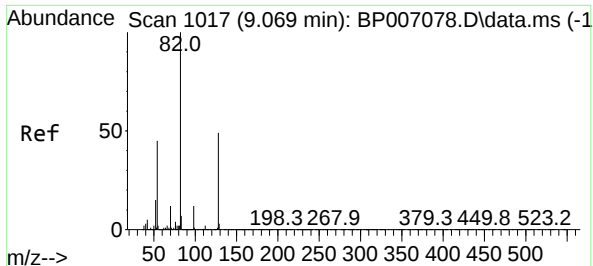

#23
Nitrobenzene-d5
Concen: 65.053 ng
RT: 9.040 min Scan# 1012
Delta R.T. -0.018 min
Lab File: BP007194.D
Acq: 25 Sep 2021 19:33




Instrument :
BNA_P
ClientSampled :


Tgt Ion: 82 Resp: 909779
Ion Ratio Lower Upper
82 100
128 47.6 35.7 53.5
54 45.1 35.0 52.4

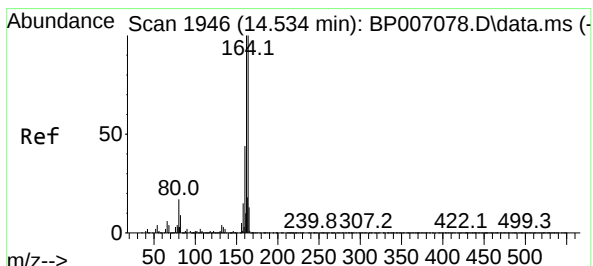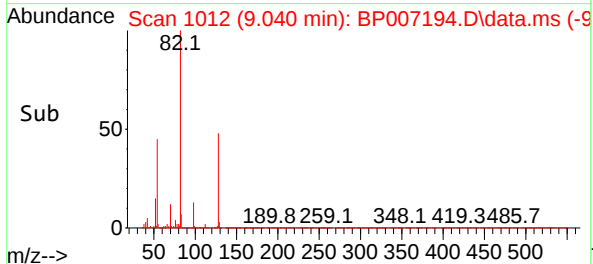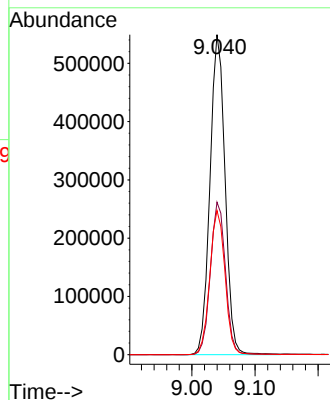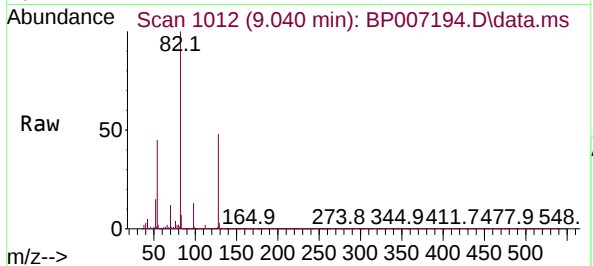

#39
Acenaphthene-d10
Concen: 20.000 ng
RT: 14.510 min Scan# 1942
Delta R.T. -0.018 min
Lab File: BP007194.D
Acq: 25 Sep 2021 19:33

Tgt Ion: 164 Resp: 517475
Ion Ratio Lower Upper
164 100
162 101.1 80.2 120.2
160 43.7 34.5 51.7


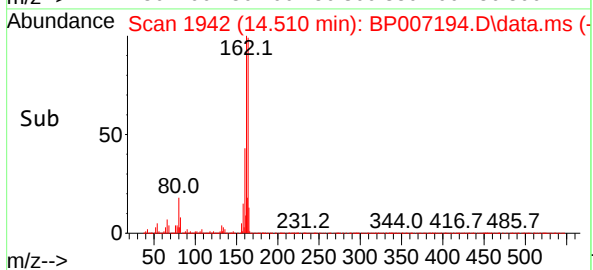
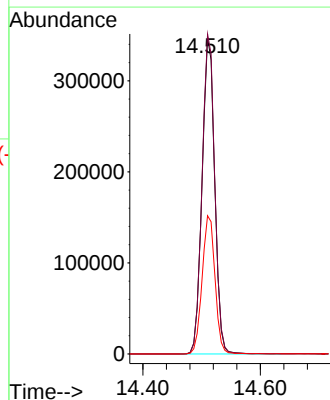
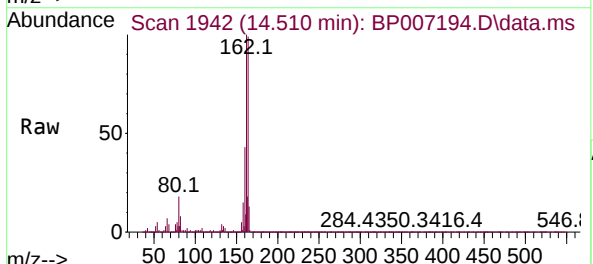




#42
2,4,6-Tribromophenol
Concen: 109.208 ng
RT: 16.004 min Scan# 2196
Delta R.T. -0.012 min
Lab File: BP007194.D
Acq: 25 Sep 2021 19:33




Instrument :
BNA_P
ClientSampleId :


Tgt Ion:330 Resp: 732654
Ion Ratio Lower Upper
330 100
332 97.4 77.8 116.8
141 28.4 25.4 38.2

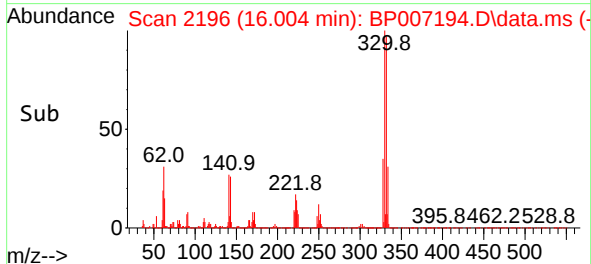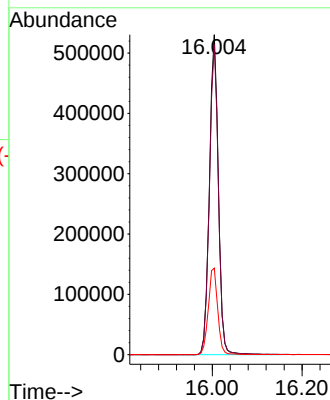

#45
2-Fluorobiphenyl
Concen: 65.594 ng
RT: 13.140 min Scan# 1709
Delta R.T. -0.012 min
Lab File: BP007194.D
Acq: 25 Sep 2021 19:33

Tgt Ion:172 Resp: 2369321
Ion Ratio Lower Upper
172 100
171 35.7 27.9 41.9
170 23.6 18.6 27.8


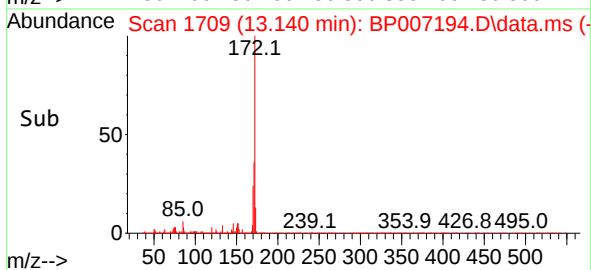
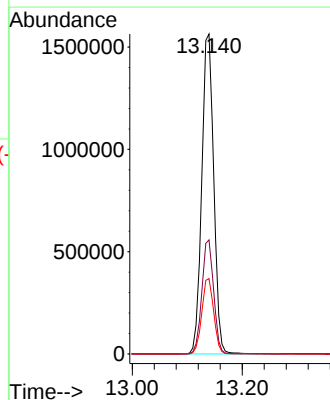
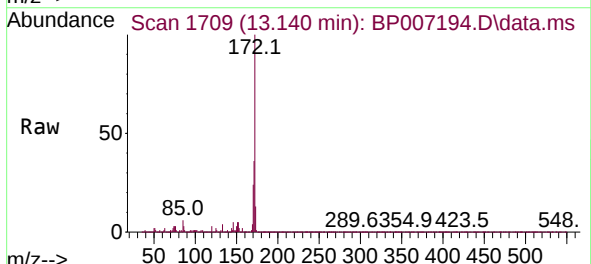




#64
Phenanthrene-d10
Concen: 20.000 ng
RT: 17.263 min Scan# 2410
Delta R.T. -0.012 min
Lab File: BP007194.D
Acq: 25 Sep 2021 19:33




Instrument :
BNA_P
ClientSampleId :


Tgt Ion:188 Resp: 1093926
Ion Ratio Lower Upper
188 100
94 8.3 5.6 8.4
80 8.9 6.3 9.5

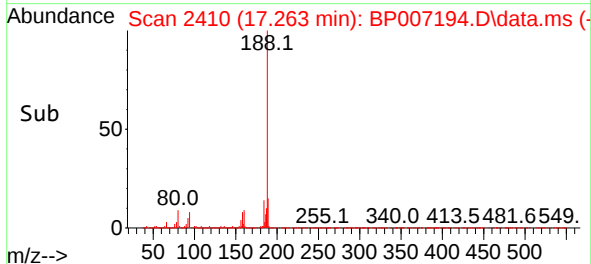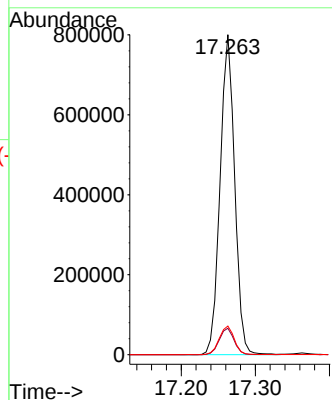

#76
Chrysene-d12
Concen: 20.000 ng
RT: 21.345 min Scan# 3104
Delta R.T. -0.012 min
Lab File: BP007194.D
Acq: 25 Sep 2021 19:33

Tgt Ion:240 Resp: 1088392
Ion Ratio Lower Upper
240 100
120 10.3 6.5 9.7#
236 26.0 20.6 31.0

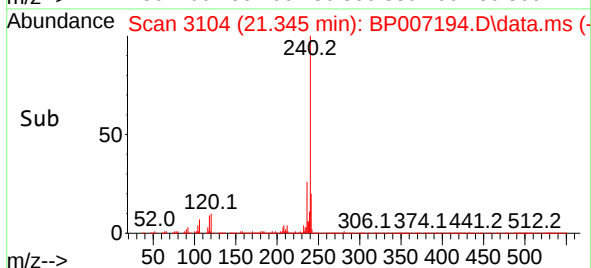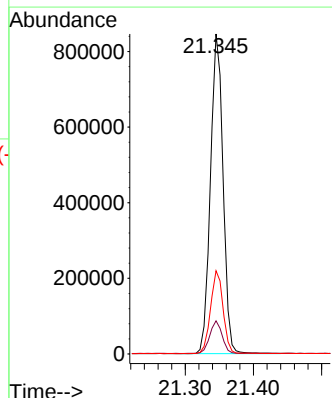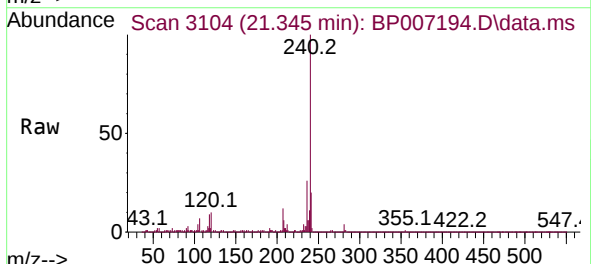







#79
 Terphenyl-d14
 Concen: 65.098 ng
 RT: 19.822 min Scan# 2845
 Delta R.T. -0.012 min
 Lab File: BP007194.D
 Acq: 25 Sep 2021 19:33

Instrument :
 BNA_P
 ClientSampleId :

Tgt Ion:244 Resp: 3697403

Ion	Ratio	Lower	Upper
244	100		
212	7.0	6.0	9.0
122	8.8	7.1	10.7

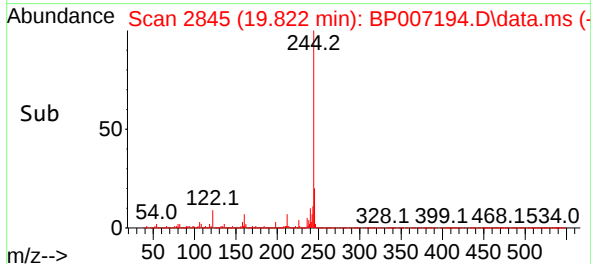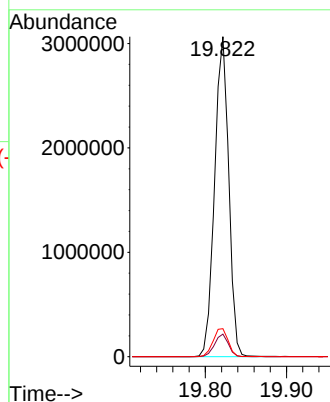

#86
 Perylene-d12
 Concen: 20.000 ng
 RT: 23.751 min Scan# 3513
 Delta R.T. -0.018 min
 Lab File: BP007194.D
 Acq: 25 Sep 2021 19:33

Tgt Ion:264 Resp: 1179523

Ion	Ratio	Lower	Upper
264	100		
260	23.8	18.6	28.0
265	22.6	17.6	26.4

