

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP092521\
 Data File : BP007195.D
 Acq On : 25 Sep 2021 20:07
 Operator : CG/JU
 Sample : M3908-06
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SUB-SLAB-06-(6-2.6)

Quant Time: Sep 26 02:16:17 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP092121.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Sep 23 11:17:25 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.881	152	207476	20.00	ng	-0.01
21) Naphthalene-d8	10.681	136	827789	20.00	ng	#-0.01
39) Acenaphthene-d10	14.510	164	526001	20.00	ng	-0.02
64) Phenanthrene-d10	17.263	188	1118096	20.00	ng	-0.01
76) Chrysene-d12	21.345	240	1110766	20.00	ng	#-0.01
86) Perylene-d12	23.751	264	1216276	20.00	ng	-0.02
System Monitoring Compounds						
5) 2-Fluorophenol	5.458	112	1262522	101.86	ng	0.00
7) Phenol-d6	7.052	99	1607823	94.91	ng	-0.01
23) Nitrobenzene-d5	9.040	82	951692	66.95	ng	-0.02
42) 2,4,6-Tribromophenol	16.004	330	793212	116.32	ng	-0.01
45) 2-Fluorobiphenyl	13.140	172	2414228	65.75	ng	-0.01
79) Terphenyl-d14	19.822	244	3646947	62.92	ng	-0.01


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP092521\
Data File : BP007195.D
Acq On : 25 Sep 2021 20:07
Operator : CG/JU
Sample : M3908-06
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SUB-SLAB-06-(6-2.6)

Quant Time: Sep 26 02:16:17 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP092121.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Sep 23 11:17:25 2021
Response via : Initial Calibration




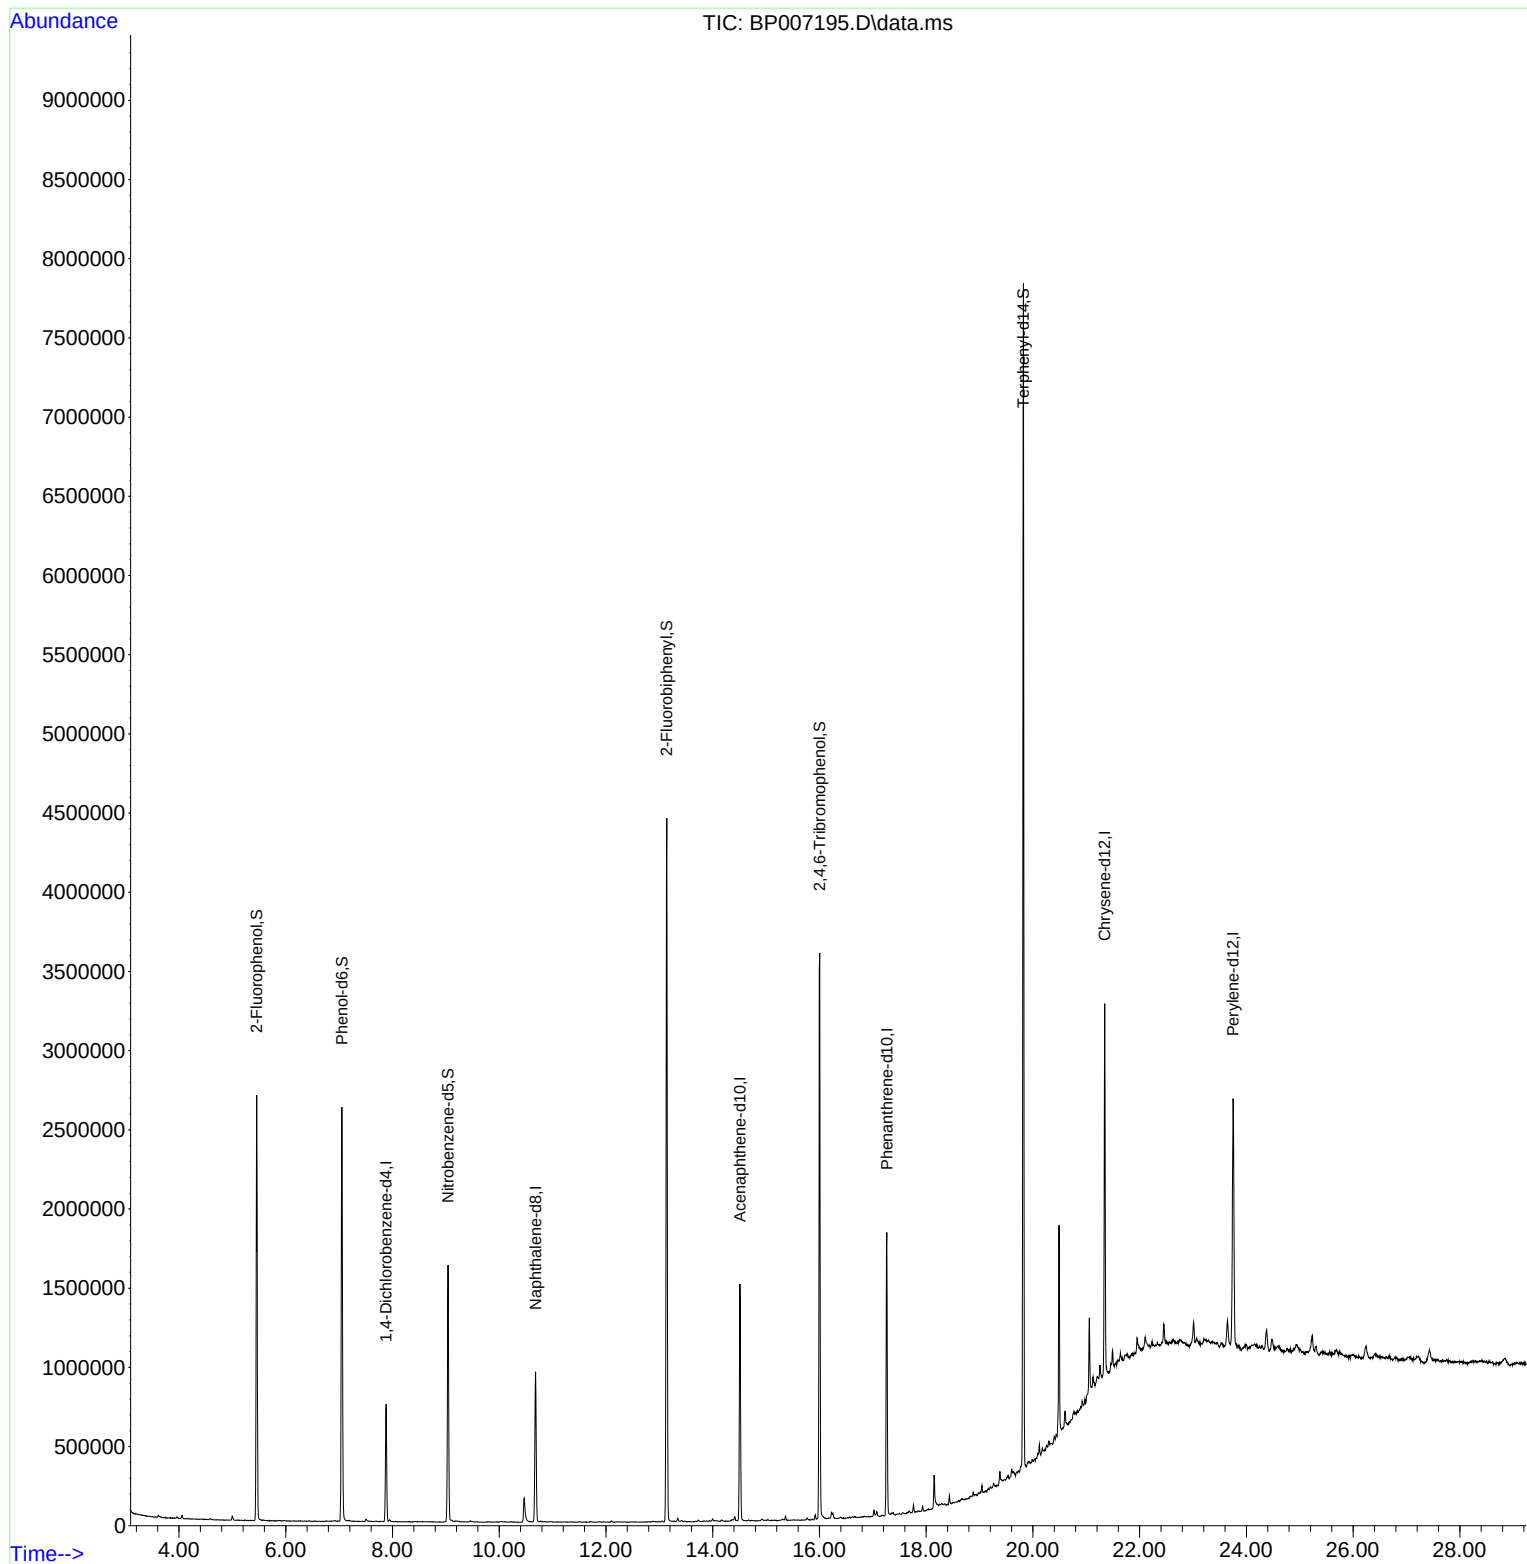




#1
1,4-Dichlorobenzene-d4
Concen: 20.00 ng
RT: 7.881 min Scan# 815
Delta R.T. -0.012 min
Lab File: BP007195.D
Acq: 25 Sep 2021 20:07




Instrument :
BNA_P
ClientSampleId :
SUB-SLAB-06-(6-2.6)


Tgt Ion:152 Resp: 207476
Ion Ratio Lower Upper
152 100
150 153.6 125.6 188.4
115 54.8 48.5 72.7

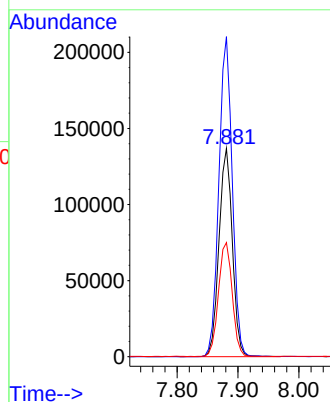

#5
2-Fluorophenol
Concen: 101.86 ng
RT: 5.458 min Scan# 403
Delta R.T. -0.006 min
Lab File: BP007195.D
Acq: 25 Sep 2021 20:07

Tgt Ion:112 Resp: 1262522
Ion Ratio Lower Upper
112 100
64 50.4 41.4 62.2
63 26.3 23.8 35.8


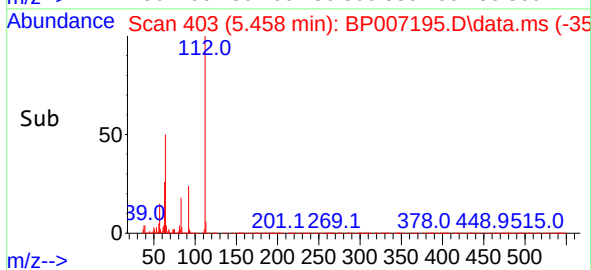
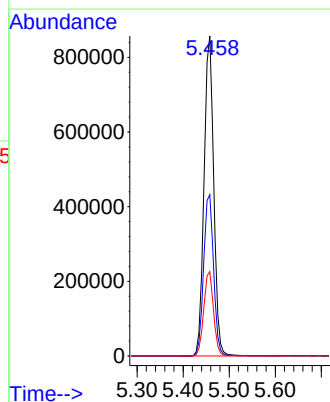





#7
Phenol-d6
Concen: 94.91 ng
RT: 7.052 min Scan# 674
Delta R.T. -0.012 min
Lab File: BP007195.D
Acq: 25 Sep 2021 20:07




Instrument :
BNA_P
ClientSampleId :
SUB-SLAB-06-(6-2.6)


Tgt Ion: 99 Resp: 1607823
Ion Ratio Lower Upper
99 100
42 13.5 13.4 20.0
71 31.1 30.6 46.0

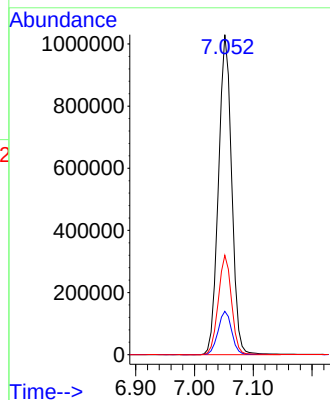

#21
Naphthalene-d8
Concen: 20.00 ng
RT: 10.681 min Scan# 1291
Delta R.T. -0.012 min
Lab File: BP007195.D
Acq: 25 Sep 2021 20:07

Tgt Ion: 136 Resp: 827789
Ion Ratio Lower Upper
136 100
137 10.8 8.6 12.8
54 6.9 4.6 6.8#
68 5.4 3.6 5.4


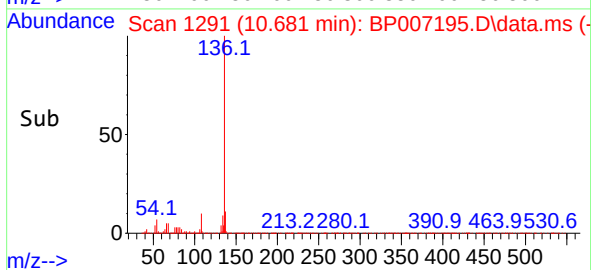
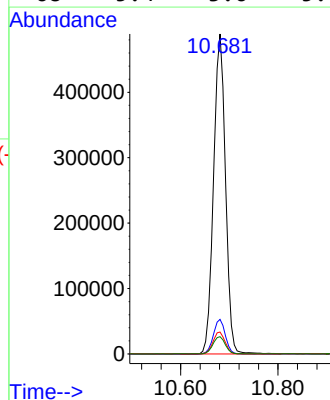



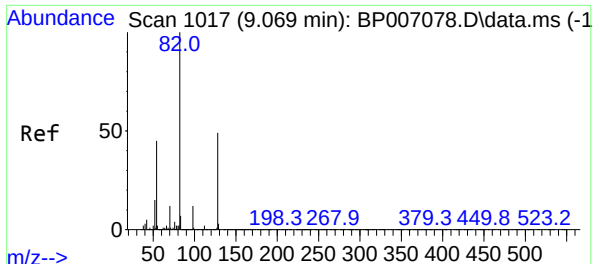

#23
Nitrobenzene-d5
Concen: 66.95 ng
RT: 9.040 min Scan# 1012
Delta R.T. -0.018 min
Lab File: BP007195.D
Acq: 25 Sep 2021 20:07




Instrument :
BNA_P
ClientSampleId :
SUB-SLAB-06-(6-2.6)


Tgt Ion: 82 Resp: 951692
Ion Ratio Lower Upper
82 100
128 47.2 35.7 53.5
54 44.3 35.0 52.4

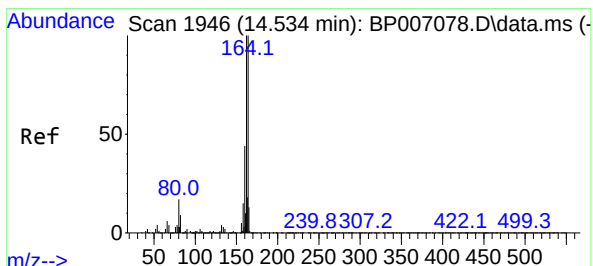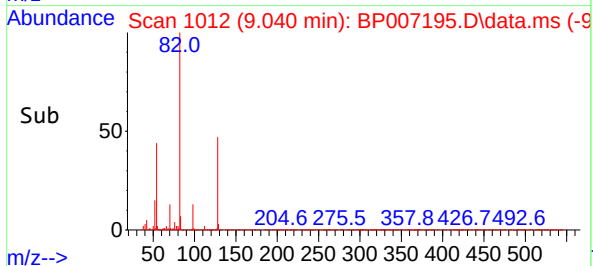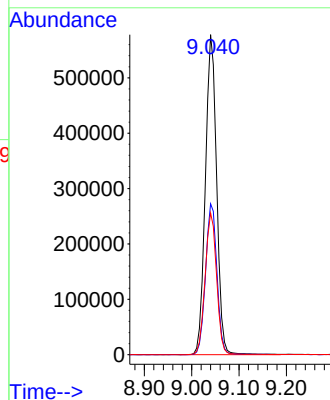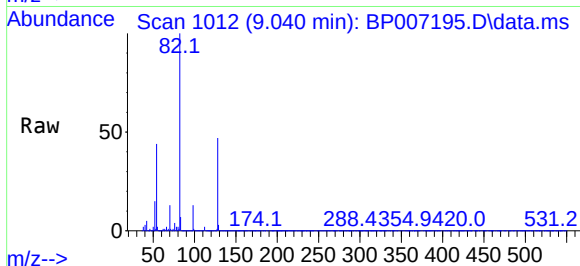

#39
Acenaphthene-d10
Concen: 20.00 ng
RT: 14.510 min Scan# 1942
Delta R.T. -0.018 min
Lab File: BP007195.D
Acq: 25 Sep 2021 20:07

Tgt Ion: 164 Resp: 526001
Ion Ratio Lower Upper
164 100
162 101.2 80.2 120.2
160 44.2 34.5 51.7


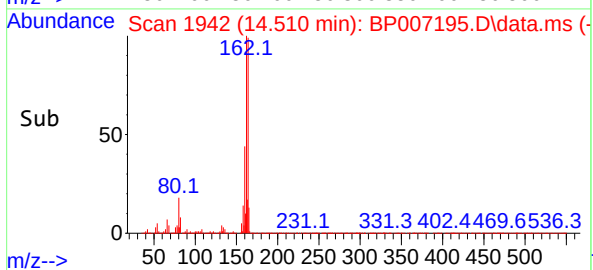
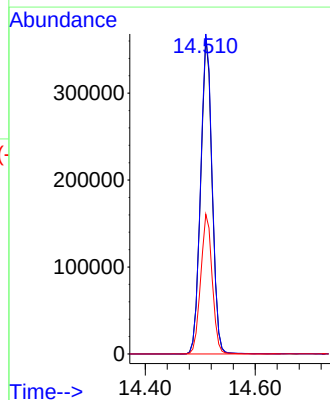
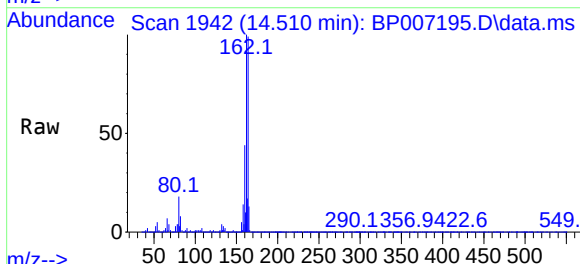




#42
2,4,6-Tribromophenol
Concen: 116.32 ng
RT: 16.004 min Scan# 2196
Delta R.T. -0.012 min
Lab File: BP007195.D
Acq: 25 Sep 2021 20:07




Instrument :
BNA_P
ClientSampleId :
SUB-SLAB-06-(6-2.6)


Tgt Ion:330 Resp: 793212
Ion Ratio Lower Upper
330 100
332 96.2 77.8 116.8
141 28.4 25.4 38.2

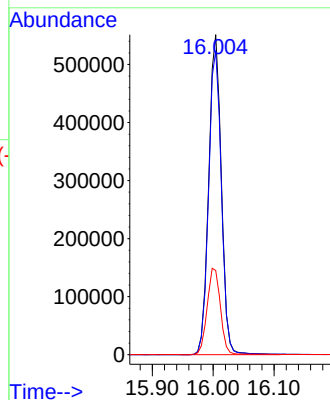

#45
2-Fluorobiphenyl
Concen: 65.75 ng
RT: 13.140 min Scan# 1709
Delta R.T. -0.012 min
Lab File: BP007195.D
Acq: 25 Sep 2021 20:07

Tgt Ion:172 Resp: 2414228
Ion Ratio Lower Upper
172 100
171 35.2 27.9 41.9
170 23.4 18.6 27.8


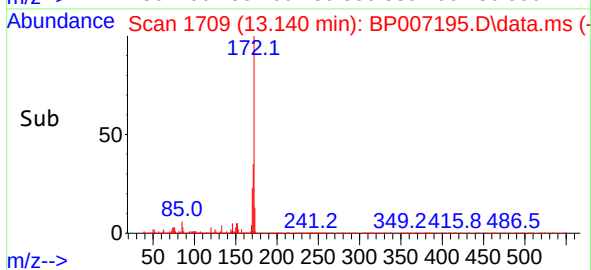
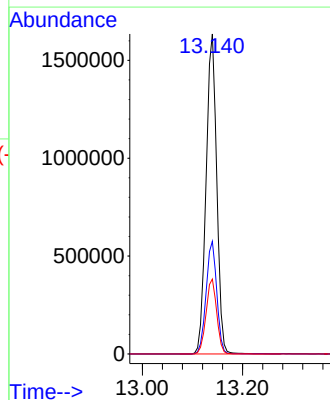





#64
Phenanthrene-d10
Concen: 20.00 ng
RT: 17.263 min Scan# 2410
Delta R.T. -0.012 min
Lab File: BP007195.D
Acq: 25 Sep 2021 20:07




Instrument :
BNA_P
ClientSampleId :
SUB-SLAB-06-(6-2.6)


Tgt Ion:188 Resp: 1118096
Ion Ratio Lower Upper
188 100
94 8.2 5.6 8.4
80 8.7 6.3 9.5

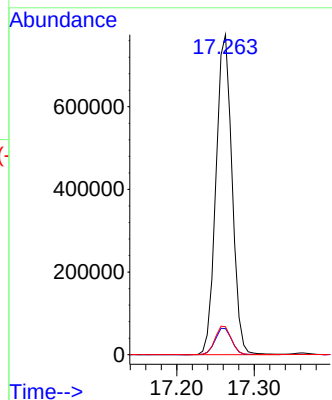

#76
Chrysene-d12
Concen: 20.00 ng
RT: 21.345 min Scan# 3104
Delta R.T. -0.012 min
Lab File: BP007195.D
Acq: 25 Sep 2021 20:07

Tgt Ion:240 Resp: 1110766
Ion Ratio Lower Upper
240 100
120 10.1 6.5 9.7#
236 25.9 20.6 31.0


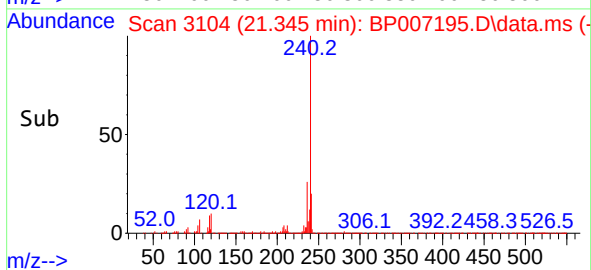
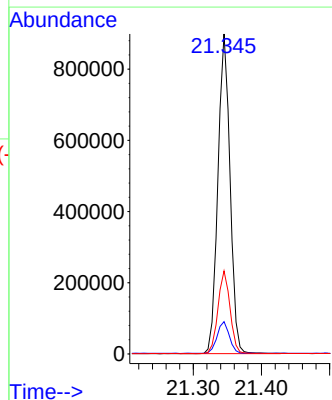





#79
Terphenyl-d14
Concen: 62.92 ng
RT: 19.822 min Scan# 2845
Delta R.T. -0.012 min
Lab File: BP007195.D
Acq: 25 Sep 2021 20:07

Instrument :
BNA_P
ClientSampleId :
SUB-SLAB-06-(6-2.6)

Tgt Ion:244 Resp: 3646947
Ion Ratio Lower Upper
244 100
212 7.1 6.0 9.0
122 8.8 7.1 10.7

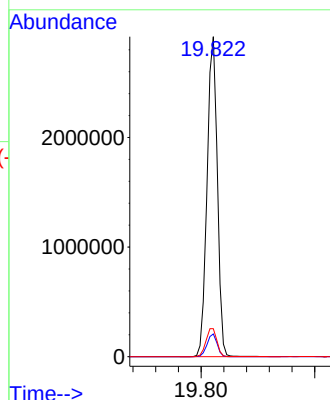

#86
Perylene-d12
Concen: 20.00 ng
RT: 23.751 min Scan# 3513
Delta R.T. -0.018 min
Lab File: BP007195.D
Acq: 25 Sep 2021 20:07

Tgt Ion:264 Resp: 1216276
Ion Ratio Lower Upper
264 100
260 23.9 18.6 28.0
265 22.3 17.6 26.4

