

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP092521\
 Data File : BP007190.D
 Acq On : 25 Sep 2021 17:17
 Operator : CG/JU
 Sample : M3927-21
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 WOOSPK-BACKFILL-05

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP092121.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BP007190.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.458	396	403	417	rBV	2658381	3975143	39.13%	7.873%
2	7.052	665	674	688	rBV	2582610	4164822	41.00%	8.249%
3	7.881	807	815	823	rBV	782478	1227226	12.08%	2.431%
4	9.040	1005	1012	1023	rBV	1549477	2633005	25.92%	5.215%
5	10.463	1248	1254	1269	rBV	414549	787652	7.75%	1.560%
6	10.681	1283	1291	1299	rBV	1085682	1811840	17.84%	3.589%
7	13.140	1701	1709	1720	rBV	4669359	6924048	68.16%	13.714%
8	14.510	1935	1942	1951	rBV	1726047	2524725	24.85%	5.001%
9	16.004	2189	2196	2212	rVB	3649282	5368021	52.85%	10.632%
10	17.263	2403	2410	2416	rBV	2080041	2975773	29.30%	5.894%
11	18.151	2556	2561	2570	rBV	254715	400369	3.94%	0.793%
12	19.622	2808	2811	2817	rVB	75514	103395	1.02%	0.205%
13	19.816	2839	2844	2850	rBV	7932121	10157848	100.00%	20.119%
14	21.057	3051	3055	3061	rBV	510104	716082	7.05%	1.418%
15	21.345	3099	3104	3109	rBV	2566802	3254471	32.04%	6.446%
16	23.751	3507	3513	3522	rVB2	1670934	3463901	34.10%	6.861%




Sum of corrected areas: 50488321

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP092521\
Data File : BP007190.D
Acq On : 25 Sep 2021 17:17
Operator : CG/JU
Sample : M3927-21
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
WOOSPK-BACKFILL-05

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP092121.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

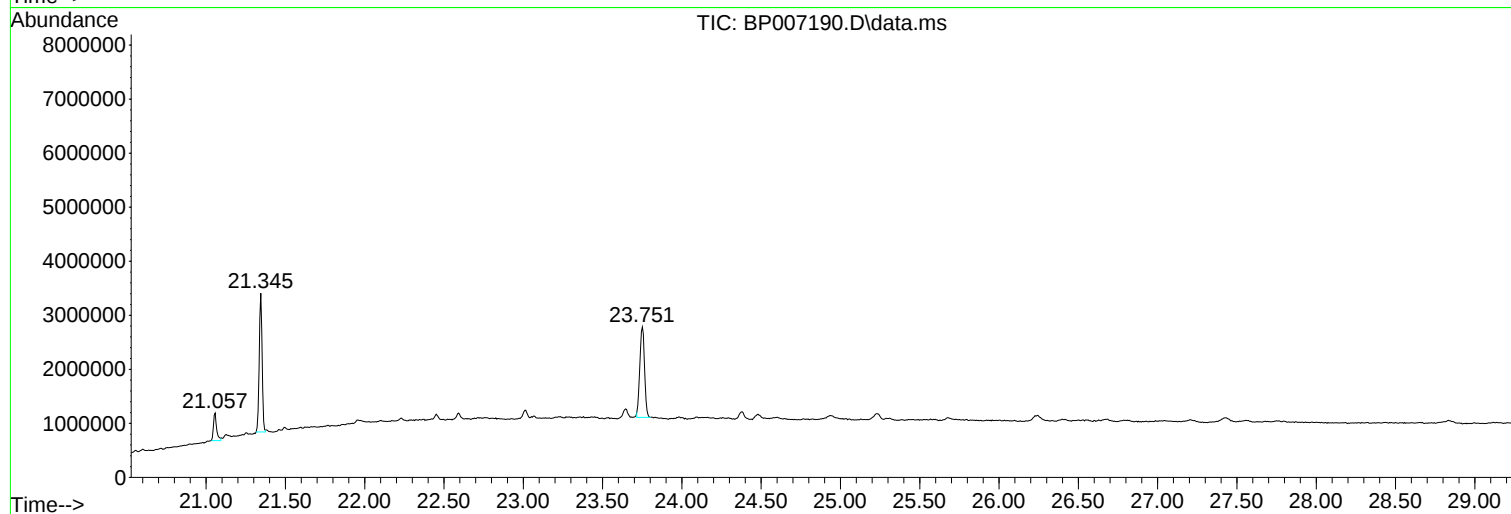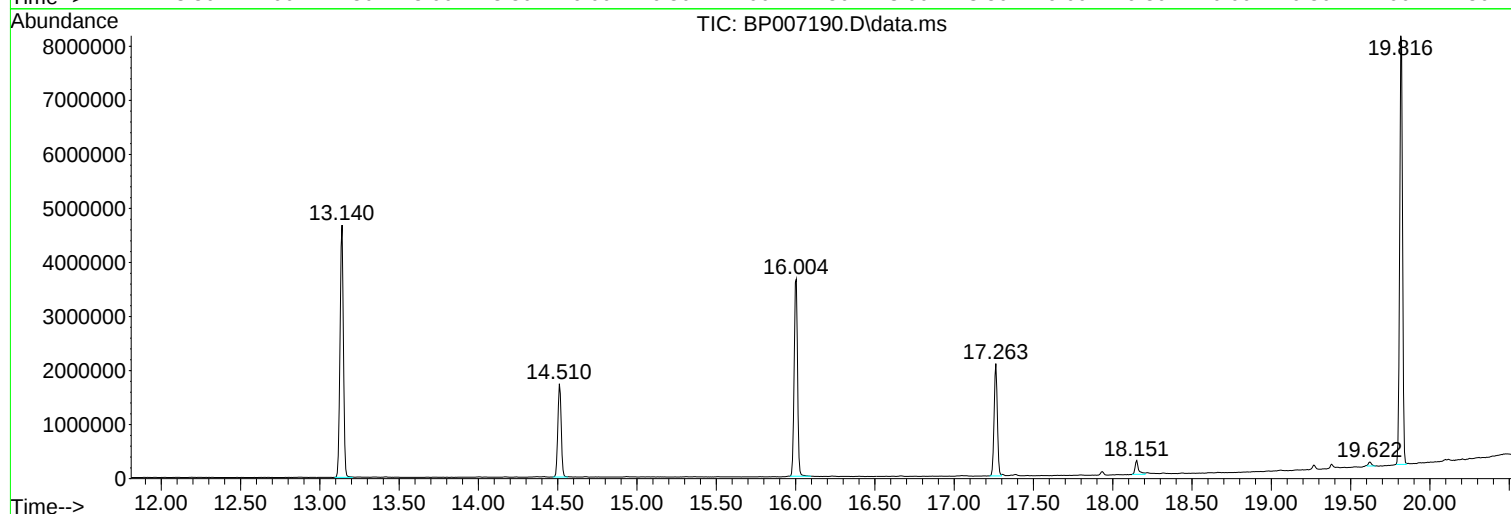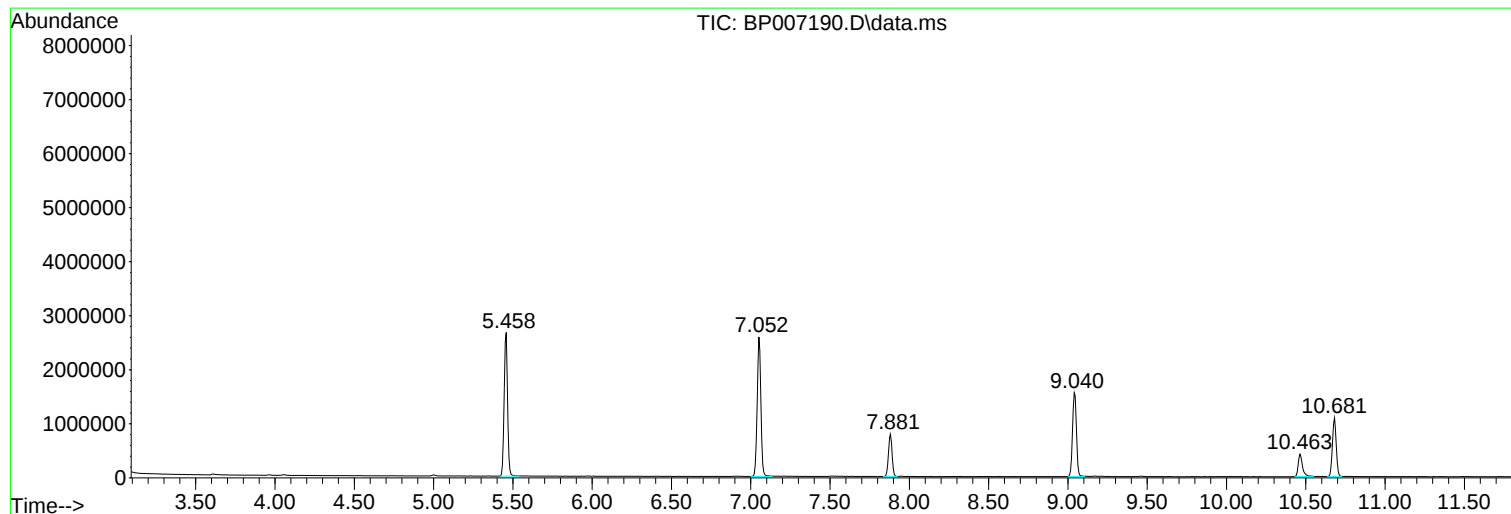

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP092521\
Data File : BP007190.D
Acq On : 25 Sep 2021 17:17
Operator : CG/JU
Sample : M3927-21
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
WOOSPK-BACKFILL-05

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP092121.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP092521\
Data File : BP007190.D
Acq On : 25 Sep 2021 17:17
Operator : CG/JU
Sample : M3927-21
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
WOOSPK-BACKFILL-05

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP092121.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------