

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP092521\
 Data File : BP007191.D
 Acq On : 25 Sep 2021 17:51
 Operator : CG/JU
 Sample : M3927-23
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 WOOSPK-BACKFILL-06

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP092121.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BP007191.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	4.993	319	324	333	rBV	91090	136895	1.43%	0.281%
2	5.458	396	403	414	rBV	2473388	3704074	38.79%	7.608%
3	7.052	667	674	693	rBV	2433775	3912333	40.97%	8.035%
4	7.881	806	815	822	rBV	778668	1215457	12.73%	2.496%
5	9.040	1004	1012	1025	rBV	1500394	2527966	26.47%	5.192%
6	10.463	1248	1254	1274	rBV	272635	572870	6.00%	1.177%
7	10.681	1283	1291	1305	rBV	1037426	1747279	18.30%	3.589%
8	13.140	1701	1709	1724	rBV	4416258	6562231	68.72%	13.478%
9	13.416	1750	1756	1762	rBV	199665	307552	3.22%	0.632%
10	14.510	1934	1942	1959	rBV	1650182	2416288	25.30%	4.963%
11	15.998	2189	2195	2216	rVB	3386369	5013121	52.50%	10.296%
12	17.263	2403	2410	2420	rBV	2006271	2853774	29.89%	5.861%
13	17.934	2520	2524	2531	rVB2	98077	124679	1.31%	0.256%
14	18.145	2556	2560	2568	rBV	170884	277002	2.90%	0.569%
15	19.063	2712	2716	2721	rVB2	209563	241220	2.53%	0.495%
16	19.192	2735	2738	2742	rVB	93567	102018	1.07%	0.210%
17	19.816	2839	2844	2850	rBV	7514152	9548837	100.00%	19.612%
18	20.122	2893	2896	2899	rVB	115987	121300	1.27%	0.249%
19	20.604	2975	2978	2981	rVB2	116828	117541	1.23%	0.241%
20	21.057	3051	3055	3059	rBV	596465	789951	8.27%	1.622%
21	21.345	3099	3104	3109	rBV	2437885	3059481	32.04%	6.284%
22	23.751	3507	3513	3522	rVB	1651346	3337672	34.95%	6.855%




Sum of corrected areas: 48689541

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP092521\
Data File : BP007191.D
Acq On : 25 Sep 2021 17:51
Operator : CG/JU
Sample : M3927-23
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
WOOSPK-BACKFILL-06

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP092121.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

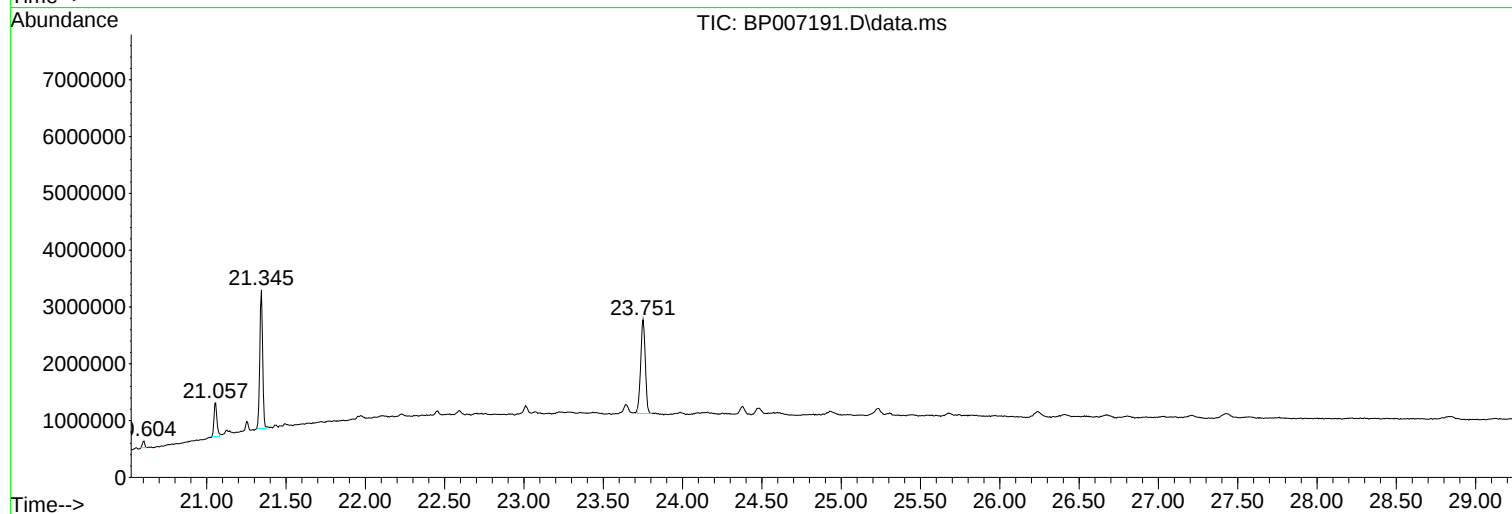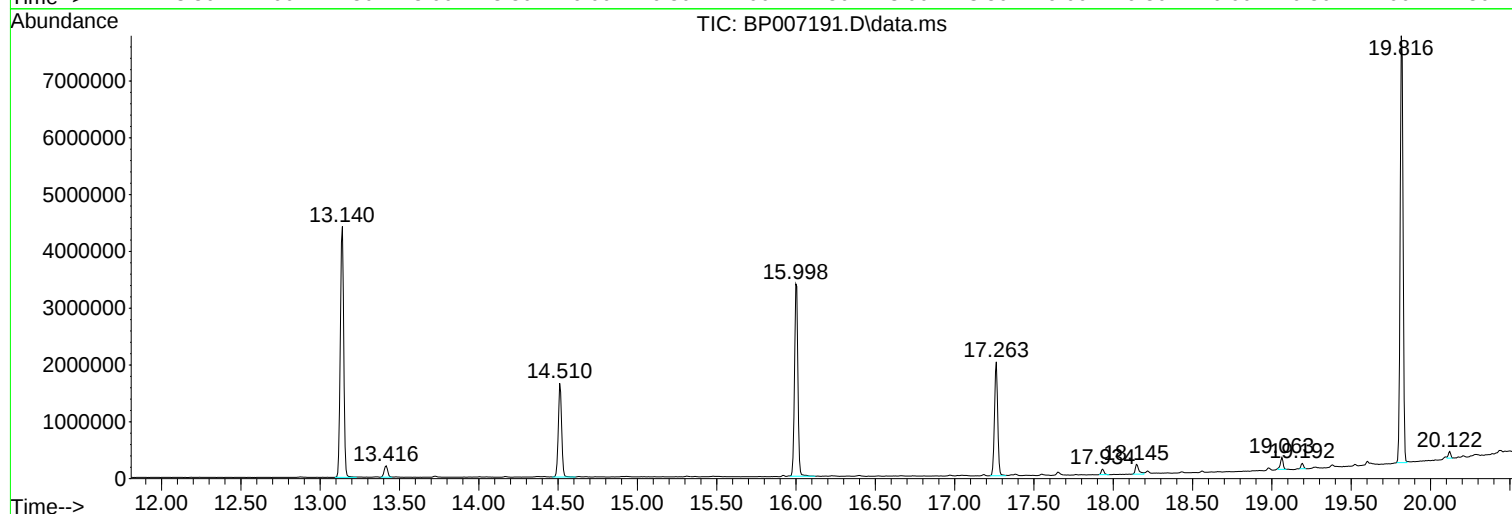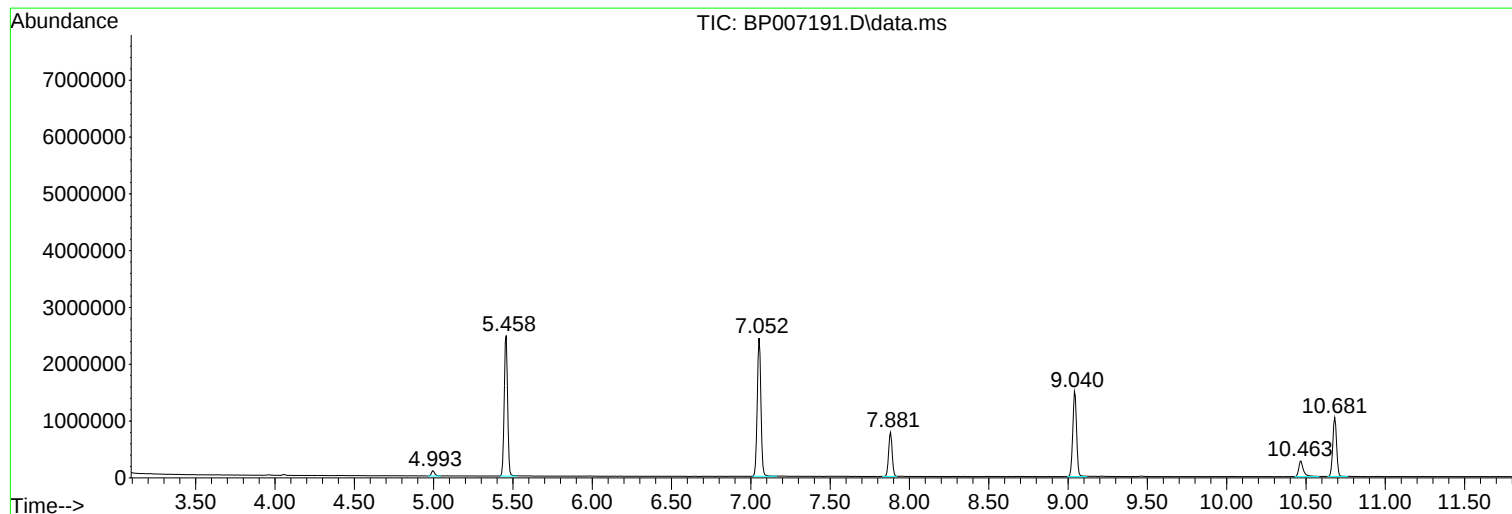

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP092521\
Data File : BP007191.D
Acq On : 25 Sep 2021 17:51
Operator : CG/JU
Sample : M3927-23
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
WOOSPK-BACKFILL-06

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP092121.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP092521\
Data File : BP007191.D
Acq On : 25 Sep 2021 17:51
Operator : CG/JU
Sample : M3927-23
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
WOOSPK-BACKFILL-06

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP092121.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------