

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP092521\
 Data File : BP007192.D
 Acq On : 25 Sep 2021 18:25
 Operator : CG/JU
 Sample : M3927-13
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 WOOSPK-BACKFILL-01

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP092121.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BP007192.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.458	396	403	416	rBV	2202695	3281136	38.81%	7.093%
2	7.052	666	674	694	rBV	2081095	3394382	40.15%	7.338%
3	7.881	807	815	823	rBV	897584	1412240	16.71%	3.053%
4	9.040	1004	1012	1026	rBV	1286439	2141309	25.33%	4.629%
5	10.463	1247	1254	1272	rBV	349587	721595	8.54%	1.560%
6	10.681	1283	1291	1304	rVB	1181474	1996230	23.61%	4.315%
7	13.140	1701	1709	1723	rBV	3683626	5552407	65.68%	12.003%
8	14.510	1931	1942	1956	rBV	1885930	2799681	33.12%	6.052%
9	15.998	2189	2195	2217	rVB	2961924	4335156	51.28%	9.372%
10	17.263	2403	2410	2423	rBV	2301479	3396382	40.18%	7.342%
11	18.151	2556	2561	2569	rBV	114792	204791	2.42%	0.443%
12	19.816	2839	2844	2850	rBV	6643587	8453411	100.00%	18.274%
13	21.057	3051	3055	3062	rBV	557026	765920	9.06%	1.656%
14	21.345	3099	3104	3110	rBV	2951693	3764472	44.53%	8.138%
15	23.751	3507	3513	3522	rVB2	1986015	4039482	47.79%	8.732%




Sum of corrected areas: 46258594

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP092521\
Data File : BP007192.D
Acq On : 25 Sep 2021 18:25
Operator : CG/JU
Sample : M3927-13
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
WOOSPK-BACKFILL-01

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP092121.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

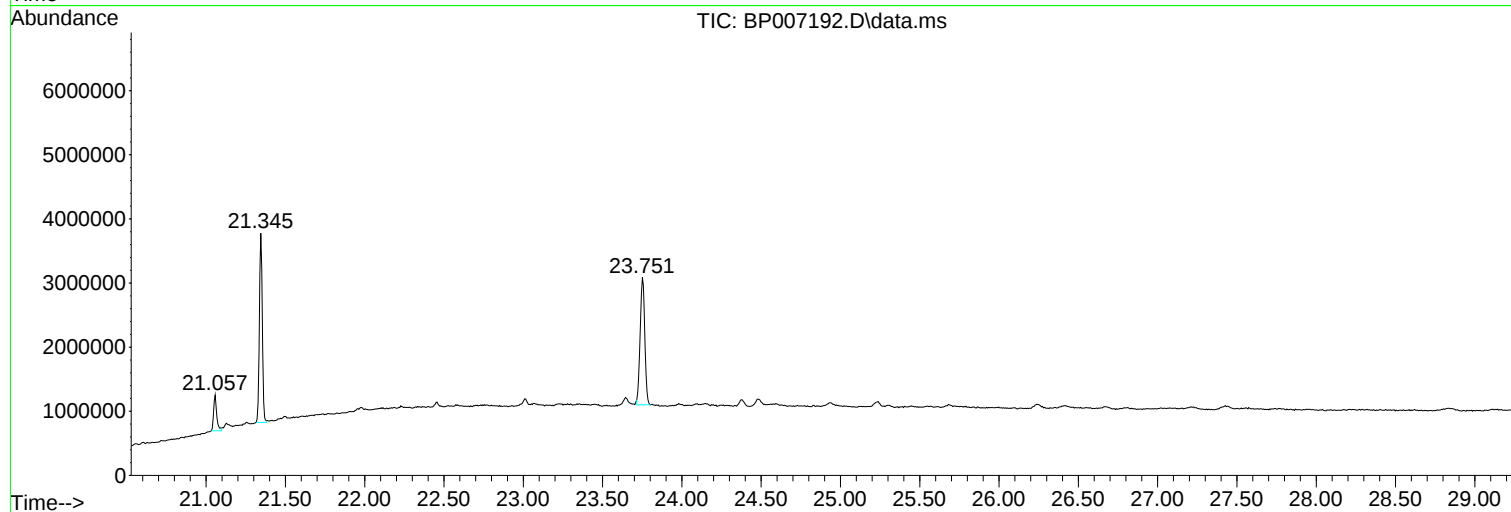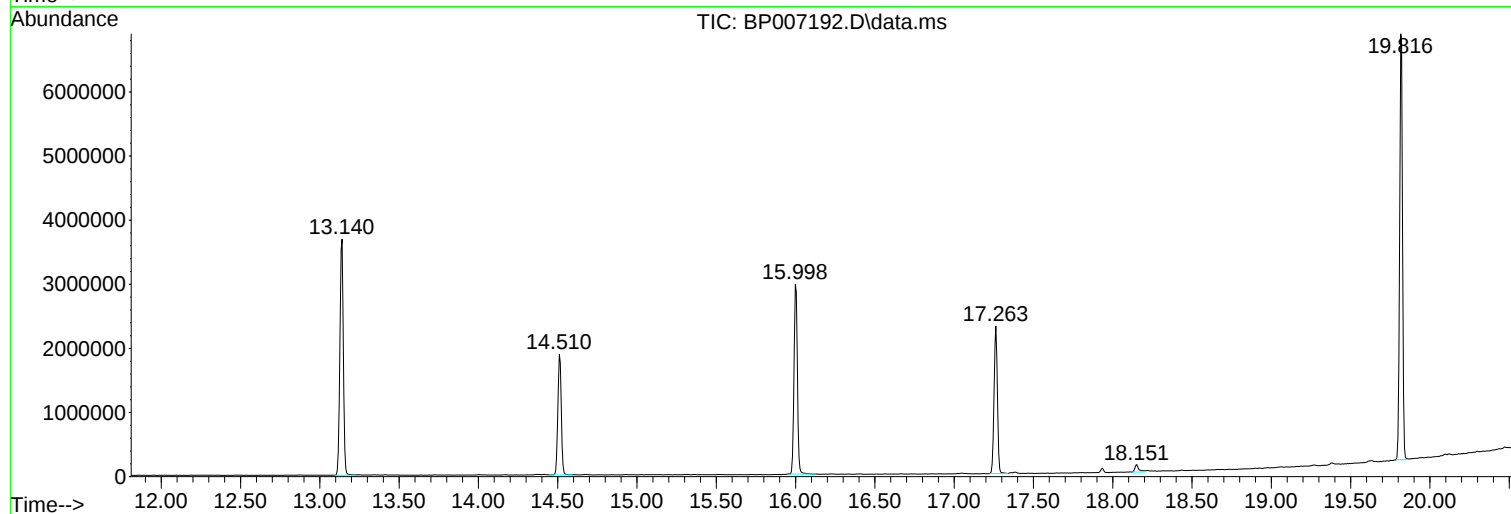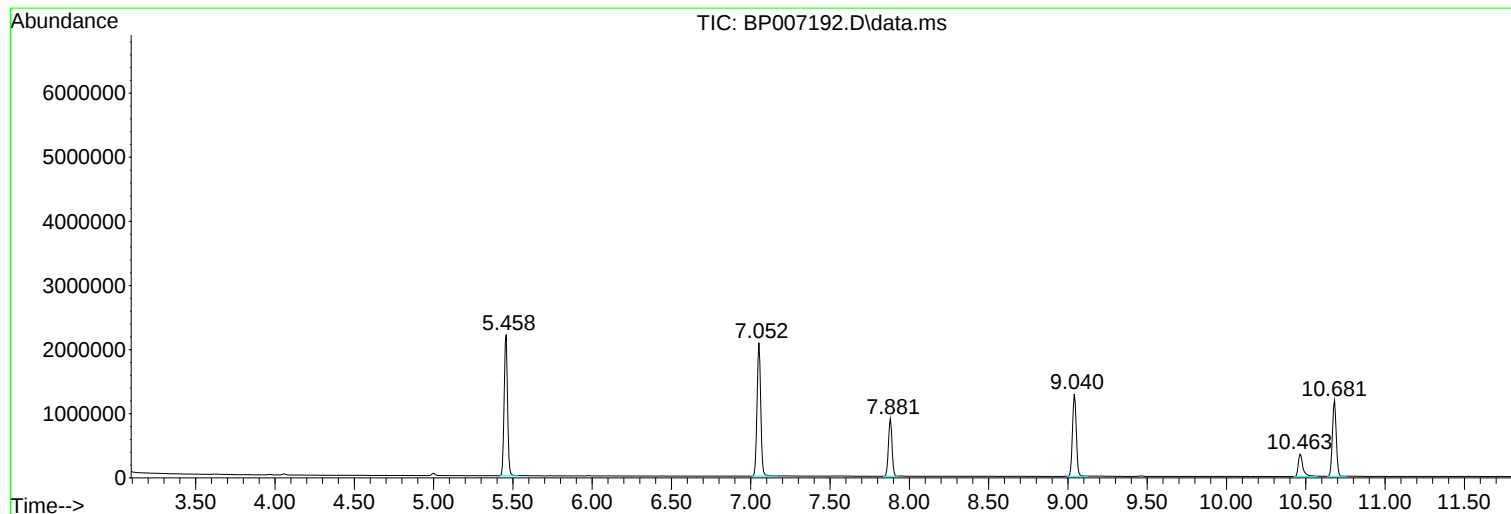

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP092521\
Data File : BP007192.D
Acq On : 25 Sep 2021 18:25
Operator : CG/JU
Sample : M3927-13
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
WOOSPK-BACKFILL-01

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP092121.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP092521\
Data File : BP007192.D
Acq On : 25 Sep 2021 18:25
Operator : CG/JU
Sample : M3927-13
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
WOOSPK-BACKFILL-01

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP092121.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------