

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP092521\
 Data File : BP007193.D
 Acq On : 25 Sep 2021 18:59
 Operator : CG/JU
 Sample : M3927-15
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 WOOSPK-BACKFILL-02

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP092121.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BP007193.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.458	396	403	416	rBV	2928212	4379251	40.67%	7.936%
2	7.052	666	674	690	rBV	2835862	4516132	41.94%	8.184%
3	7.881	808	815	823	rBV	908329	1431877	13.30%	2.595%
4	9.040	1004	1012	1024	rBV	1725499	2916184	27.08%	5.285%
5	10.463	1245	1254	1270	rBV	548241	1060703	9.85%	1.922%
6	10.681	1283	1291	1301	rBV	1202418	2026625	18.82%	3.673%
7	13.140	1699	1709	1723	rBV	4968092	7356051	68.32%	13.331%
8	14.510	1935	1942	1954	rBV	1871242	2752468	25.56%	4.988%
9	16.004	2189	2196	2213	rVB	3913108	5626475	52.25%	10.197%
10	17.263	2403	2410	2421	rBV	2298991	3262852	30.30%	5.913%
11	17.933	2520	2524	2529	rVB	95533	111962	1.04%	0.203%
12	18.151	2556	2561	2567	rBV	139765	217175	2.02%	0.394%
13	19.816	2839	2844	2850	rBV	8375324	10767827	100.00%	19.514%
14	21.057	3051	3055	3063	rBV	709322	948540	8.81%	1.719%
15	21.345	3099	3104	3112	rBV	2944050	3648945	33.89%	6.613%
16	23.751	3507	3513	3522	rVB2	2005941	4156604	38.60%	7.533%




Sum of corrected areas: 55179671

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP092521\
Data File : BP007193.D
Acq On : 25 Sep 2021 18:59
Operator : CG/JU
Sample : M3927-15
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
WOOSPK-BACKFILL-02

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP092121.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

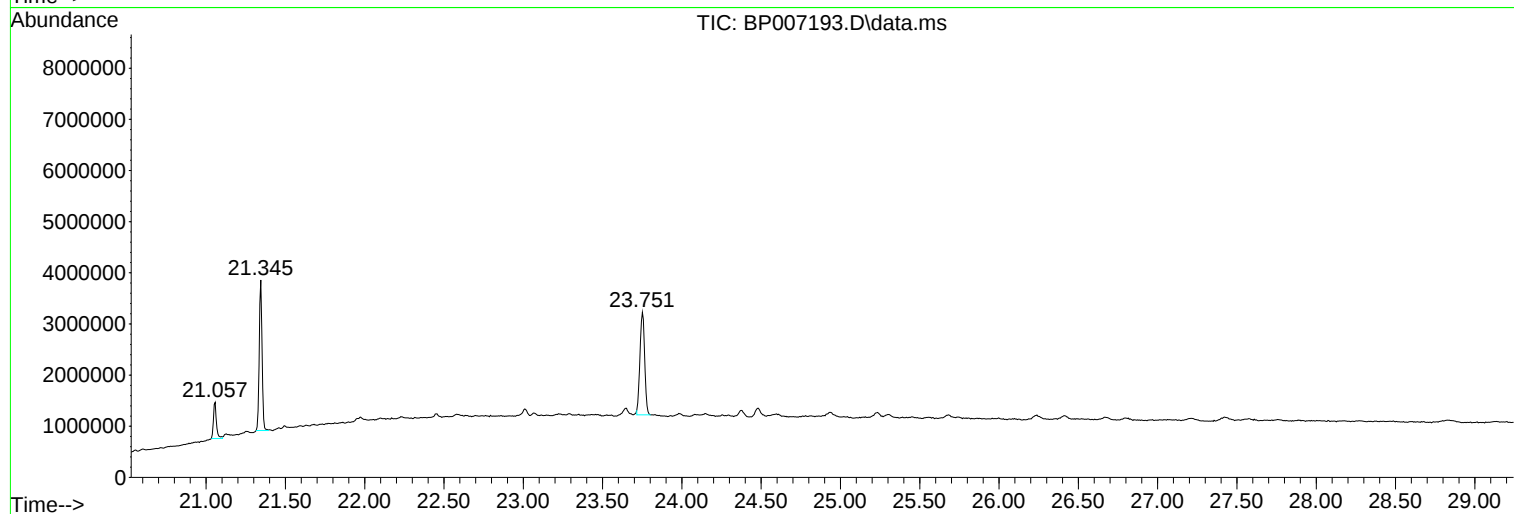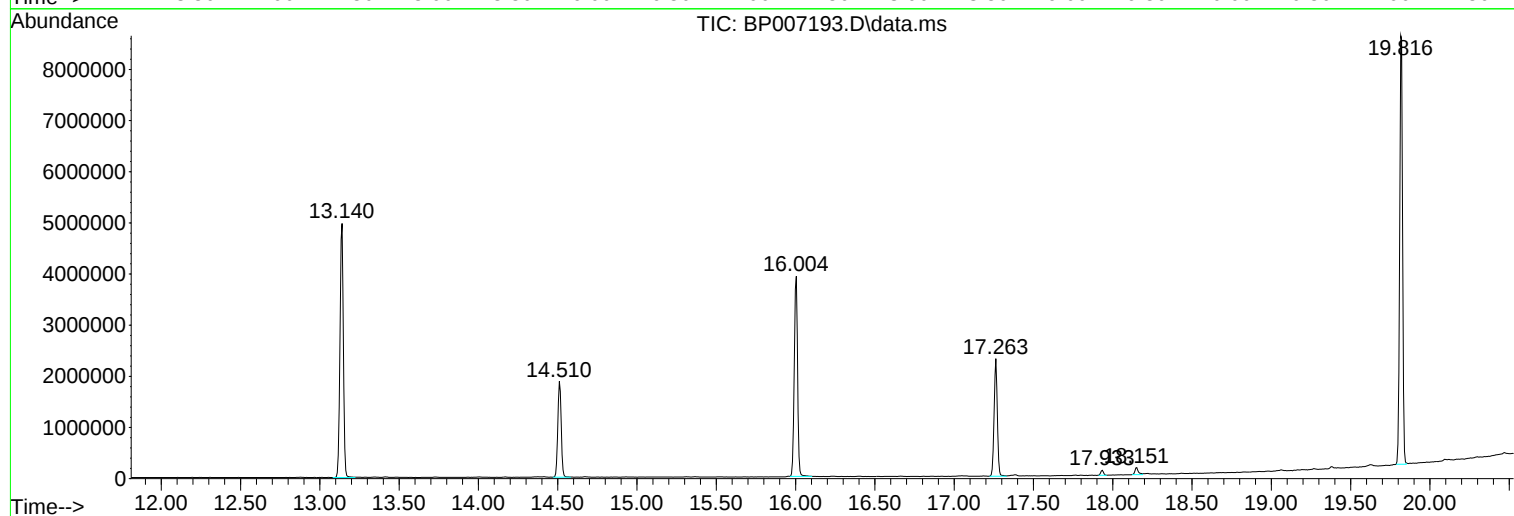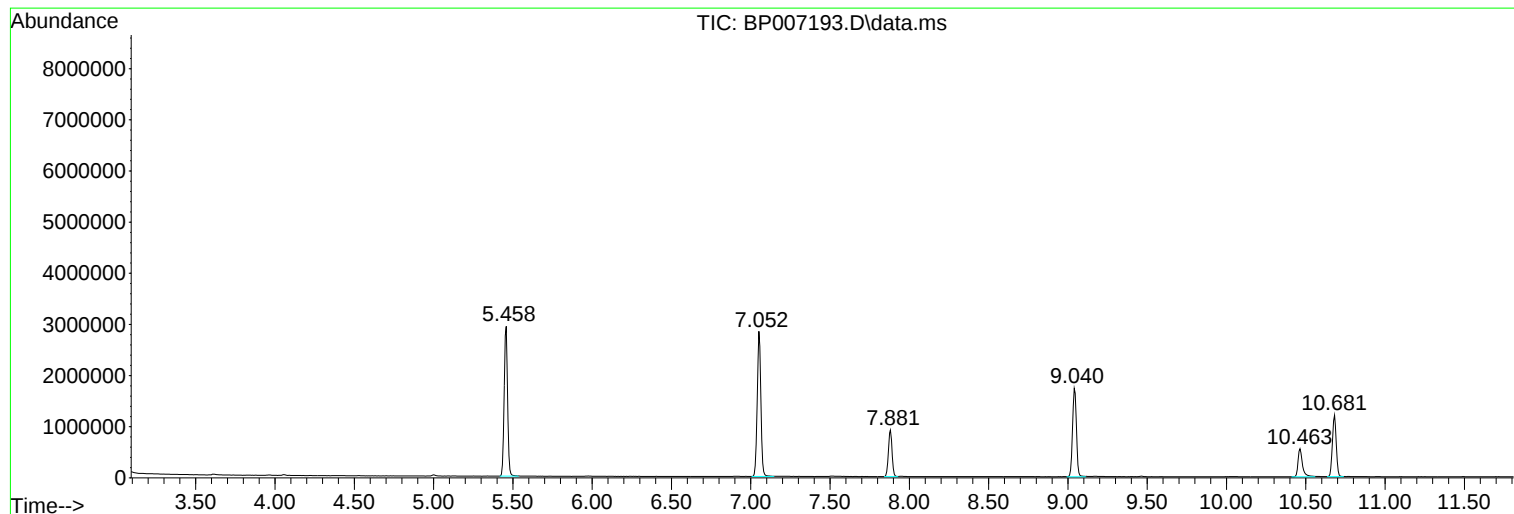

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP092521\
Data File : BP007193.D
Acq On : 25 Sep 2021 18:59
Operator : CG/JU
Sample : M3927-15
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
WOOSPK-BACKFILL-02

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP092121.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP092521\
Data File : BP007193.D
Acq On : 25 Sep 2021 18:59
Operator : CG/JU
Sample : M3927-15
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
WOOSPK-BACKFILL-02

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP092121.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------