

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP092521\
 Data File : BP007194.D
 Acq On : 25 Sep 2021 19:33
 Operator : CG/JU
 Sample : M3927-17
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 WOOSPK-BACKFILL-03

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP092121.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BP007194.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.452	396	402	417	rBV	2645068	3977218	41.62%	8.510%
2	7.052	666	674	691	rBV	2542541	4078159	42.67%	8.726%
3	7.881	808	815	822	rBV	706345	1105734	11.57%	2.366%
4	9.040	1004	1012	1026	rBV	1547681	2590629	27.11%	5.543%
5	10.463	1247	1254	1270	rBV	544420	1028800	10.76%	2.201%
6	10.681	1282	1291	1299	rBV	938057	1590350	16.64%	3.403%
7	13.140	1701	1709	1722	rBV	4268494	6508559	68.10%	13.926%
8	14.510	1935	1942	1955	rVB	1430676	2152516	22.52%	4.606%
9	16.004	2189	2196	2214	rVB	3486591	4995328	52.27%	10.688%
10	17.263	2403	2410	2421	rBV	1849870	2567662	26.87%	5.494%
11	17.933	2520	2524	2530	rBV	90981	111495	1.17%	0.239%
12	18.151	2556	2561	2569	rBV	106872	185097	1.94%	0.396%
13	19.822	2839	2845	2850	rBV	7841814	9556973	100.00%	20.448%
14	21.057	3052	3055	3062	rBV2	385697	503638	5.27%	1.078%
15	21.345	3100	3104	3109	rVB	2177011	2738500	28.65%	5.859%
16	23.751	3508	3513	3522	rVB2	1526496	3047254	31.89%	6.520%




Sum of corrected areas: 46737912

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP092521\
Data File : BP007194.D
Acq On : 25 Sep 2021 19:33
Operator : CG/JU
Sample : M3927-17
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
WOOSPK-BACKFILL-03

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP092121.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

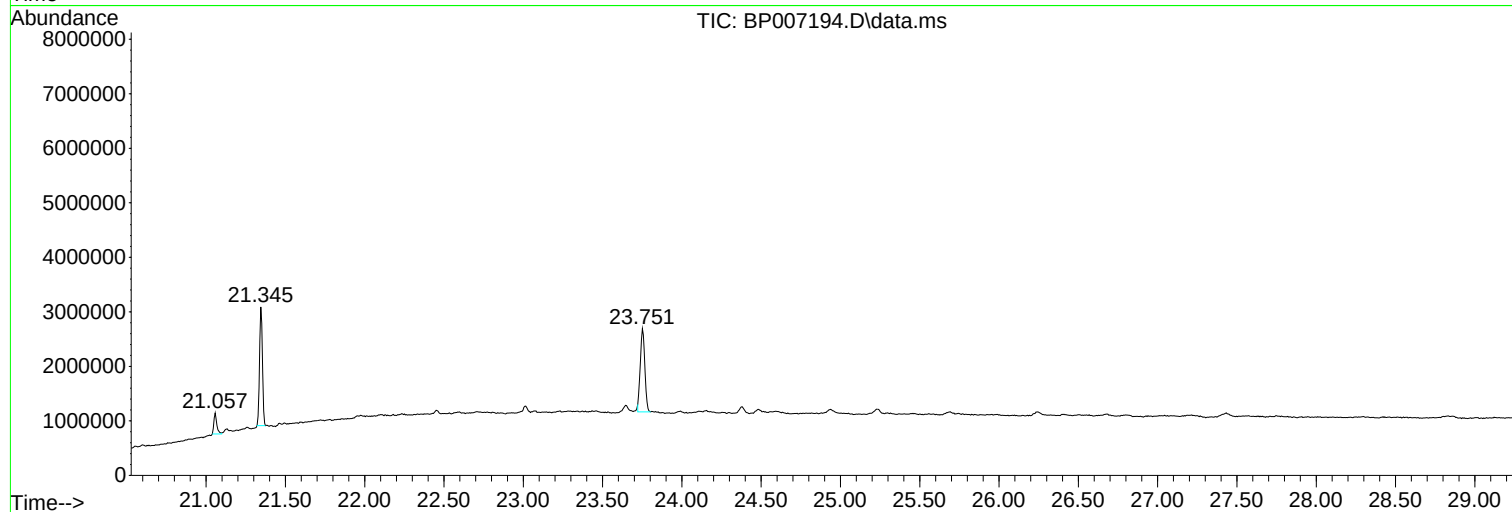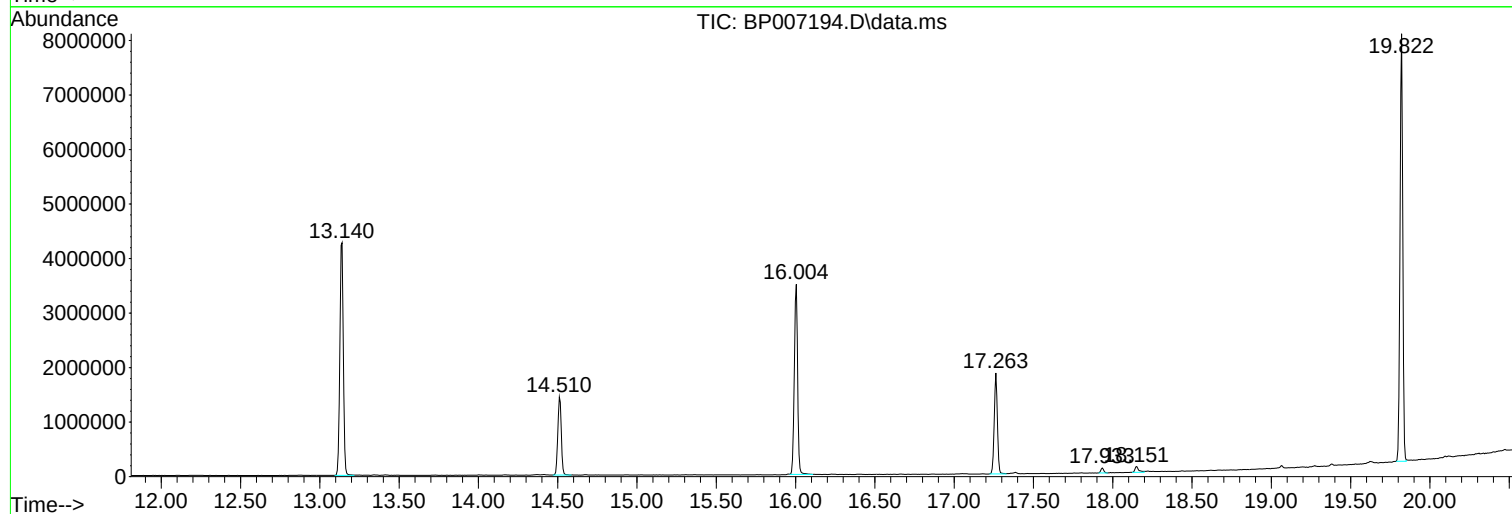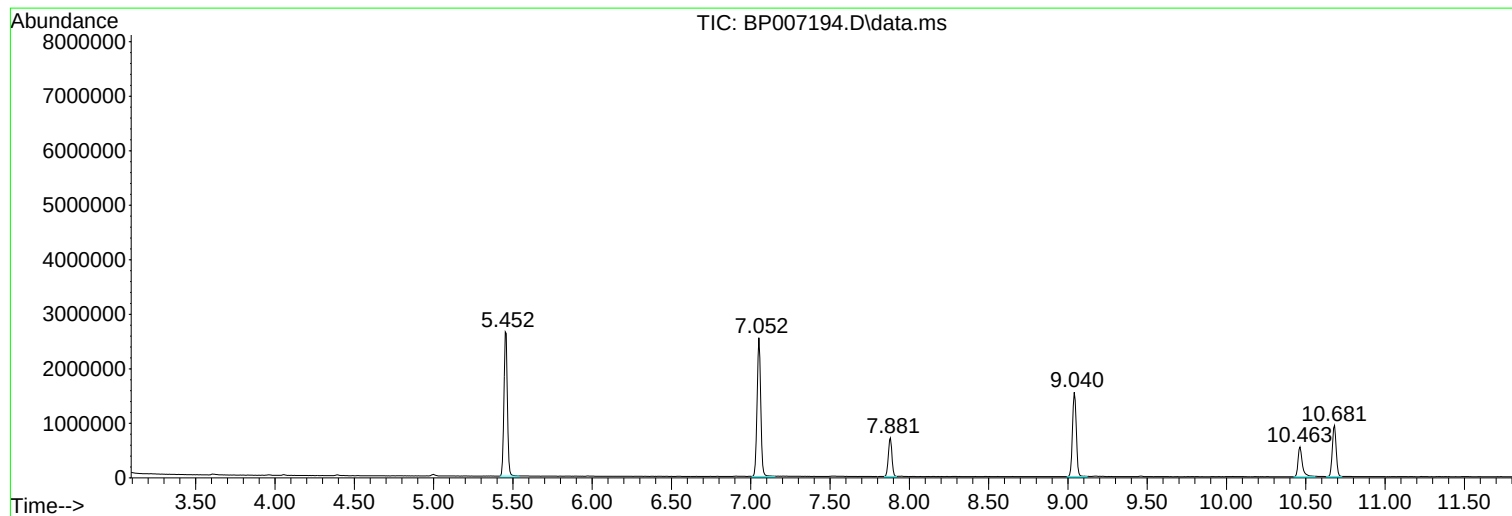

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP092521\
Data File : BP007194.D
Acq On : 25 Sep 2021 19:33
Operator : CG/JU
Sample : M3927-17
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
WOOSPK-BACKFILL-03

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP092121.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP092521\
Data File : BP007194.D
Acq On : 25 Sep 2021 19:33
Operator : CG/JU
Sample : M3927-17
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
WOOSPK-BACKFILL-03

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP092121.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
