
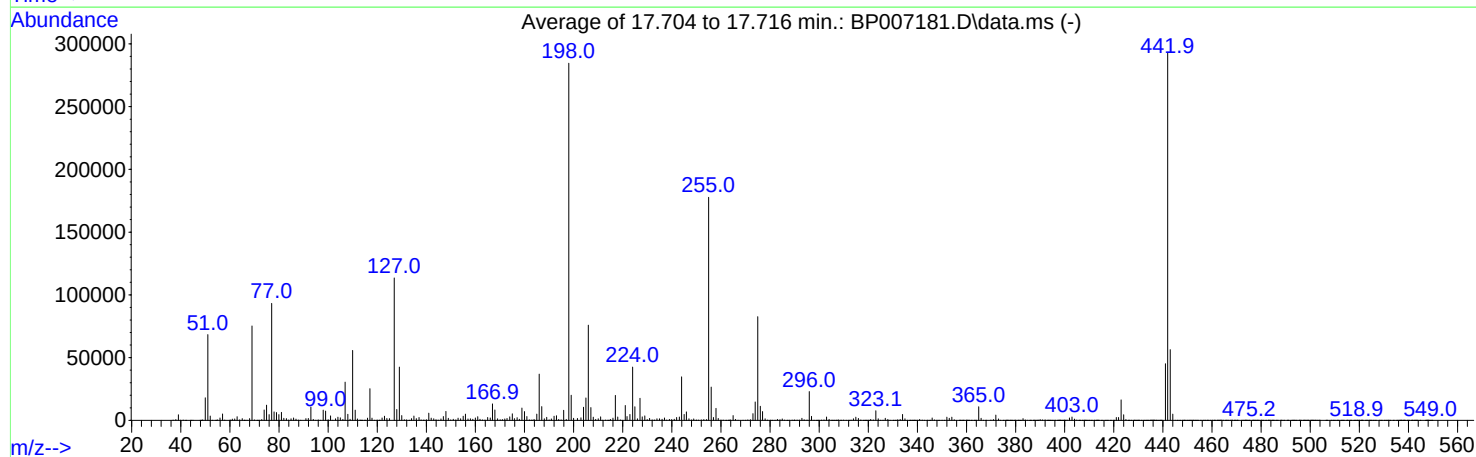


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP092521\
 Data File : BP007181.D
 Acq On : 25 Sep 2021 11:53
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP092121.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Sep 23 11:17:25 2021

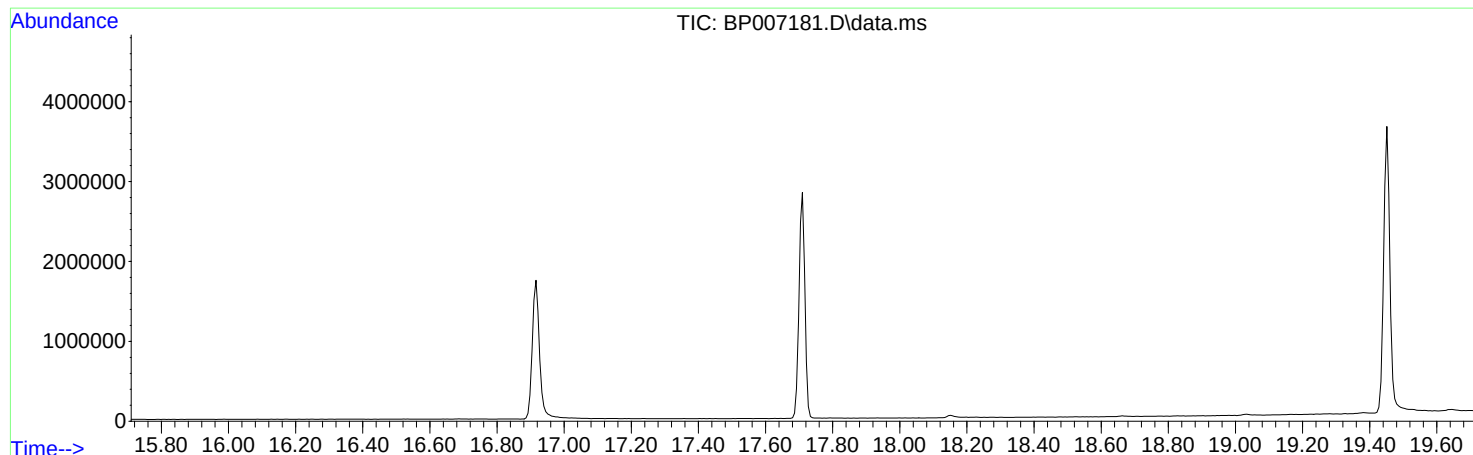




AutoFind: Scans 2485, 2486, 2487; Background Corrected with Scan 2475

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	24.0	68371	PASS
68	69	0.00	2	1.9	1417	PASS
69	198	0.00	100	26.5	75268	PASS
70	69	0.00	2	0.5	413	PASS
127	198	10	80	39.9	113430	PASS
197	198	0.00	2	0.3	804	PASS
198	198	100	100	100.0	284544	PASS
199	198	5	9	7.0	20007	PASS
275	198	10	60	29.0	82587	PASS
365	198	1	100	3.8	10903	PASS
441	198	0.01	100	15.9	45181	PASS
442	442	100	100	100.0	293124	PASS
443	442	15	24	19.2	56406	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP092521\
Data File : BP007181.D
Acq On : 25 Sep 2021 11:53
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: Sep 26 06:27:06 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP092121.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Sep 23 11:17:25 2021
Response via : Initial Calibration

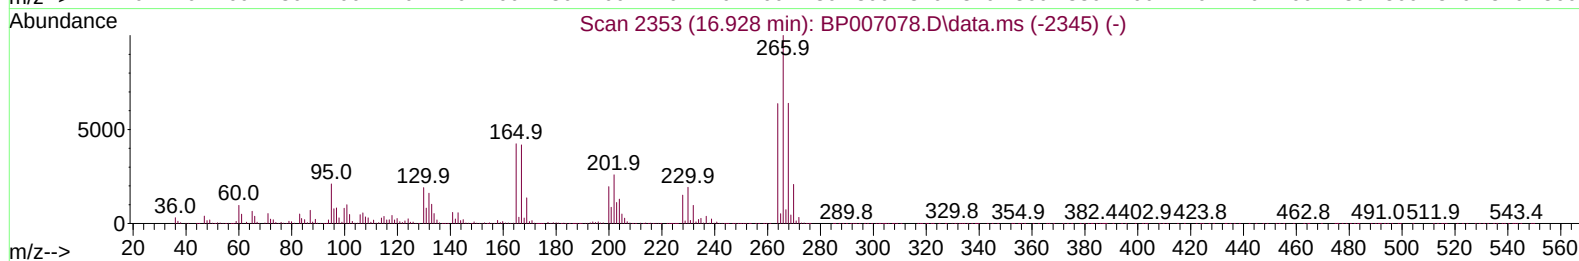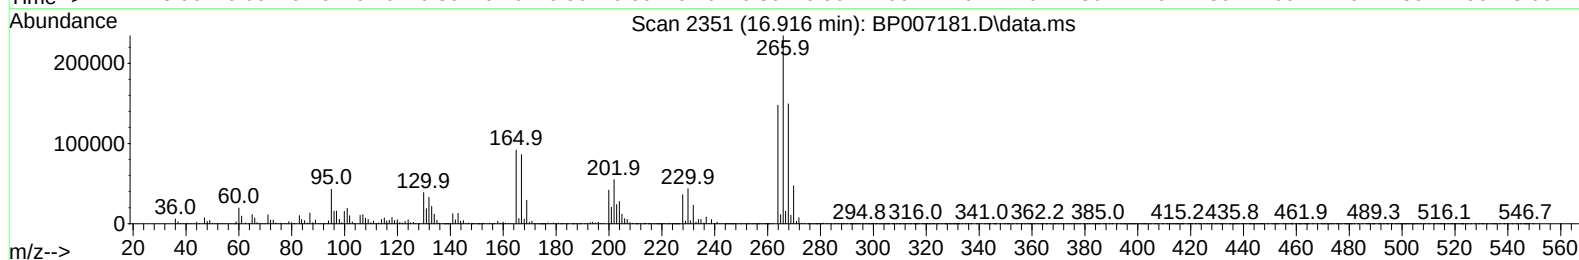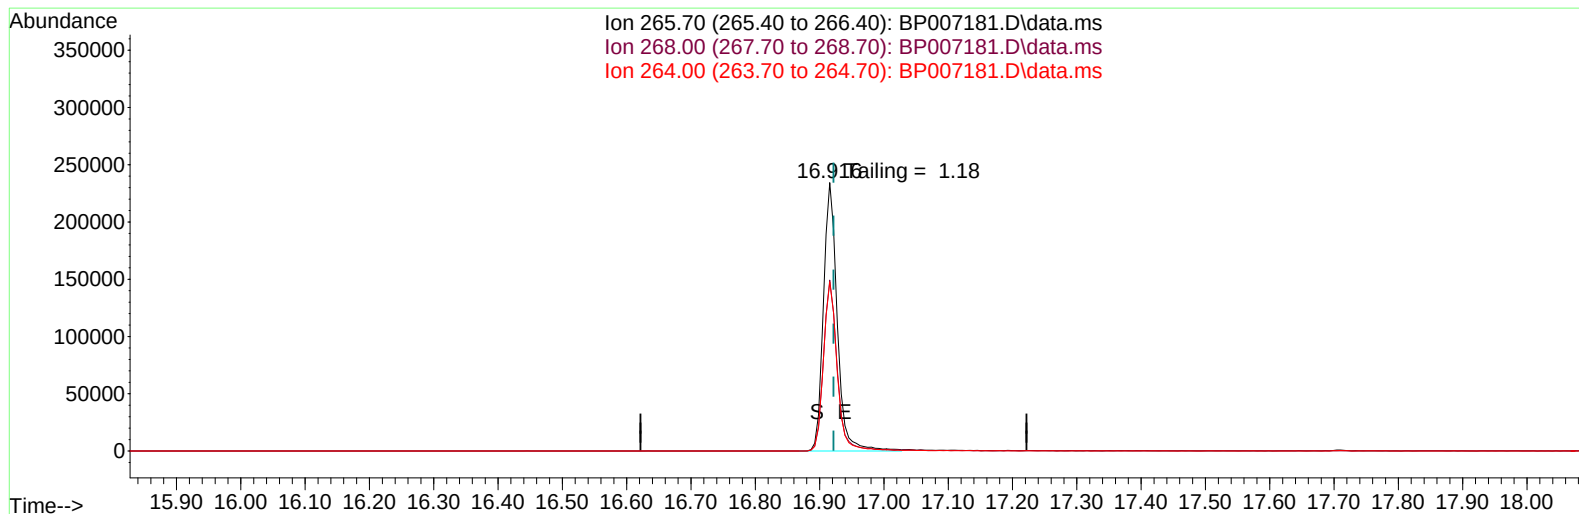

TIC: BP007181.D\data.ms

(70) Pentachlorophenol (C)

16.916min (-0.006) 2479346.40 ng




response 354359

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.50	63.71
264.00	62.90	63.05
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP092521\
 Data File : BP007181.D
 Acq On : 25 Sep 2021 11:53
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Quant Time: Sep 26 06:27:06 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP092121.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Sep 23 11:17:25 2021
 Response via : Initial Calibration

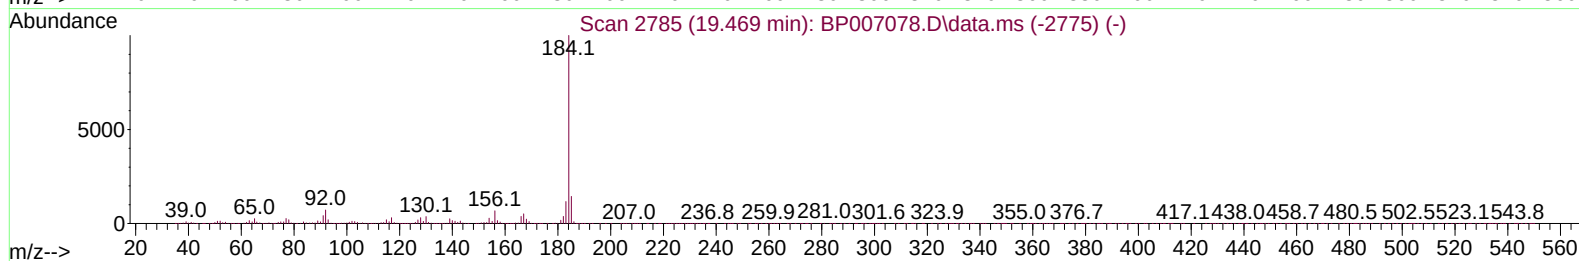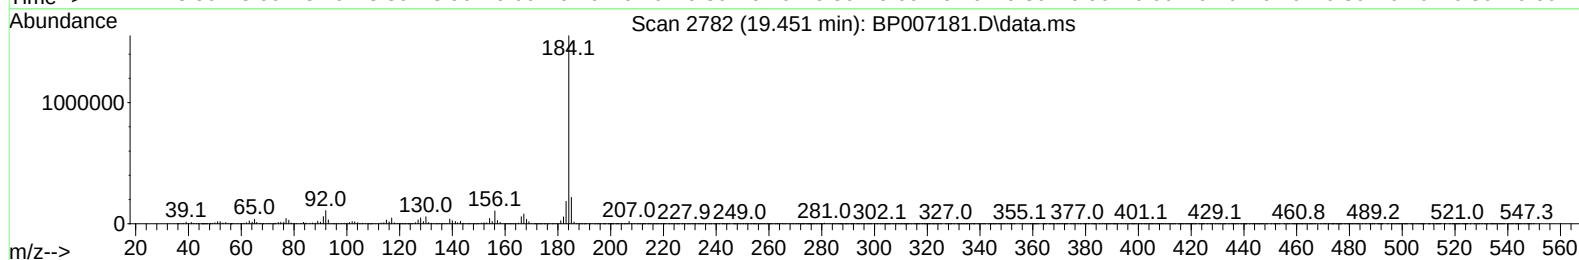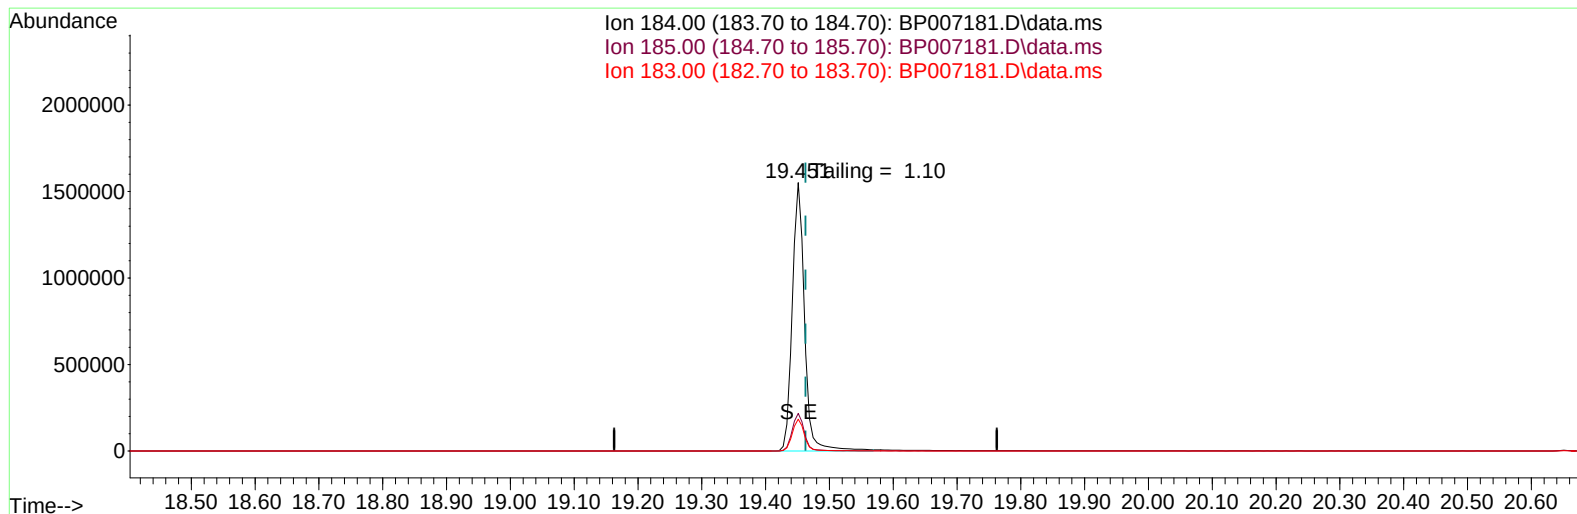

TIC: BP007181.D\data.ms

(77) Benzidine

19.451min (-0.012) 15280.00 ng

response 2091971

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.70	14.05
183.00	11.90	11.89
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
9/25/2021	BNA_P	<u>BP007181.D</u>
Compound Name	Response	Retention Time
DDT	1075166	20.651
DDD	13339	20.222
DDE	1000	19.733
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
14339	1089505	1.32