

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP092523\
 Data File : BP017366.D
 Acq On : 26 Sep 2023 17:36
 Operator : MA/JU
 Sample : 04450-10
 Misc :
 ALS Vial : 58 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BBKB0

Quant Time: Sep 27 00:29:29 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP092023.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Sep 26 04:52:29 2023
 Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.922	152	163498	20.000	ng/ul	0.00
20) Naphthalene-d8	10.746	136	713189	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.587	164	440290	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.357	188	931401	20.000	ng/ul	0.00
79) Chrysene-d12	21.463	240	863665	20.000	ng/ul	0.00
88) Perylene-d12	23.974	264	951499	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.299	96	15814	3.973	ng/uL	0.00
4) Pyridine-d5	3.734	84	128215	11.522	ng/ul	0.00
7) Phenol-d5	7.081	99	91313	6.800	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.269	67	302064	37.275	ng/ul	0.00
11) 2-Chlorophenol-d4	7.446	132	291738	27.393	ng/ul	0.00
15) 4-Methylphenol-d8	8.640	113	177039	16.958	ng/ul	0.00
21) Nitrobenzene-d5	9.122	128	193015	37.436	ng/ul	0.00
24) 2-Nitrophenol-d4	9.840	143	197185	35.222	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.363	165	333411	31.522	ng/ul	0.00
31) 4-Chloroaniline-d4	10.916	131	493440	32.206	ng/ul	0.00
46) Dimethylphthalate-d6	14.004	166	1199099	38.017	ng/ul	0.00
49) Acenaphthylene-d8	14.287	160	1295355	35.708	ng/ul	0.00
54) 4-Nitrophenol-d4	14.828	143	19125	3.480	ng/ul	0.01
60) Fluorene-d10	15.581	176	1050811	38.698	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.716	200	113175	21.559	ng/ul	0.00
73) Anthracene-d10	17.457	188	1803910	43.669	ng/ul	0.00
81) Pyrene-d10	19.704	212	2098623	44.934	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.815	264	2075899	45.314	ng/ul	0.00
Target Compounds						
35) 4-Chloro-3-methylphenol	12.046	107	26247	2.504	ng/ul	Qvalue 98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP092523\
Data File : BP017366.D
Acq On : 26 Sep 2023 17:36
Operator : MA/JU
Sample : 04450-10
Misc :
ALS Vial : 58 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BBKB0

Quant Time: Sep 27 00:29:29 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP092023.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Sep 26 04:52:29 2023
Response via : Initial Calibration

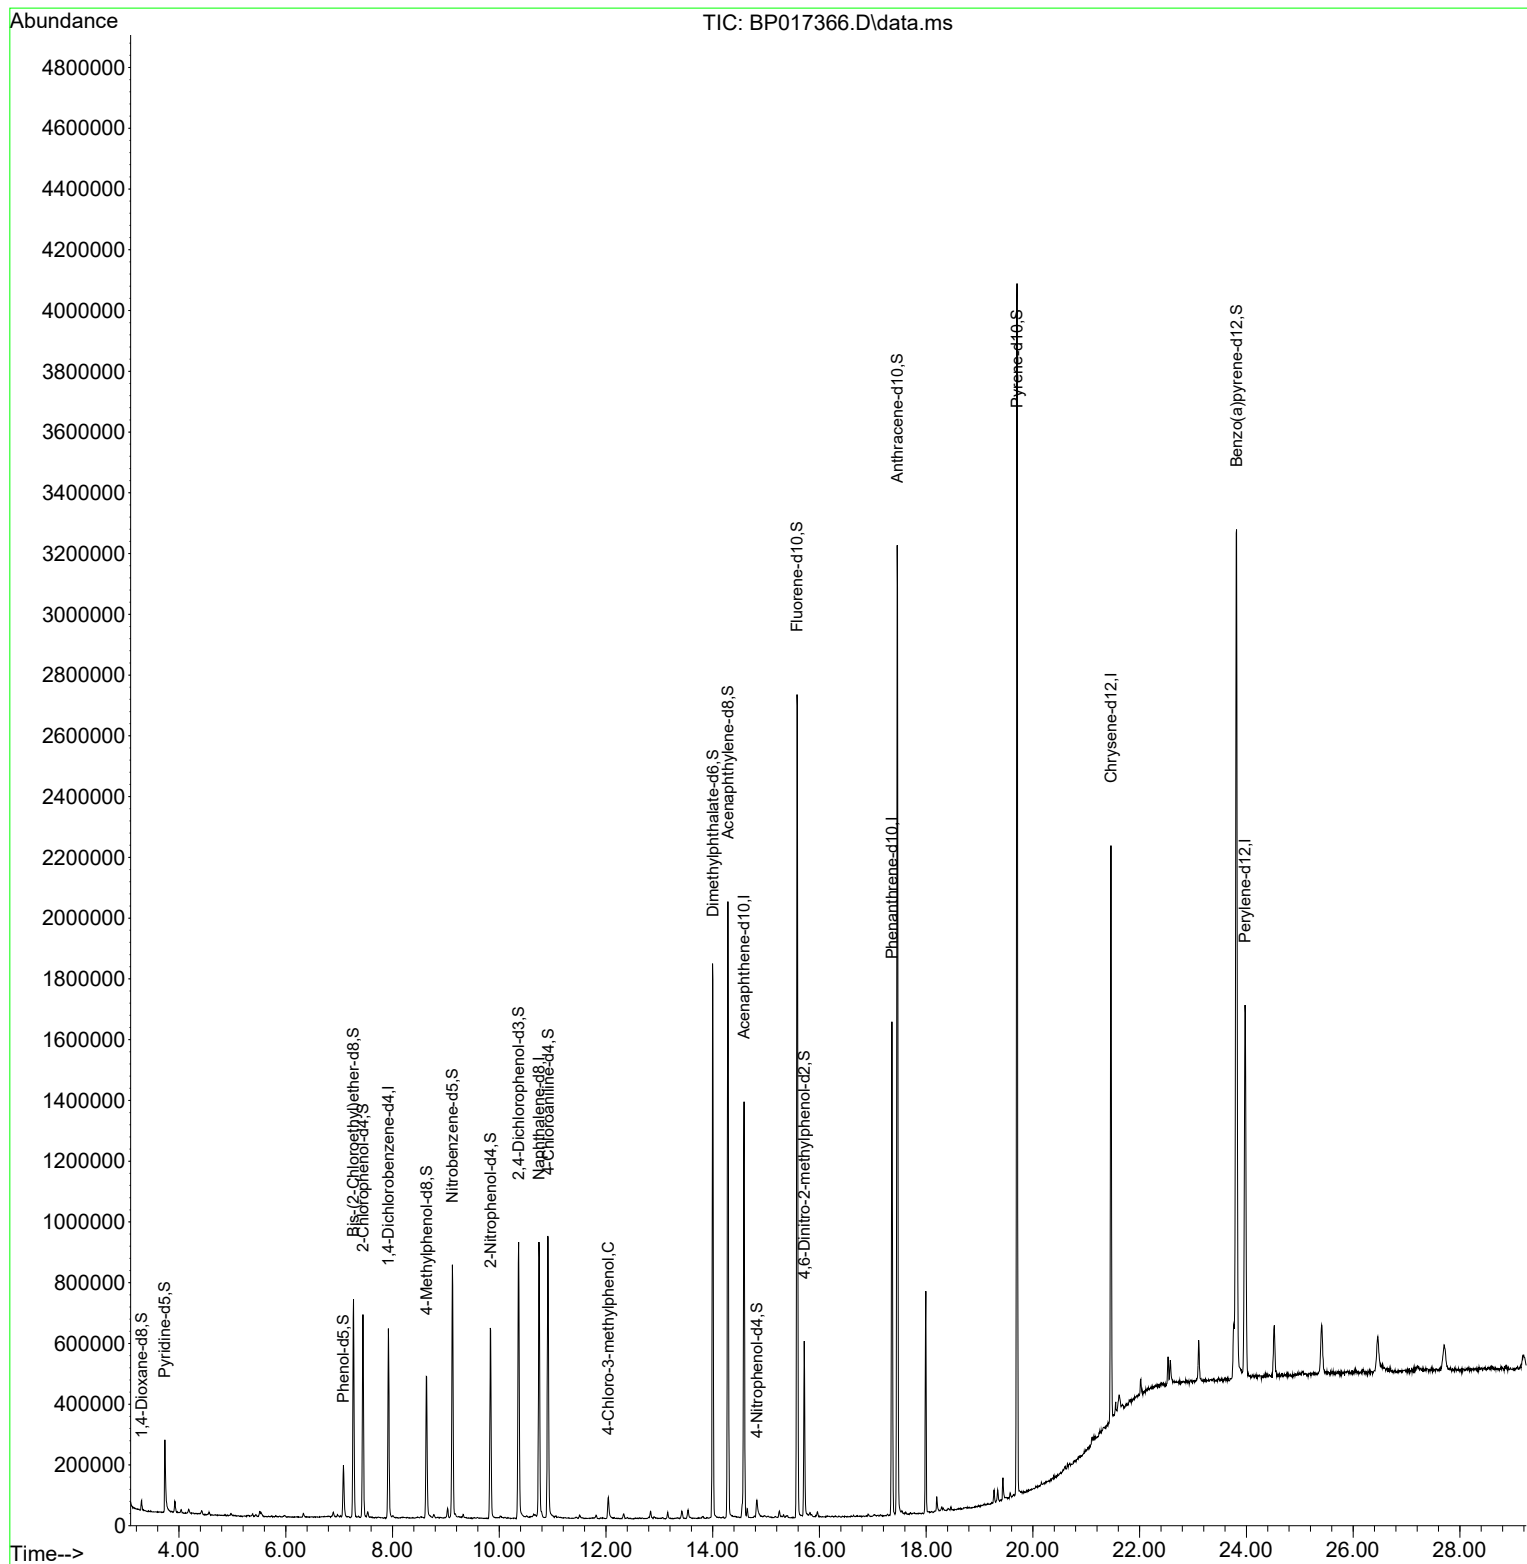

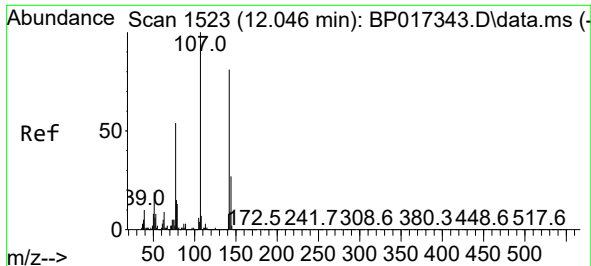

#35

4-Chloro-3-methylphenol

Concen: 2.504 ng/ul

RT: 12.046 min Scan# 1

Delta R.T. 0.000 min

Lab File: BP017366.D


Acq: 26 Sep 2023 17:36

Instrument :

BNA_P

ClientSampleId :

BBKB0

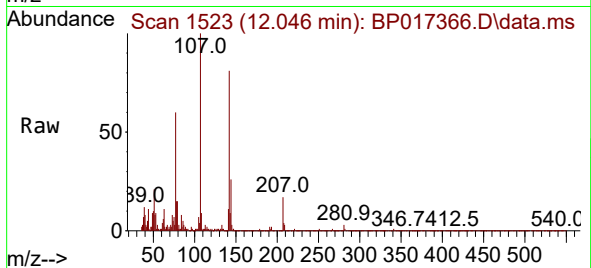

Tgt Ion:107 Resp: 26247

Ion Ratio Lower Upper

107 100

144 25.7 20.6 31.0

142 81.2 62.9 94.3

