




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP092523\
 Data File : BP017365.D
 Acq On : 26 Sep 2023 17:02
 Operator : MA/JU
 Sample : 04450-04
 Misc :
 ALS Vial : 57 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BBJ65

Manual IntegrationsAPPROVED

Quant Time: Sep 27 00:29:19 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP092023.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Sep 26 04:52:29 2023
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 09/27/2023
 Supervised By :mohammad ahmed 09/29/2023

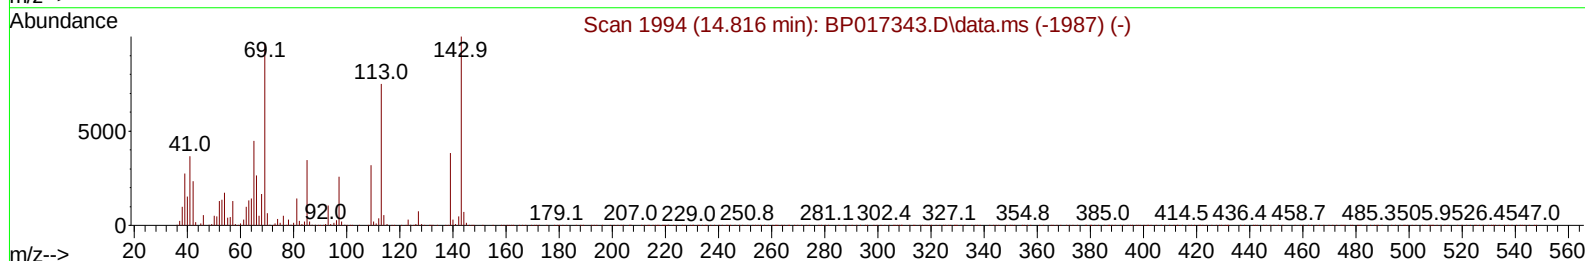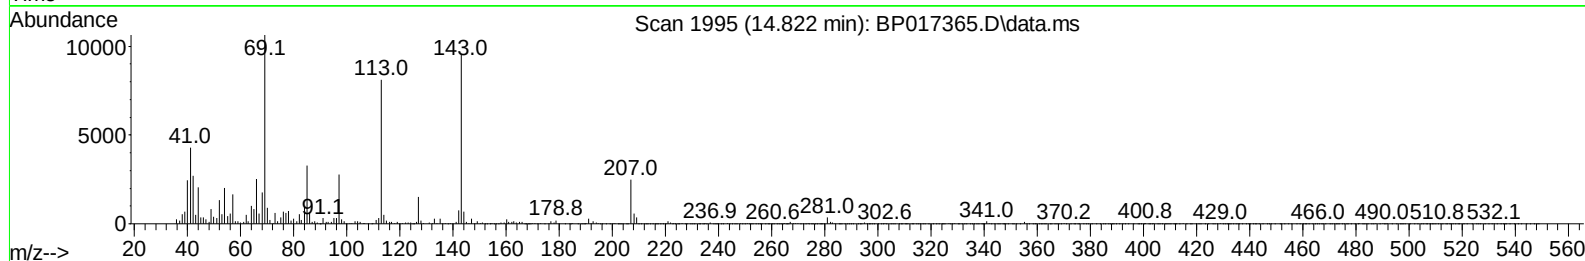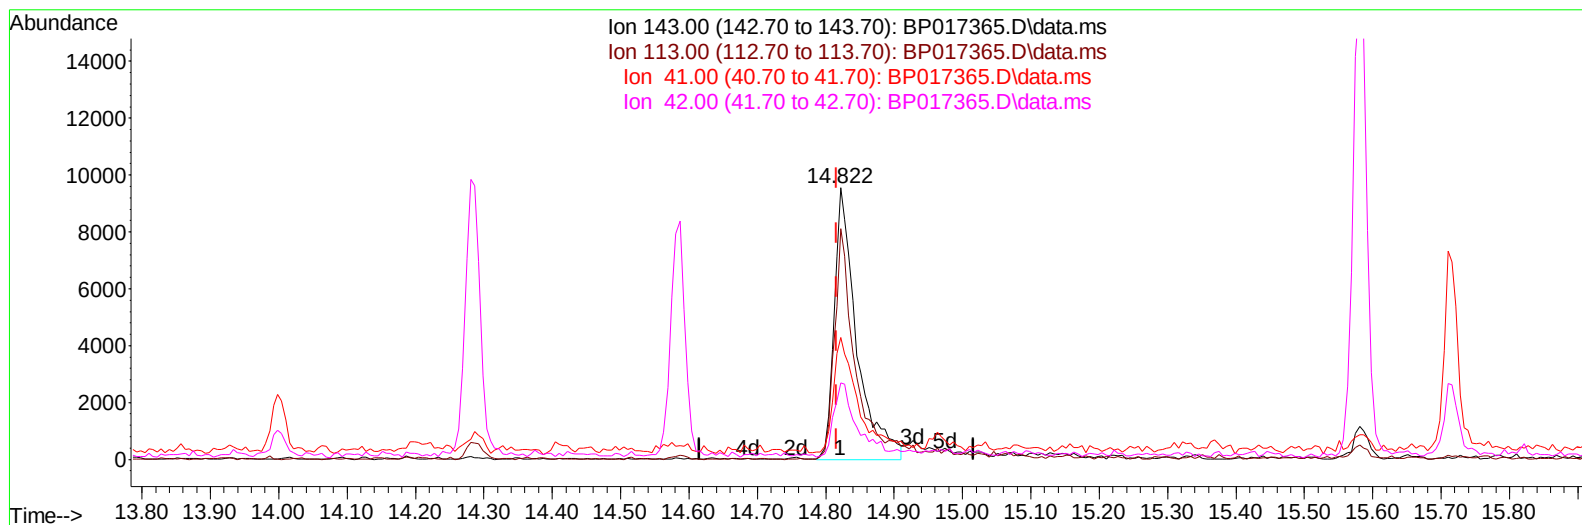

TIC: BP017365.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.822min (+ 0.006) 4.61 ng/ul m

response 21775

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	74.90	84.90
41.00	36.70	44.88#
42.00	26.40	28.30

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP092523\
 Data File : BP017365.D
 Acq On : 26 Sep 2023 17:02
 Operator : MA/JU
 Sample : 04450-04
 Misc :
 ALS Vial : 57 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BBJ65

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 09/27/2023
 Supervised By :mohammad ahmed 09/29/2023

Quant Time: Sep 27 01:32:29 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP092023.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Sep 26 04:52:29 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.922	152	145224	20.000	ng/ul	0.00
20) Naphthalene-d8	10.746	136	627189	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.587	164	378062	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.357	188	834654	20.000	ng/ul	0.00
79) Chrysene-d12	21.463	240	803128	20.000	ng/ul	0.00
88) Perylene-d12	23.974	264	893236	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.299	96	16941	4.792	ng/uL	0.00
4) Pyridine-d5	3.734	84	91639	9.271	ng/ul	0.00
7) Phenol-d5	7.081	99	87727	7.355	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.269	67	269684	37.467	ng/ul	0.00
11) 2-Chlorophenol-d4	7.446	132	268067	28.337	ng/ul	0.00
15) 4-Methylphenol-d8	8.634	113	163429	17.624	ng/ul	0.00
21) Nitrobenzene-d5	9.122	128	171632	37.853	ng/ul	0.00
24) 2-Nitrophenol-d4	9.834	143	177116	35.975	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.363	165	302031	32.471	ng/ul	0.00
31) 4-Chloroaniline-d4	10.910	131	398520	29.577	ng/ul	0.00
46) Dimethylphthalate-d6	13.998	166	1109992	40.985	ng/ul	0.00
49) Acenaphthylene-d8	14.287	160	1161196	37.279	ng/ul	0.00
54) 4-Nitrophenol-d4	14.822	143	21775m	4.615	ng/ul	0.00
60) Fluorene-d10	15.581	176	948106	40.663	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.716	200	119743	25.454	ng/ul	0.00
73) Anthracene-d10	17.457	188	1620039	43.764	ng/ul	0.00
81) Pyrene-d10	19.698	212	2001982	46.096	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.810	264	1960895	45.595	ng/ul	0.00

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP092523\
Data File : BP017365.D
Acq On : 26 Sep 2023 17:02
Operator : MA/JU
Sample : 04450-04
Misc :
ALS Vial : 57 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BBJ65

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 09/27/2023
Supervised By :mohammad ahmed 09/29/2023

Quant Time: Sep 27 01:32:29 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP092023.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Sep 26 04:52:29 2023
Response via : Initial Calibration

