

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP092523\
 Data File : BP017338.D
 Acq On : 26 Sep 2023 00:58
 Operator : MA/JU
 Sample : 04472-17
 Misc :
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 EZYM6

Quant Time: Sep 26 01:59:04 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP092023.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Sep 21 23:51:07 2023
 Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.928	152	158268	20.000	ng/u1	-0.01
20) Naphthalene-d8	10.746	136	681368	20.000	ng/u1	-0.02
38) Acenaphthene-d10	14.587	164	424593	20.000	ng/u1	-0.01
64) Phenanthrene-d10	17.357	188	949799	20.000	ng/u1	-0.01
79) Chrysene-d12	21.463	240	871104	20.000	ng/u1	-0.01
88) Perylene-d12	23.974	264	955069	20.000	ng/u1	-0.02
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.299	96	14596	3.788	ng/uL	0.00
4) Pyridine-d5	3.746	84	24895	2.311	ng/u1	0.00
7) Phenol-d5	7.081	99	190045	14.621	ng/u1	-0.02
9) Bis-(2-Chloroethyl)eth...	7.269	67	167448	21.346	ng/u1	-0.01
11) 2-Chlorophenol-d4	7.446	132	128410	12.455	ng/u1	-0.02
15) 4-Methylphenol-d8	8.640	113	140132	13.867	ng/u1	-0.02
21) Nitrobenzene-d5	9.122	128	98552	20.007	ng/u1	-0.02
24) 2-Nitrophenol-d4	9.840	143	54636	10.215	ng/u1	-0.01
28) 2,4-Dichlorophenol-d3	10.363	165	107529	10.641	ng/u1	-0.02
31) 4-Chloroaniline-d4	10.916	131	247450	16.905	ng/u1	-0.01
46) Dimethylphthalate-d6	13.998	166	671618	22.081	ng/u1	-0.02
49) Acenaphthylene-d8	14.287	160	708104	20.241	ng/u1	-0.01
54) 4-Nitrophenol-d4	14.828	143	19624	3.703	ng/u1	0.00
60) Fluorene-d10	15.581	176	578705	22.100	ng/u1	-0.02
65) 4,6-Dinitro-2-methylph...	15.722	200	12017	2.245	ng/u1	0.00
73) Anthracene-d10	17.457	188	883530	20.974	ng/u1	-0.01
81) Pyrene-d10	19.698	212	1157537	24.573	ng/u1	-0.02
92) Benzo(a)pyrene-d12	23.804	264	1060390	23.060	ng/u1	-0.03
Target Compounds						
16) Acetophenone	8.775	105	54448	3.487	ng/u1	97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP092523\
Data File : BP017338.D
Acq On : 26 Sep 2023 00:58
Operator : MA/JU
Sample : 04472-17
Misc :
ALS Vial : 29 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
EZY6

Quant Time: Sep 26 01:59:04 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP092023.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Sep 21 23:51:07 2023
Response via : Initial Calibration

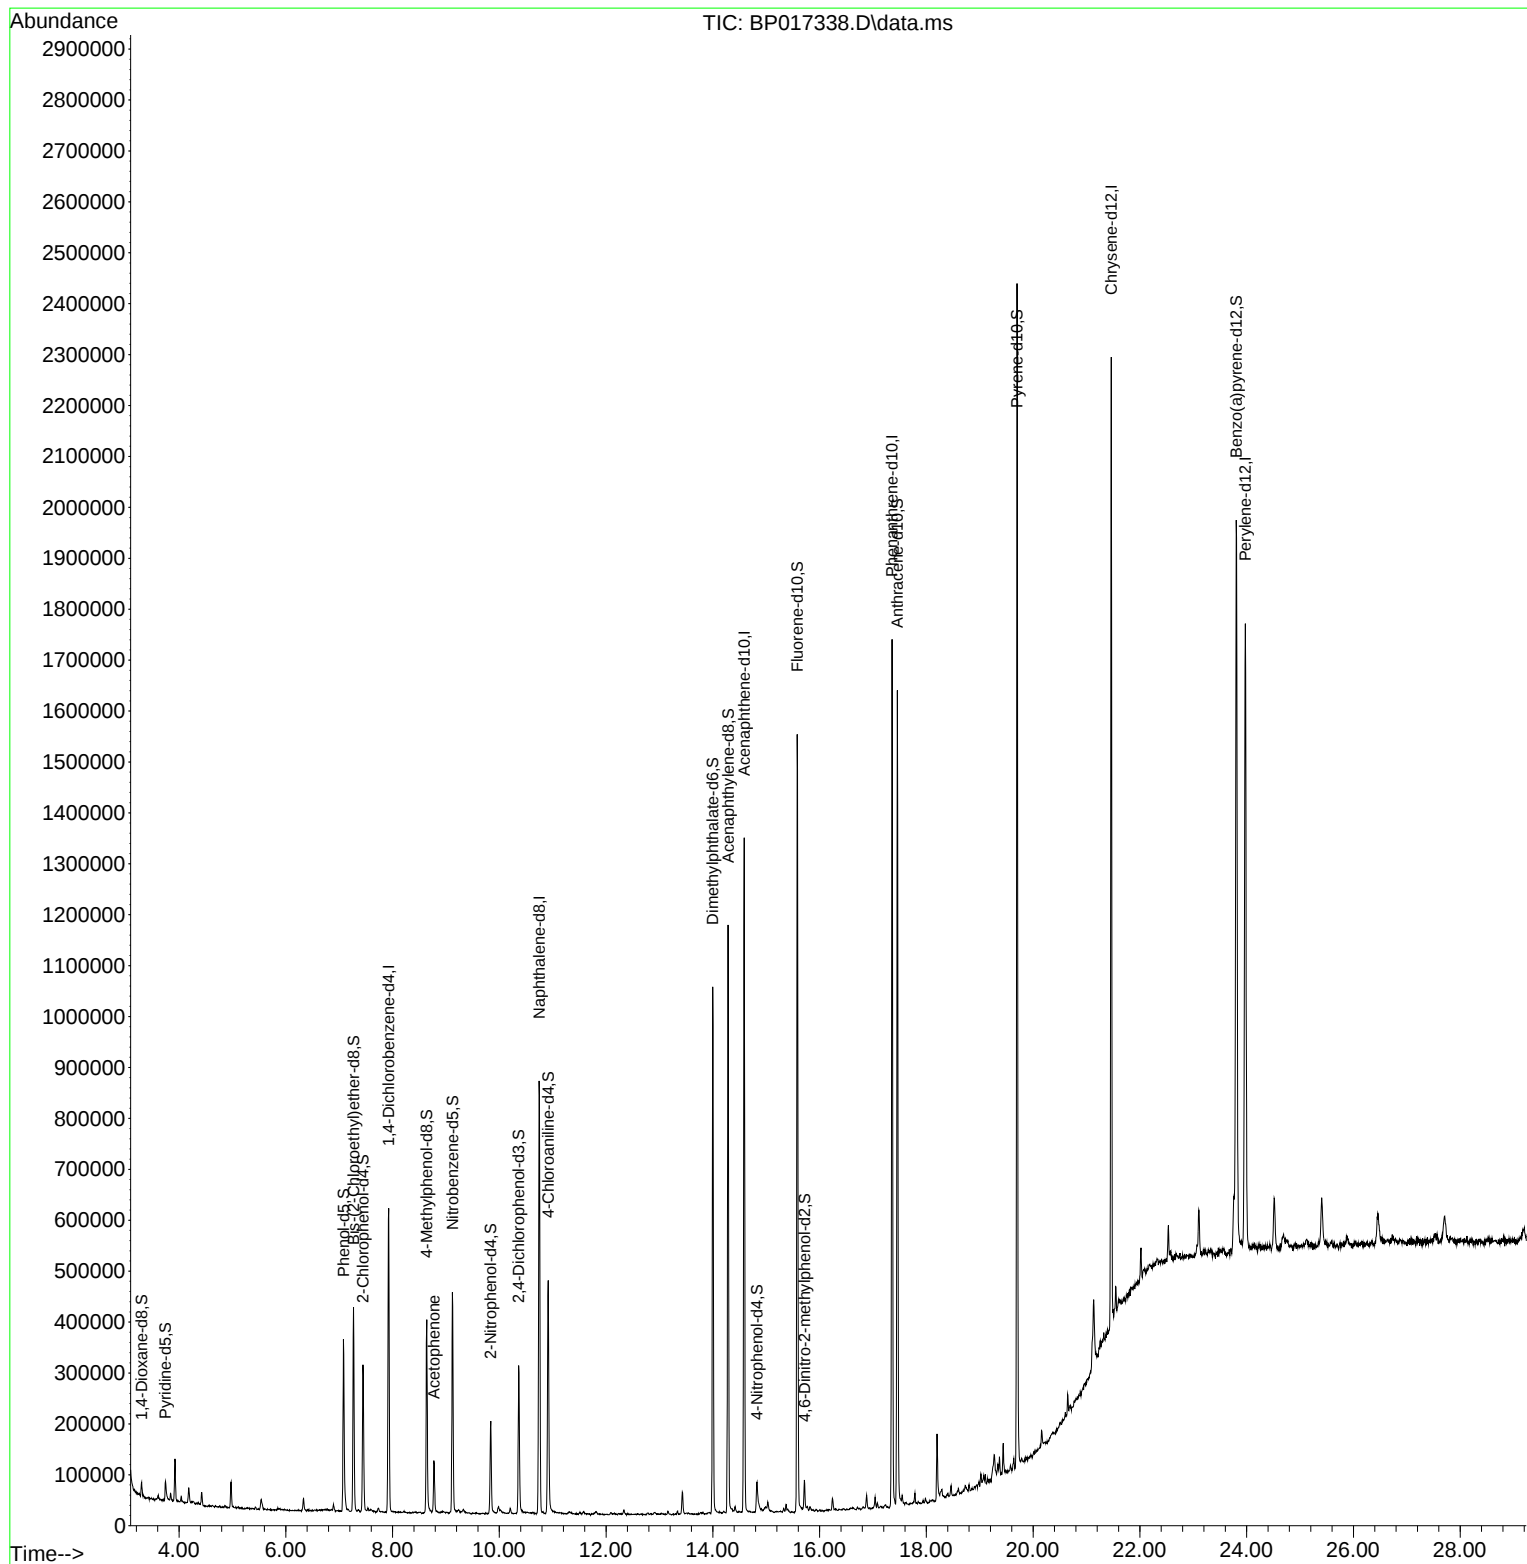

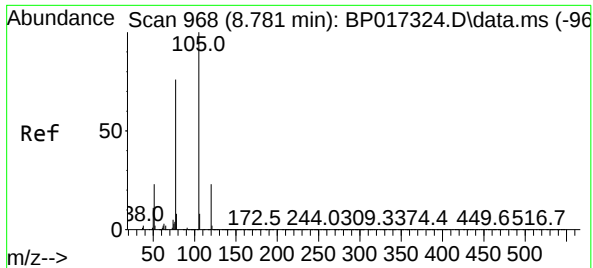

#16
 Acetophenone
 Concen: 3.487 ng/ul
 RT: 8.775 min Scan# 90
 Delta R.T. -0.012 min
 Lab File: BP017338.D
 Acq: 26 Sep 2023 00:58

Instrument :
 BNA_P
 ClientSampleId :
 EZYM6

Tgt Ion:	105	Resp:	54448
Ion	Ratio	Lower	Upper
105	100		
77	77.2	63.6	95.4
51	26.0	19.2	28.8

