

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP092523\
 Data File : BP017347.D
 Acq On : 26 Sep 2023 06:37
 Operator : MA/JU
 Sample : 04450-03
 Misc :
 ALS Vial : 39 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BBJN8

Quant Time: Sep 26 07:07:10 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP092023.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Sep 26 04:52:29 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.922	152	206663	20.000	ng/u1	0.00
20) Naphthalene-d8	10.746	136	906364	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.587	164	558561	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.357	188	1224089	20.000	ng/u1	0.00
79) Chrysene-d12	21.463	240	1117922	20.000	ng/u1	0.00
88) Perylene-d12	23.974	264	1216679	20.000	ng/u1	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.299	96	24184	4.807	ng/uL	0.00
4) Pyridine-d5	3.734	84	196891	13.998	ng/u1	0.00
7) Phenol-d5	7.081	99	155305	9.150	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.269	67	460083	44.916	ng/u1	0.00
11) 2-Chlorophenol-d4	7.446	132	453869	33.715	ng/u1	0.00
15) 4-Methylphenol-d8	8.640	113	303367	22.990	ng/u1	0.00
21) Nitrobenzene-d5	9.122	128	301820	46.062	ng/u1	0.00
24) 2-Nitrophenol-d4	9.840	143	314343	44.182	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.363	165	538315	40.048	ng/u1	0.00
31) 4-Chloroaniline-d4	10.910	131	666334	34.221	ng/u1	0.00
46) Dimethylphthalate-d6	14.004	166	2059356	51.466	ng/u1	0.00
49) Acenaphthylene-d8	14.287	160	2150641	46.732	ng/u1	0.00
54) 4-Nitrophenol-d4	14.822	143	48141	6.906	ng/u1	0.00
60) Fluorene-d10	15.581	176	1753763	50.910	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.716	200	288221	41.776	ng/u1	0.00
73) Anthracene-d10	17.457	188	2901518	53.446	ng/u1	0.00
81) Pyrene-d10	19.704	212	3409499	56.398	ng/u1	0.00
92) Benzo(a)pyrene-d12	23.810	264	3207833	54.760	ng/u1	0.00
Target Compounds						
2) 1,4-Dioxane	3.334	88	20728	4.023	ng/uL	89


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP092523\
Data File : BP017347.D
Acq On : 26 Sep 2023 06:37
Operator : MA/JU
Sample : 04450-03
Misc :
ALS Vial : 39 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BBJN8

Quant Time: Sep 26 07:07:10 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP092023.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Sep 26 04:52:29 2023
Response via : Initial Calibration

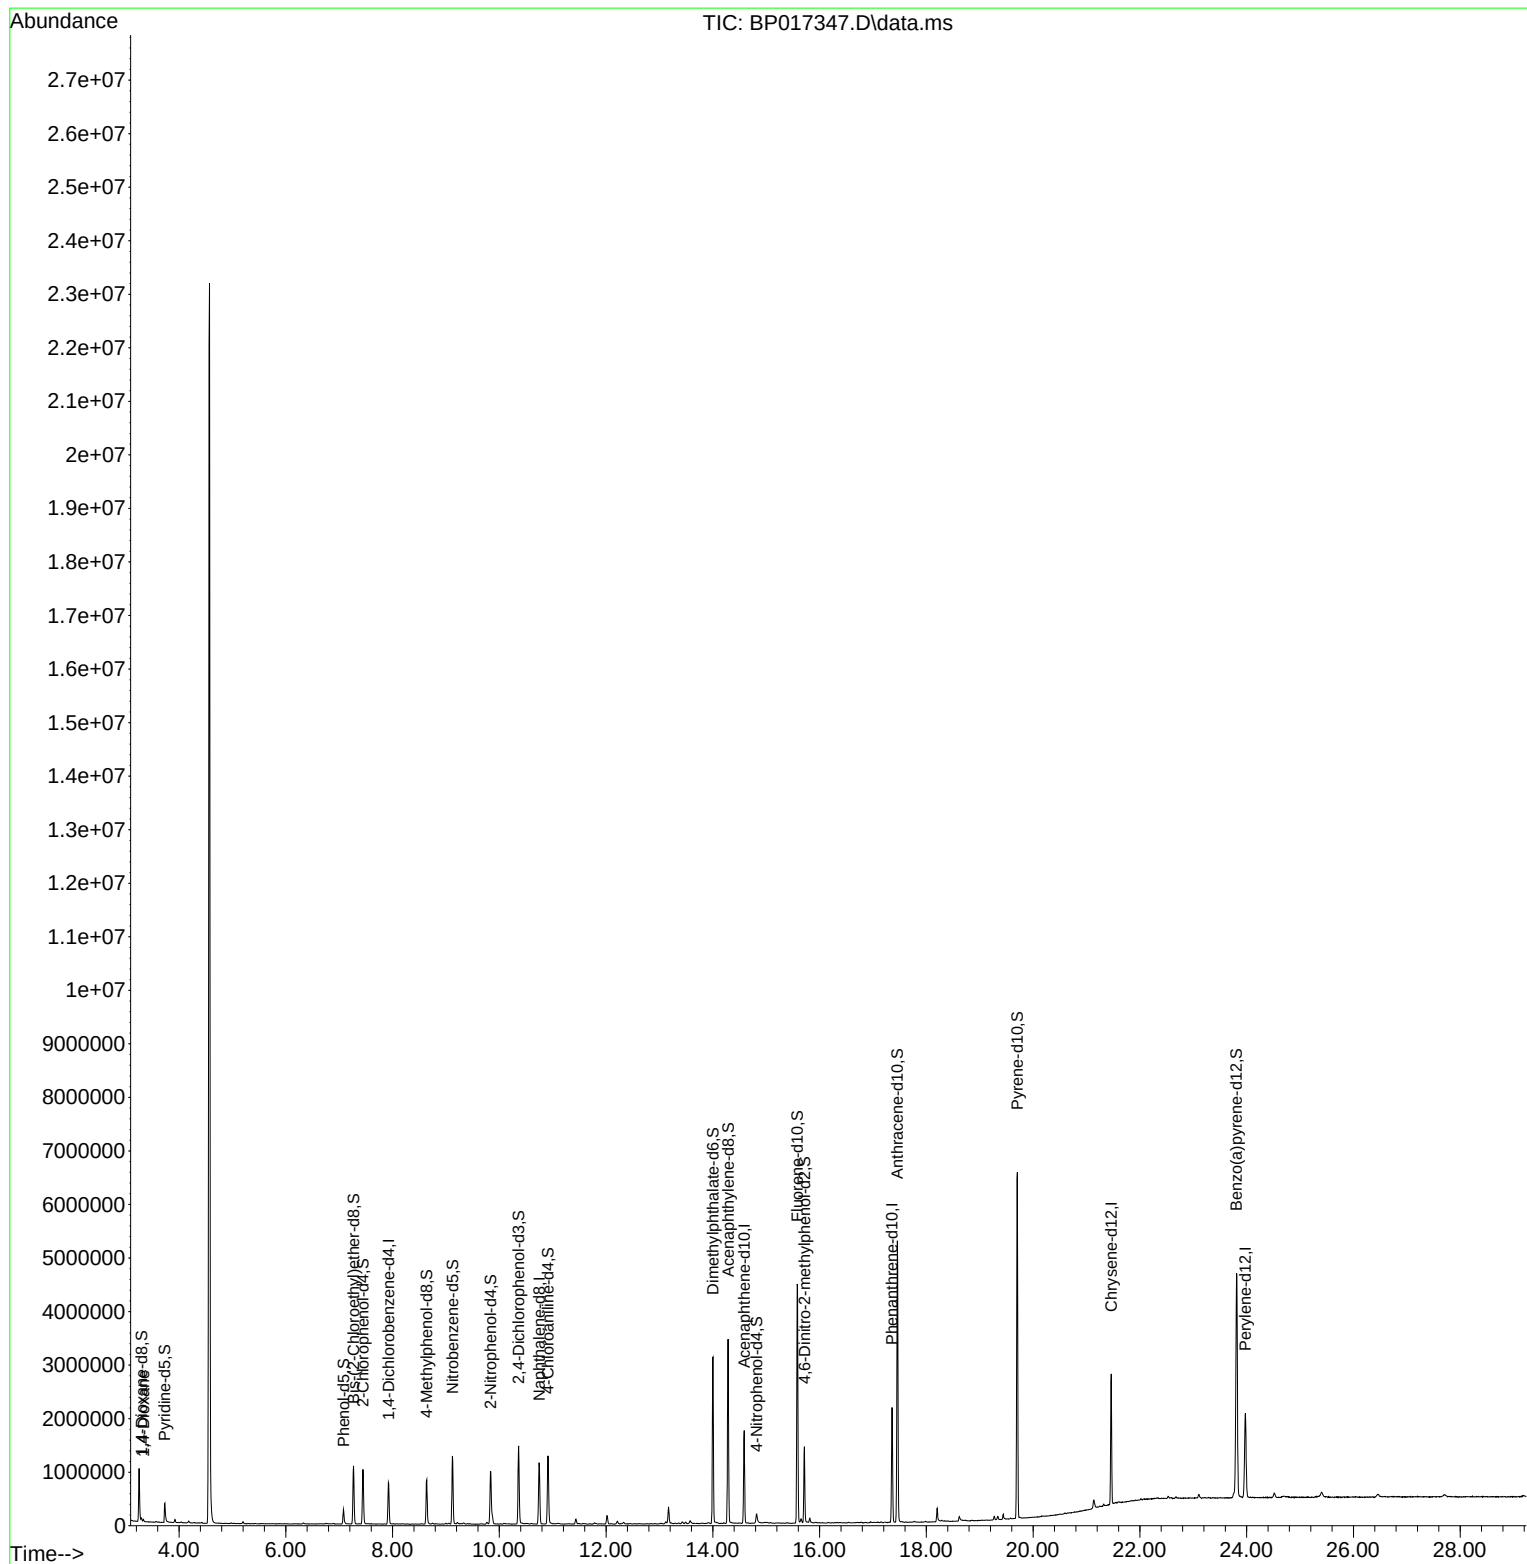

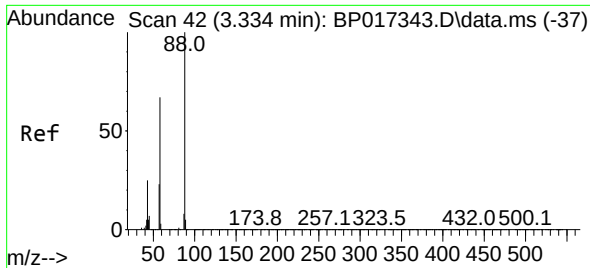

#2
 1,4-Dioxane
 Concen: 4.023 ng/uL
 RT: 3.334 min Scan# 41
 Delta R.T. 0.000 min
 Lab File: BP017347.D
 Acq: 26 Sep 2023 06:37

Instrument :
 BNA_P
 ClientSampleId :
 BBJN8

Tgt Ion: 88 Resp: 20728
 Ion Ratio Lower Upper
 88 100
 43 26.5 25.0 37.4
 58 61.0 56.6 84.8

