

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP092523\
 Data File : BP017353.D
 Acq On : 26 Sep 2023 10:00
 Operator : MA/JU
 Sample : 04472-14
 Misc :
 ALS Vial : 45 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 EZYM3

Quant Time: Sep 27 00:25:57 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP092023.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Sep 26 04:52:29 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.928	152	216386	20.000	ng/u1	0.00
20) Naphthalene-d8	10.745	136	915232	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.586	164	530521	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.357	188	1108345	20.000	ng/u1	0.00
79) Chrysene-d12	21.462	240	1029087	20.000	ng/u1	0.00
88) Perylene-d12	23.974	264	1151349	20.000	ng/u1	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.299	96	15498	2.942	ng/uL	0.00
4) Pyridine-d5	3.746	84	25035	1.700	ng/u1	0.02
7) Phenol-d5	7.081	99	256807	14.450	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.269	67	188263	17.553	ng/u1	0.00
11) 2-Chlorophenol-d4	7.446	132	174295	12.365	ng/u1	0.00
15) 4-Methylphenol-d8	8.640	113	116029	8.398	ng/u1	0.00
21) Nitrobenzene-d5	9.122	128	115460	17.450	ng/u1	0.00
24) 2-Nitrophenol-d4	9.840	143	63878	8.891	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.363	165	127797	9.415	ng/u1	0.00
31) 4-Chloroaniline-d4	10.916	131	217463	11.060	ng/u1	0.00
46) Dimethylphthalate-d6	13.998	166	677503	17.827	ng/u1	0.00
49) Acenaphthylene-d8	14.286	160	747980	17.112	ng/u1	0.00
54) 4-Nitrophenol-d4	14.816	143	84	0.013	ng/u1	0.00
60) Fluorene-d10	15.580	176	582791	17.812	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.722	200	363	0.058	ng/u1	0.00
73) Anthracene-d10	17.457	188	794721	16.167	ng/u1	0.00
81) Pyrene-d10	19.698	212	1082098	19.445	ng/u1	0.00
92) Benzo(a)pyrene-d12	23.803	264	1038364	18.732	ng/u1	0.00


Target Compounds					Qvalue
16) Acetophenone	8.775	105	70380	3.296 ng/u1	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP092523\
Data File : BP017353.D
Acq On : 26 Sep 2023 10:00
Operator : MA/JU
Sample : 04472-14
Misc :
ALS Vial : 45 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
EZYM3

Quant Time: Sep 27 00:25:57 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP092023.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Sep 26 04:52:29 2023
Response via : Initial Calibration

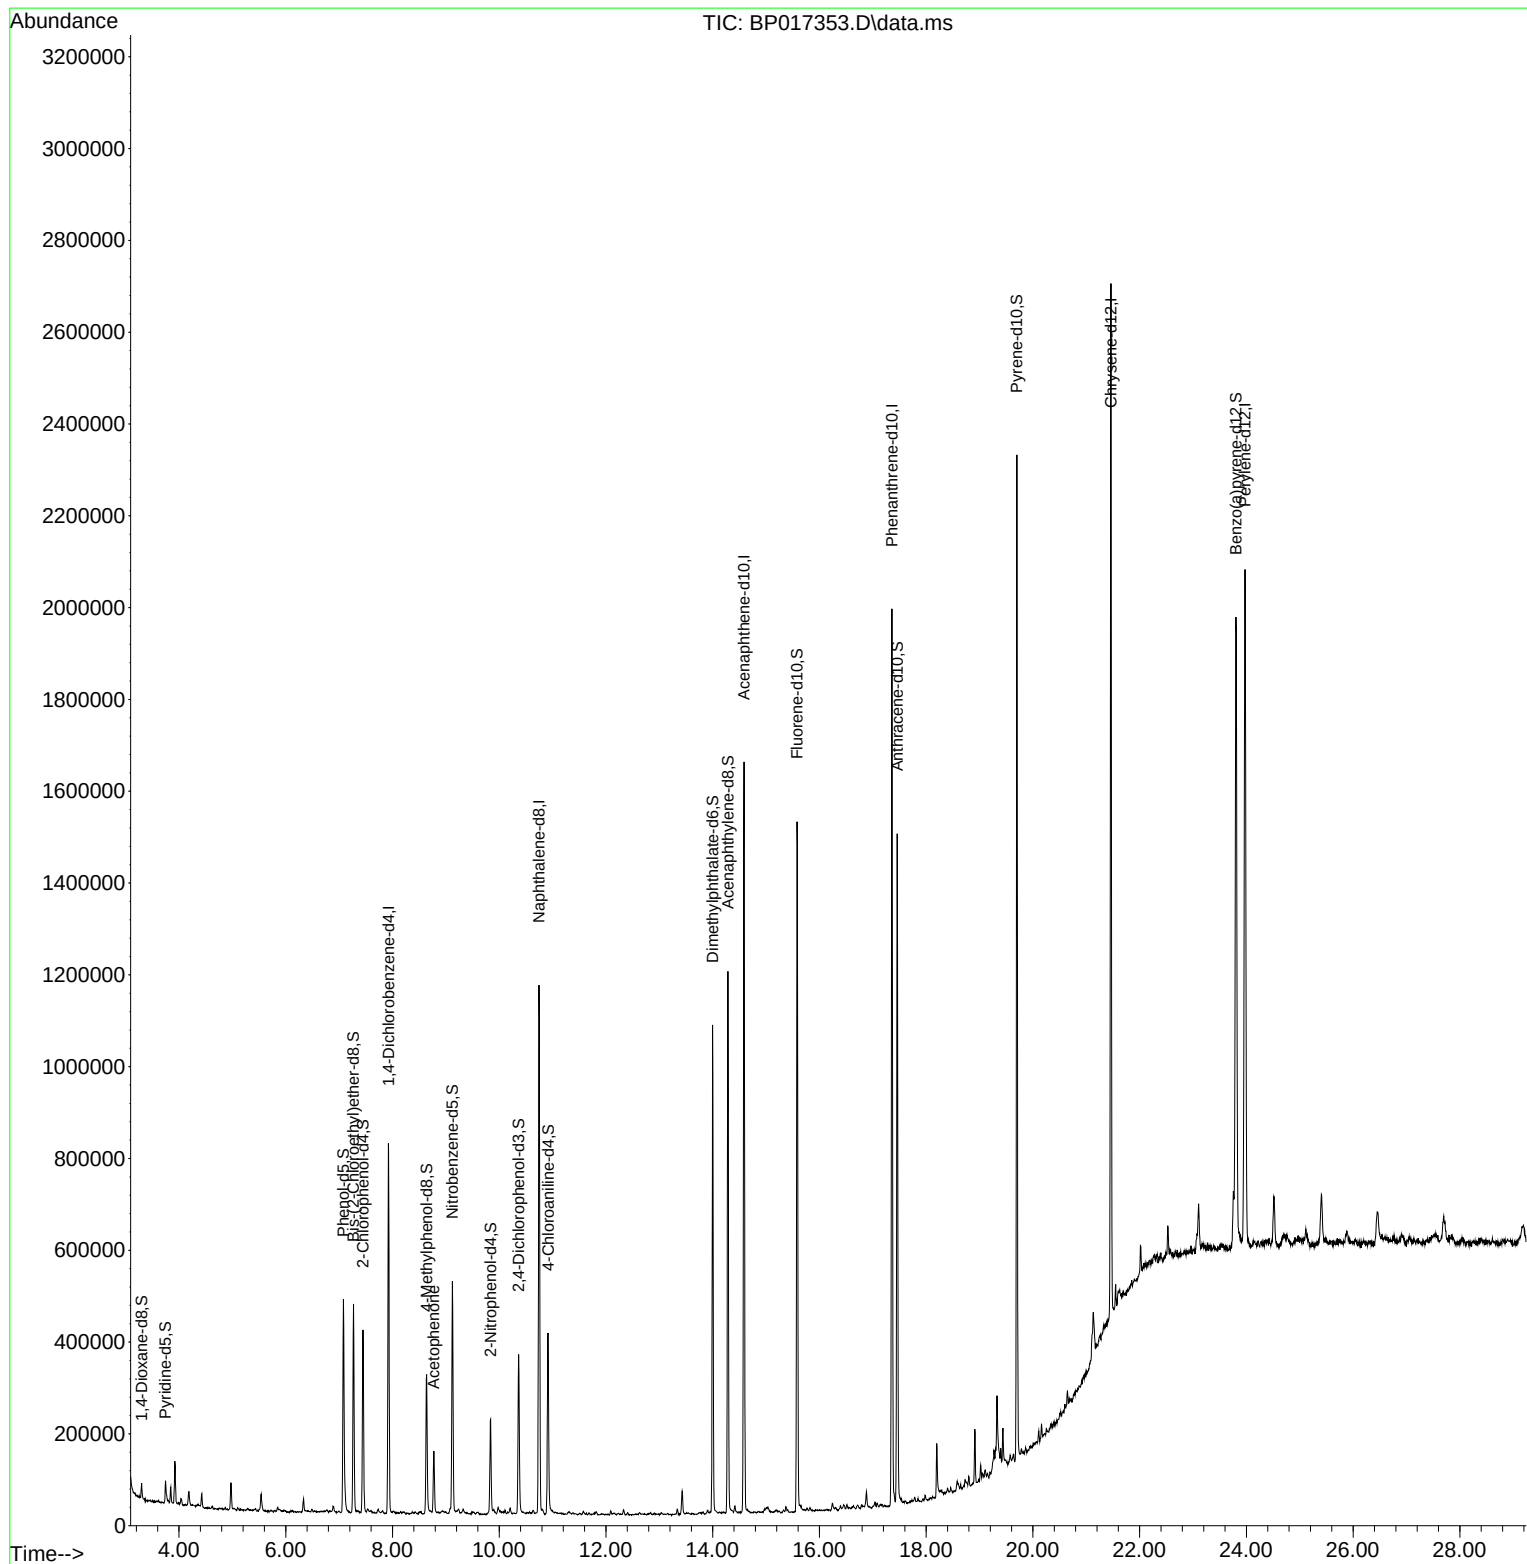

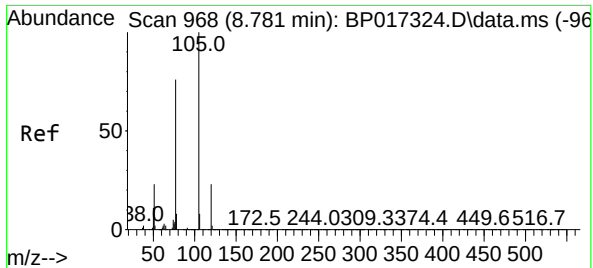

#16
 Acetophenone
 Concen: 3.296 ng/ul
 RT: 8.775 min Scan# 90
 Delta R.T. -0.000 min
 Lab File: BP017353.D
 Acq: 26 Sep 2023 10:00

Instrument :
 BNA_P
 ClientSampleId :
 EZYM3

Tgt Ion:	105	Resp:	70380
Ion	Ratio	Lower	Upper
105	100		
77	78.9	63.6	95.4
51	28.0	19.2	28.8

