

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP092523\
 Data File : BP017371.D
 Acq On : 26 Sep 2023 20:26
 Operator : MA/JU
 Sample : 04450-15
 Misc :
 ALS Vial : 63 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BBBN0

Quant Time: Sep 27 01:55:41 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP092023.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Sep 26 04:52:29 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.922	152	134572	20.000	ng/u1	0.00
20) Naphthalene-d8	10.746	136	578736	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.581	164	343133	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.357	188	776333	20.000	ng/u1	0.00
79) Chrysene-d12	21.457	240	747868	20.000	ng/u1	0.00
88) Perylene-d12	23.968	264	843654	20.000	ng/u1	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.299	96	20780	6.343	ng/uL	0.00
4) Pyridine-d5	3.740	84	163365	17.836	ng/u1	0.01
7) Phenol-d5	7.081	99	109912	9.945	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.263	67	292557	43.861	ng/u1	0.00
11) 2-Chlorophenol-d4	7.446	132	294461	33.591	ng/u1	0.00
15) 4-Methylphenol-d8	8.640	113	157692	18.352	ng/u1	0.00
21) Nitrobenzene-d5	9.122	128	177762	42.487	ng/u1	0.00
24) 2-Nitrophenol-d4	9.834	143	172300	37.927	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.363	165	333645	38.873	ng/u1	0.00
31) 4-Chloroaniline-d4	10.916	131	332932	26.778	ng/u1	0.00
46) Dimethylphthalate-d6	13.998	166	1174280	47.772	ng/u1	0.00
49) Acenaphthylene-d8	14.281	160	1298410	45.927	ng/u1	0.00
54) 4-Nitrophenol-d4	14.822	143	32396	7.565	ng/u1	0.00
60) Fluorene-d10	15.581	176	1020282	48.213	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.716	200	114888	26.257	ng/u1	0.00
73) Anthracene-d10	17.457	188	1641224	47.667	ng/u1	0.00
81) Pyrene-d10	19.698	212	2029779	50.189	ng/u1	0.00
92) Benzo(a)pyrene-d12	23.804	264	1982094	48.797	ng/u1	0.00
Target Compounds						
					Qvalue	
43) 1,1'-Biphenyl	13.416	154	30385	1.167	ng/u1	95
59) Diethylphthalate	15.398	149	38054	1.590	ng/u1	96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP092523\
Data File : BP017371.D
Acq On : 26 Sep 2023 20:26
Operator : MA/JU
Sample : 04450-15
Misc :
ALS Vial : 63 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BBBN0

Quant Time: Sep 27 01:55:41 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP092023.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Sep 26 04:52:29 2023
Response via : Initial Calibration




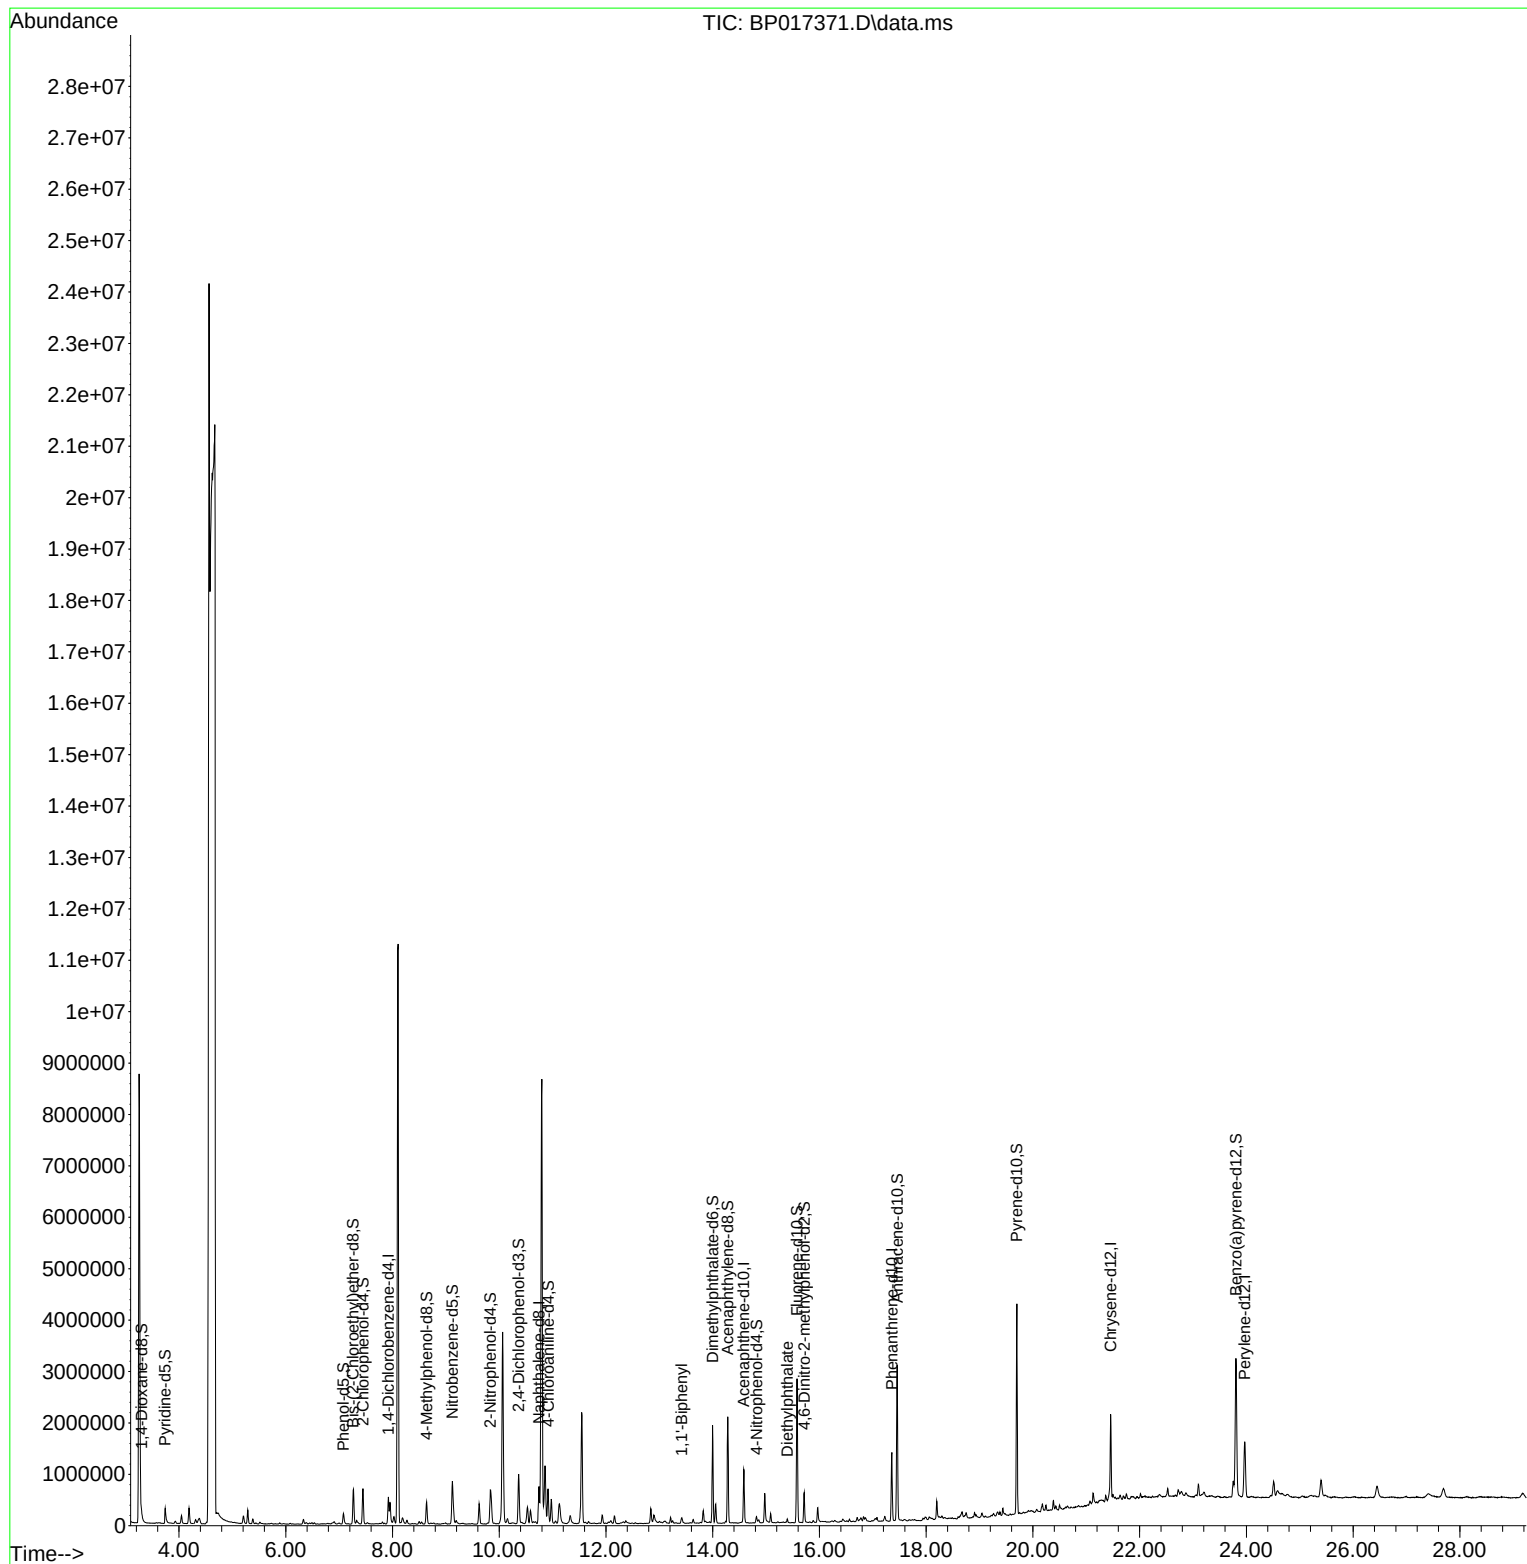


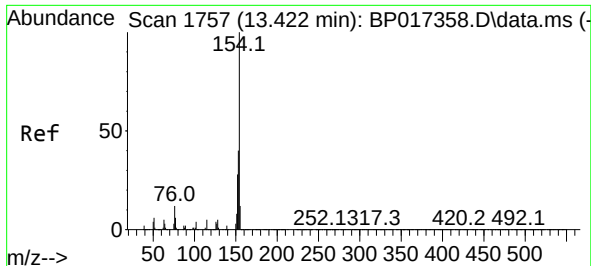

#43
1,1'-Biphenyl
Concen: 1.167 ng/ul
RT: 13.416 min Scan# 1756
Delta R.T. -0.000 min
Lab File: BP017371.D
Acq: 26 Sep 2023 20:26

Instrument :
BNA_P
ClientSampleId :
BBBN0

Tgt Ion:154	Resp:	30385
Ion Ratio	Lower	Upper
154	100	
153	43.5	31.5 47.3
76	13.1	11.0 16.6

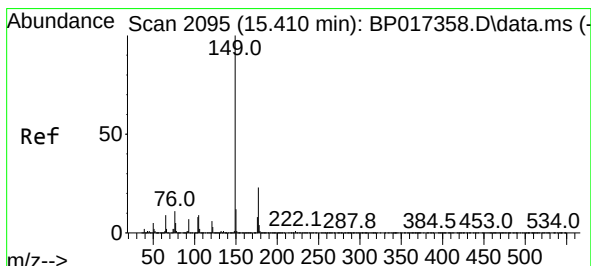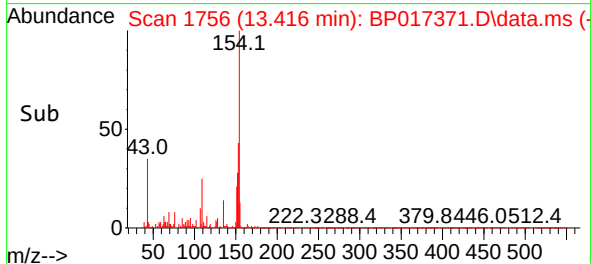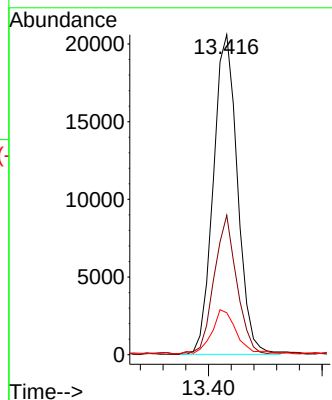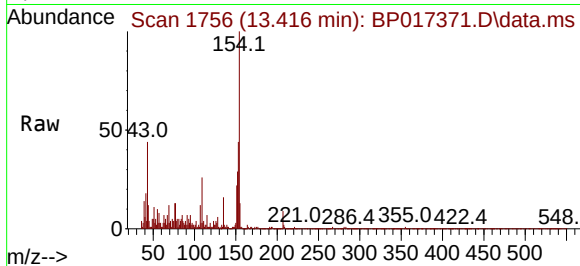

#59
Diethylphthalate
Concen: 1.590 ng/ul
RT: 15.398 min Scan# 2093
Delta R.T. -0.006 min
Lab File: BP017371.D
Acq: 26 Sep 2023 20:26

Tgt Ion:149	Resp:	38054
Ion Ratio	Lower	Upper
149	100	
177	23.6	17.0 25.6
150	11.1	9.8 14.6

