

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP092523\
 Data File : BP017311.D
 Acq On : 25 Sep 2023 09:28
 Operator : MA/JU
 Sample : PB155714BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK714

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP092023.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP017311.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.299	32	36	44	rVB	58322	79091	1.78%	0.179%
2	3.734	106	110	133	rBV	674586	1046035	23.52%	2.361%
3	4.046	159	163	167	rVB3	10029	15475	0.35%	0.035%
4	7.081	673	679	694	rBV	788957	1226020	27.57%	2.768%
5	7.269	705	711	720	rVB	644320	976709	21.96%	2.205%
6	7.445	734	741	751	rBV	797382	1270464	28.56%	2.868%
7	7.928	816	823	832	rVB	632745	963632	21.67%	2.175%
8	8.640	937	944	956	rBV	927729	1497370	33.67%	3.380%
9	9.128	1017	1027	1036	rBV	694604	1139184	25.61%	2.572%
10	9.839	1137	1148	1156	rBV	575510	936627	21.06%	2.114%
11	10.369	1230	1238	1254	rBV	883604	1514838	34.06%	3.420%
12	10.751	1293	1303	1311	rBV	839923	1389812	31.25%	3.137%
13	10.916	1322	1331	1344	rBV	896235	1555019	34.96%	3.510%
14	12.339	1568	1573	1579	rVB3	14715	26064	0.59%	0.059%
15	13.433	1754	1759	1765	rBV4	8900	14763	0.33%	0.033%
16	14.004	1850	1856	1869	rBV	1532734	2063378	46.39%	4.658%
17	14.292	1898	1905	1916	rBV	1686167	2486926	55.91%	5.614%
18	14.592	1949	1956	1966	rBV	1204568	1761337	39.60%	3.976%
19	14.822	1988	1995	2011	rBV	452996	875741	19.69%	1.977%
20	15.274	2069	2072	2076	rVB6	3451	4647	0.10%	0.010%
21	15.586	2119	2125	2140	rBV	2230265	3224839	72.51%	7.280%
22	15.721	2142	2148	2161	rVV	493073	689613	15.50%	1.557%
23	15.827	2161	2166	2172	rVB7	12347	21125	0.47%	0.048%
24	17.363	2421	2427	2438	rBV	1570459	2165255	48.68%	4.888%
25	17.463	2438	2444	2456	rBV	2653440	3622310	81.44%	8.177%
26	19.274	2749	2752	2757	rVB3	32301	42221	0.95%	0.095%
27	19.345	2761	2764	2768	rVB2	27521	34798	0.78%	0.079%
28	19.704	2820	2825	2835	rBV	3462281	4447736	100.00%	10.040%
29	21.468	3120	3125	3132	rBV	1867637	2410311	54.19%	5.441%
30	23.815	3518	3524	3535	rVB2	2139488	4314850	97.01%	9.740%
31	23.986	3547	3553	3564	rVB	1213866	2483005	55.83%	5.605%




Sum of corrected areas: 44299195

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP092523\
Data File : BP017311.D
Acq On : 25 Sep 2023 09:28
Operator : MA/JU
Sample : PB155714BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK714

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP092023.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

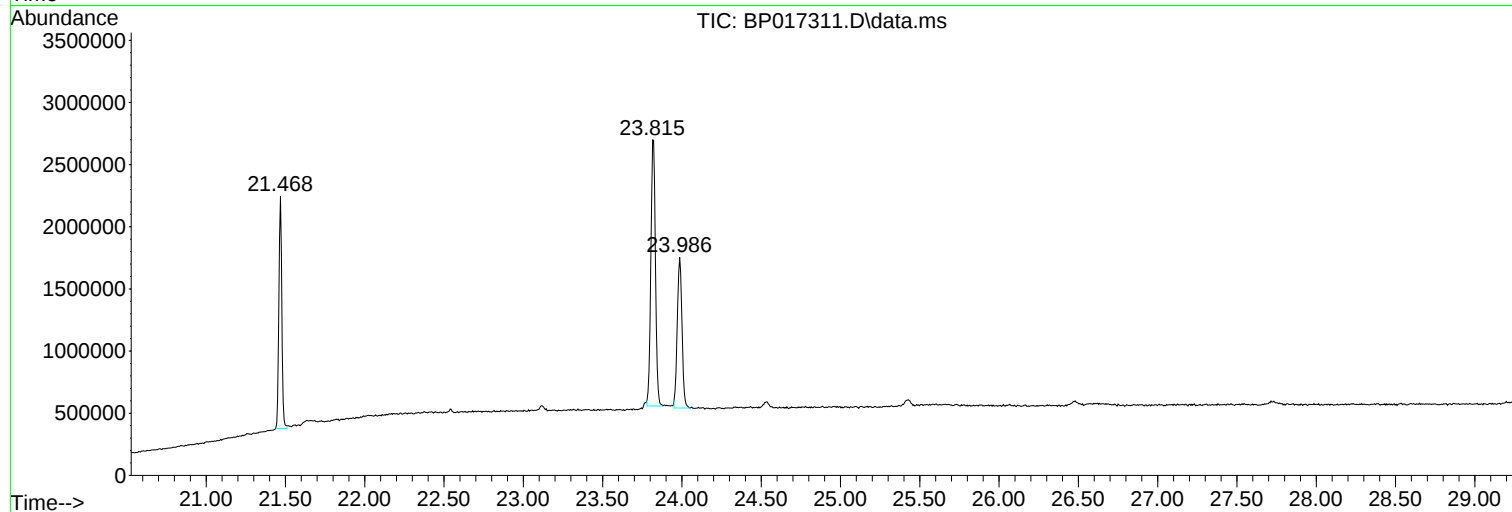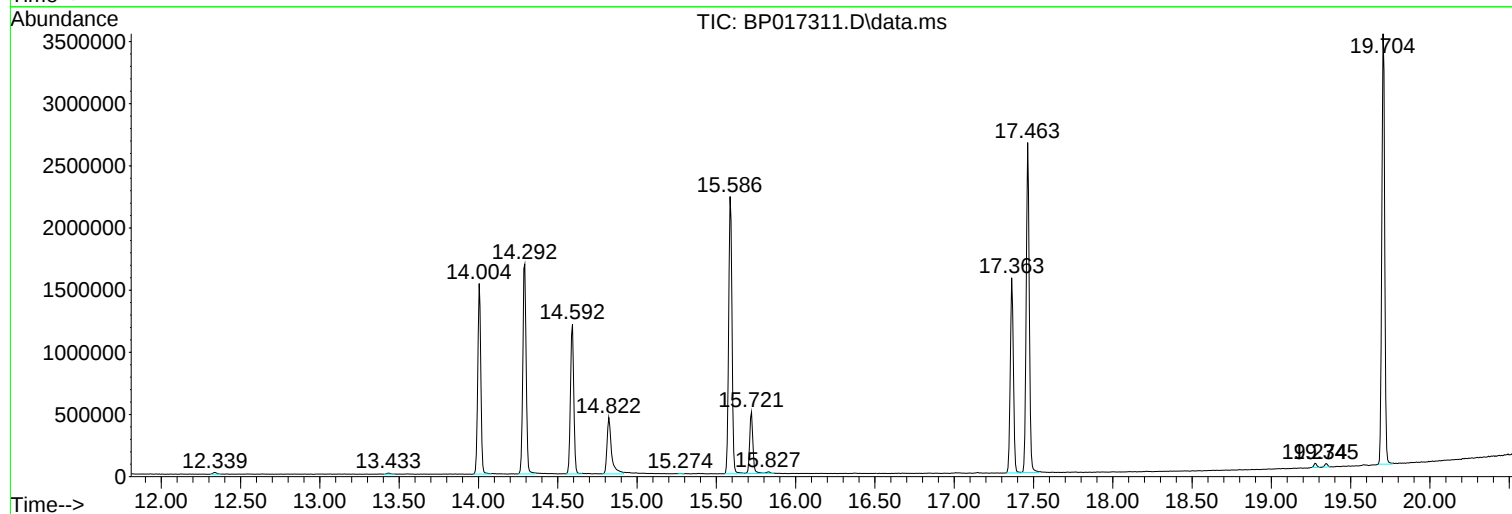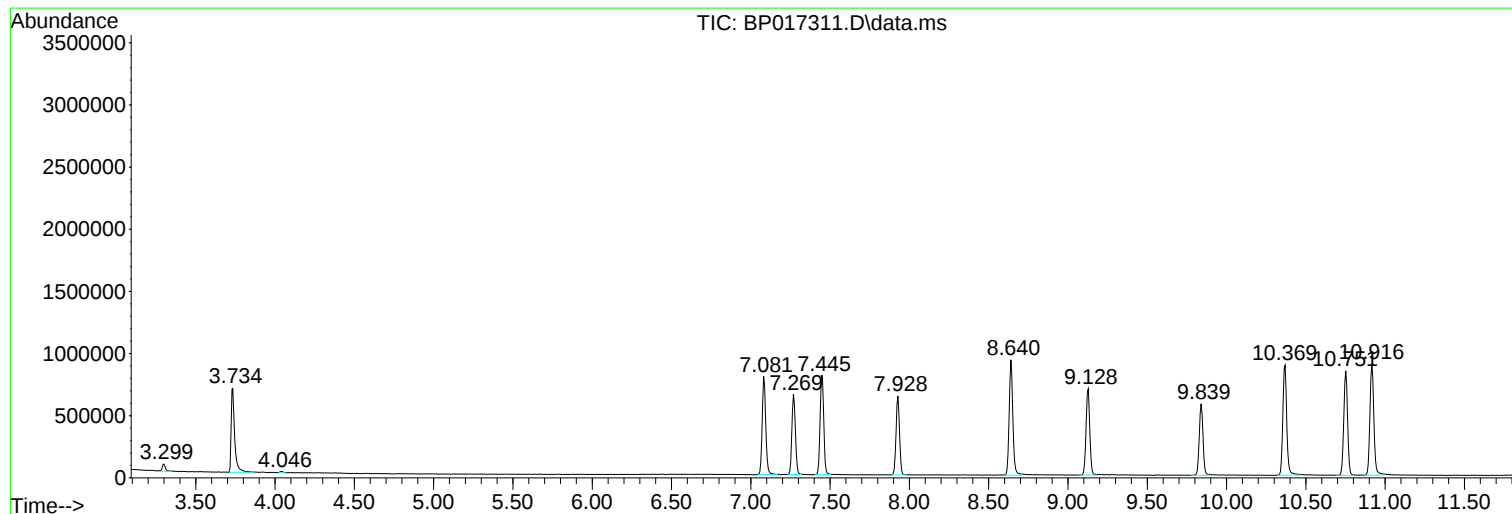

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP092523\
Data File : BP017311.D
Acq On : 25 Sep 2023 09:28
Operator : MA/JU
Sample : PB155714BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK714

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP092023.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP092523\
Data File : BP017311.D
Acq On : 25 Sep 2023 09:28
Operator : MA/JU
Sample : PB155714BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK714

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP092023.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------