

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP092523\
 Data File : BP017322.D
 Acq On : 25 Sep 2023 15:44
 Operator : MA/JU
 Sample : 04410-10
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BBJL8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP092023.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP017322.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.252	24	28	33	rBV	158244	198007	6.41%	0.731%
2	3.299	33	36	41	rVB	28605	35200	1.14%	0.130%
3	3.740	108	111	122	rBV	104583	161233	5.22%	0.596%
4	4.034	159	161	168	rVB2	10180	14660	0.47%	0.054%
5	4.564	245	251	266	rBV	2176944	3088481	100.00%	11.410%
6	5.746	448	452	456	rVB7	3889	6990	0.23%	0.026%
7	5.793	457	460	463	rBV5	2506	3248	0.11%	0.012%
8	5.864	469	472	477	rVB7	2987	4393	0.14%	0.016%
9	6.175	522	525	528	rVB5	3835	5535	0.18%	0.020%
10	6.340	548	553	558	rBV9	6945	9628	0.31%	0.036%
11	6.899	646	648	652	rVB5	4998	4790	0.16%	0.018%
12	6.952	653	657	660	rVB6	3420	4533	0.15%	0.017%
13	6.999	663	665	669	rVB5	3689	3834	0.12%	0.014%
14	7.087	674	680	688	rVV	143109	228059	7.38%	0.843%
15	7.140	688	689	693	rVB4	3357	3303	0.11%	0.012%
16	7.269	705	711	720	rVB	209894	325861	10.55%	1.204%
17	7.452	736	742	755	rBV	214744	357319	11.57%	1.320%
18	7.928	816	823	835	rBV	631867	981052	31.76%	3.624%
19	8.028	838	840	844	rVB5	2656	3394	0.11%	0.013%
20	8.405	899	904	908	rVB8	2361	4249	0.14%	0.016%
21	8.640	939	944	957	rBV	195920	334016	10.81%	1.234%
22	9.128	1020	1027	1034	rBV	225566	382028	12.37%	1.411%
23	9.257	1043	1049	1057	rBV9	7213	14344	0.46%	0.053%
24	9.840	1141	1148	1158	rBV	172722	290760	9.41%	1.074%
25	10.369	1230	1238	1248	rBV	263146	455228	14.74%	1.682%
26	10.751	1295	1303	1314	rBV	887309	1459692	47.26%	5.392%
27	10.916	1324	1331	1345	rBV	184736	332809	10.78%	1.229%
28	11.516	1428	1433	1434	rBV4	2584	3595	0.12%	0.013%
29	11.904	1494	1499	1503	rBV8	2027	3802	0.12%	0.014%
30	12.310	1564	1568	1569	rBV4	4795	5166	0.17%	0.019%
31	12.346	1572	1574	1579	rVB6	5281	5678	0.18%	0.021%
32	13.434	1749	1759	1768	rVV	69999	117621	3.81%	0.435%
33	13.551	1773	1779	1782	rBV8	3473	6665	0.22%	0.025%
34	13.769	1814	1816	1820	rVB5	2774	3603	0.12%	0.013%
35	14.004	1850	1856	1863	rBV	536505	716502	23.20%	2.647%
36	14.287	1896	1904	1918	rBV	589896	875627	28.35%	3.235%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP092523\
 Data File : BP017322.D
 Acq On : 25 Sep 2023 15:44
 Operator : MA/JU
 Sample : 04410-10
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BBJL8

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP092023.MA.M
 Title : SVOA CALIBRATION

37	14.592	1948	1956	1967	rBV	1338519	1970510	63.80%	7.280%
38	14.834	1989	1997	2010	rBV	58416	146020	4.73%	0.539%
39	15.381	2086	2090	2092	rBV5	3239	4730	0.15%	0.017%
40	15.587	2119	2125	2134	rBV	874439	1203254	38.96%	4.445%
41	15.657	2135	2137	2141	rVV5	10809	16265	0.53%	0.060%
42	15.722	2142	2148	2160	rVV	127740	202826	6.57%	0.749%
43	15.828	2163	2166	2169	rVB5	3198	4598	0.15%	0.017%
44	16.251	2235	2238	2242	rVV6	2158	3602	0.12%	0.013%
45	16.634	2301	2303	2307	rBV5	2430	3108	0.10%	0.011%
46	16.804	2328	2332	2334	rBV5	3592	5219	0.17%	0.019%
47	16.863	2339	2342	2348	rVB7	5983	9408	0.30%	0.035%
48	17.151	2385	2391	2394	rBV6	6908	10468	0.34%	0.039%
49	17.222	2397	2403	2404	rBV6	4520	6787	0.22%	0.025%
50	17.363	2420	2427	2436	rBV	1732739	2411377	78.08%	8.908%
51	17.463	2438	2444	2458	rVB	1053415	1499971	48.57%	5.541%
52	17.981	2529	2532	2536	rBV6	8082	9964	0.32%	0.037%
53	18.204	2565	2570	2578	rBV	79162	125559	4.07%	0.464%
54	18.604	2636	2638	2642	rBV5	9229	9287	0.30%	0.034%
55	19.122	2723	2726	2730	rVB5	22132	26562	0.86%	0.098%
56	19.439	2777	2780	2783	rBV4	27864	35002	1.13%	0.129%
57	19.575	2801	2803	2806	rBV2	15210	16084	0.52%	0.059%
58	19.704	2819	2825	2833	rBV	1470316	1889171	61.17%	6.979%
59	21.463	3120	3124	3132	rBV	1925003	2560193	82.89%	9.458%
60	23.816	3518	3524	3534	rVB2	895649	1789635	57.95%	6.611%
61	23.980	3546	3552	3563	rVB	1305045	2658767	86.09%	9.822%




Sum of corrected areas: 27069272

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP092523\
Data File : BP017322.D
Acq On : 25 Sep 2023 15:44
Operator : MA/JU
Sample : 04410-10
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BBJL8

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP092023.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

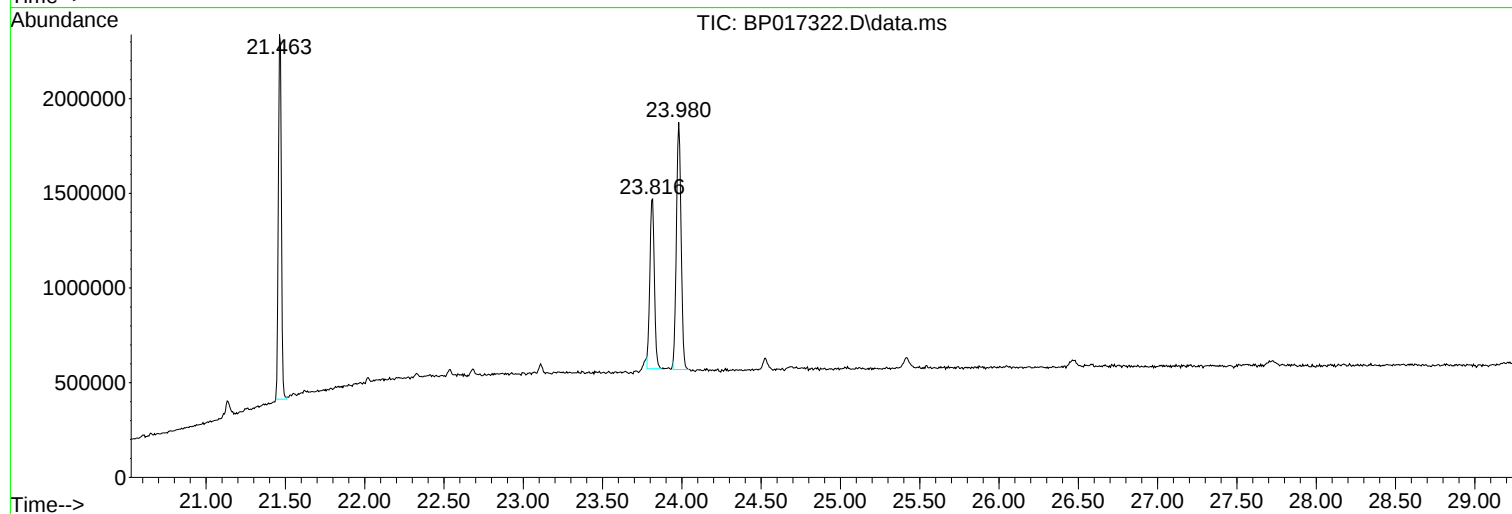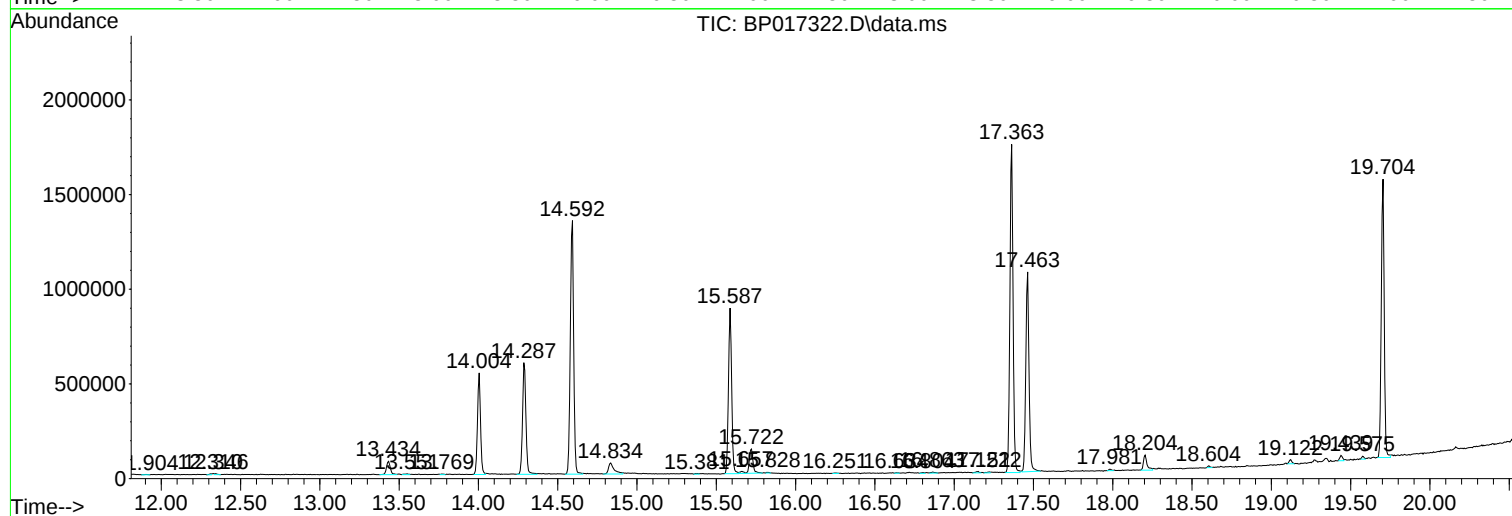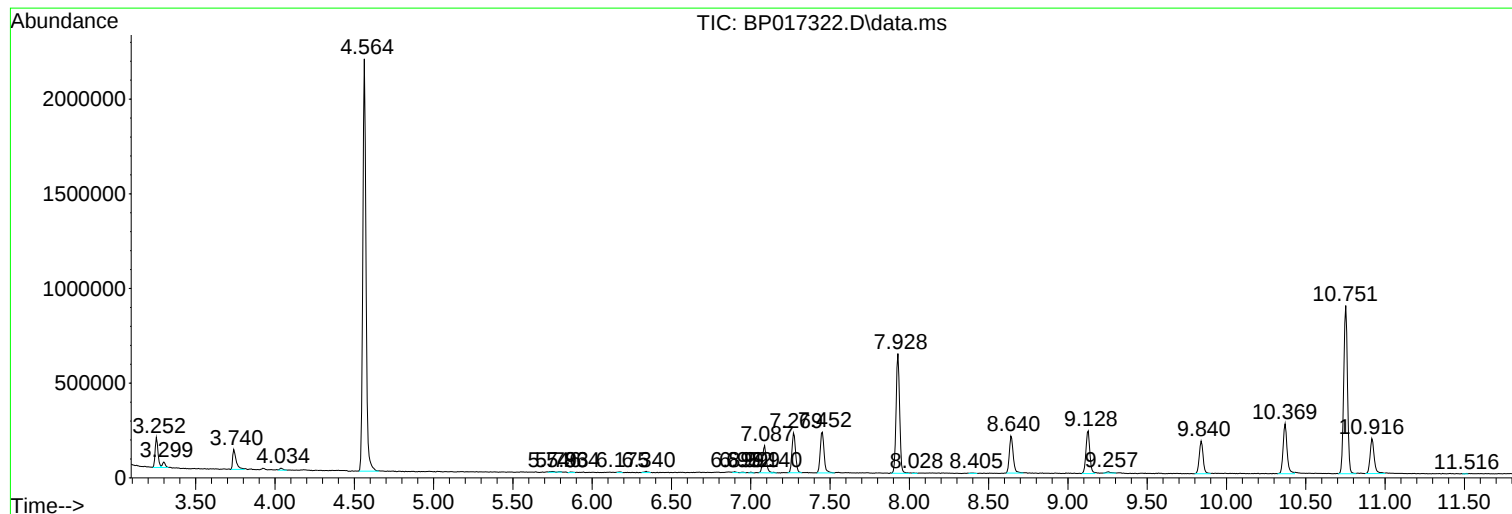

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP092523\
Data File : BP017322.D
Acq On : 25 Sep 2023 15:44
Operator : MA/JU
Sample : 04410-10
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BBJL8










Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP092023.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Tetrachloroethylene Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
4.564	62.96 ng/ul	3088480	1,4-Dichlorobenzene-d4	7.928

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Tetrachloroethylene	164	C2Cl4	000127-18-4	98
2			Tetrachloroethylene	164	C2Cl4	000127-18-4	98
3			Tetrachloroethylene	164	C2Cl4	000127-18-4	97
4			Tetrachloroethylene	164	C2Cl4	000127-18-4	72
5			Pyrimidine, 5-fluoro-2,4-dichloro-	166	C4HC12FN2	002927-71-1	38

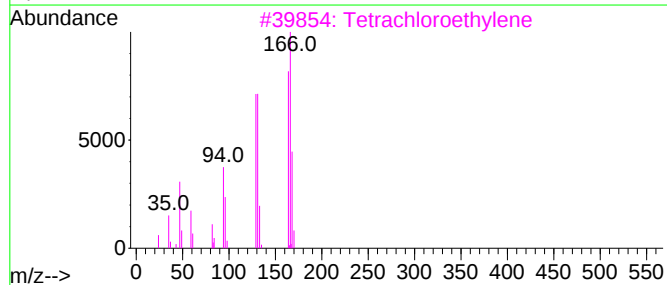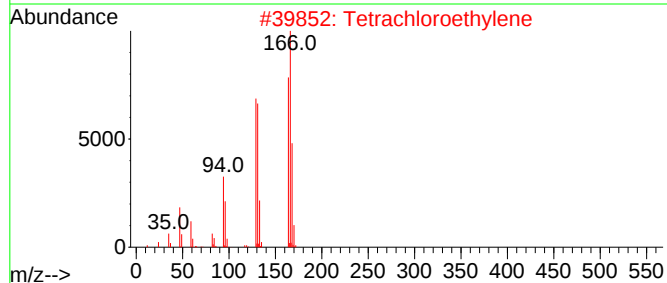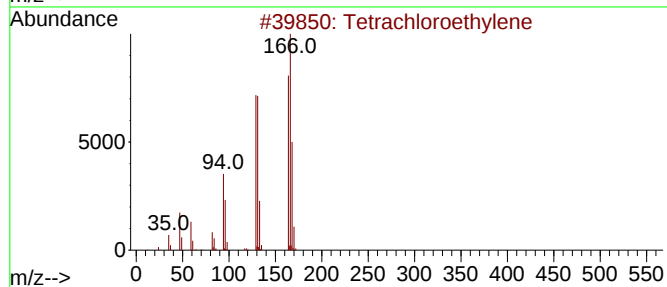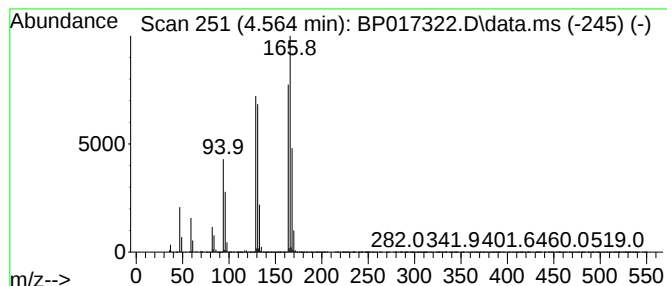

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP092523\
Data File : BP017322.D
Acq On : 25 Sep 2023 15:44
Operator : MA/JU
Sample : 04410-10
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BBJL8

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP092023.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Tetrachloroethy...	4.564	63.0	ng/ul	3088480	1	7.928	981052	20.0