

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP092523\
 Data File : BP017326.D
 Acq On : 25 Sep 2023 18:09
 Operator : MA/JU
 Sample : PB155714BL
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK714

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP092023.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP017326.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.293	32	35	42	rVB	62887	78733	1.63%	0.157%
2	3.728	105	109	123	rBV	756065	1095651	22.70%	2.191%
3	4.034	158	161	167	rVB2	9496	13053	0.27%	0.026%
4	7.081	672	679	693	rBV	834705	1318845	27.33%	2.638%
5	7.264	704	710	722	rVB	687528	1089855	22.58%	2.180%
6	7.446	734	741	749	rBV	878098	1378125	28.56%	2.756%
7	7.922	815	822	830	rBV	686662	1042256	21.60%	2.085%
8	8.640	936	944	960	rBV	1015248	1667633	34.56%	3.335%
9	9.122	1019	1026	1041	rBV	806673	1300486	26.95%	2.601%
10	9.834	1140	1147	1160	rBV	661146	1092647	22.64%	2.185%
11	10.363	1230	1237	1253	rBV	1020661	1713870	35.52%	3.428%
12	10.752	1295	1303	1312	rBV	916294	1553211	32.19%	3.106%
13	10.916	1323	1331	1342	rBV	1022242	1753801	36.34%	3.508%
14	12.340	1567	1573	1579	rBV	16024	26791	0.56%	0.054%
15	13.428	1754	1758	1764	rBV4	14208	25336	0.53%	0.051%
16	13.551	1775	1779	1783	rBV7	4101	7251	0.15%	0.015%
17	13.816	1818	1824	1829	rBV9	3838	6834	0.14%	0.014%
18	14.004	1850	1856	1868	rBV	1929624	2564324	53.14%	5.129%
19	14.293	1896	1905	1915	rBV	2036637	2985422	61.87%	5.971%
20	14.593	1949	1956	1965	rBV	1398882	2066195	42.82%	4.132%
21	14.822	1988	1995	2015	rBV	566454	1058956	21.94%	2.118%
22	15.275	2068	2072	2074	rBV5	6142	8317	0.17%	0.017%
23	15.387	2086	2091	2095	rBV8	3164	5364	0.11%	0.011%
24	15.587	2118	2125	2138	rBV	2654384	3788207	78.50%	7.576%
25	15.722	2141	2148	2160	rVV	608512	849340	17.60%	1.699%
26	15.822	2163	2165	2172	rVB5	12810	20472	0.42%	0.041%
27	16.645	2302	2305	2312	rVB10	2720	5255	0.11%	0.011%
28	17.028	2367	2370	2374	rBV6	4071	5816	0.12%	0.012%
29	17.157	2387	2392	2396	rBV6	3929	6939	0.14%	0.014%
30	17.363	2421	2427	2437	rBV	1771965	2456622	50.91%	4.913%
31	17.463	2438	2444	2461	rVV2	2943762	4125541	85.49%	8.251%
32	19.281	2748	2753	2757	rBV3	35704	54372	1.13%	0.109%
33	19.345	2761	2764	2768	rVB	29713	36261	0.75%	0.073%
34	19.710	2820	2826	2833	rBV	3665284	4825686	100.00%	9.651%
35	21.469	3120	3125	3133	rBV	2091995	2609065	54.07%	5.218%
36	23.821	3518	3525	3538	rVB2	2314685	4728586	97.99%	9.457%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP092523\
Data File : BP017326.D
Acq On : 25 Sep 2023 18:09
Operator : MA/JU
Sample : PB155714BL
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK714

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP092023.MA.M
Title : SVOA CALIBRATION

37	23.986	3547	3553	3565	rVB	1239083	2634561	54.59%	5.269%
----	--------	------	------	------	-----	---------	---------	--------	--------




Sum of corrected areas: 49999679

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP092523\
Data File : BP017326.D
Acq On : 25 Sep 2023 18:09
Operator : MA/JU
Sample : PB155714BL
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK714

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP092023.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

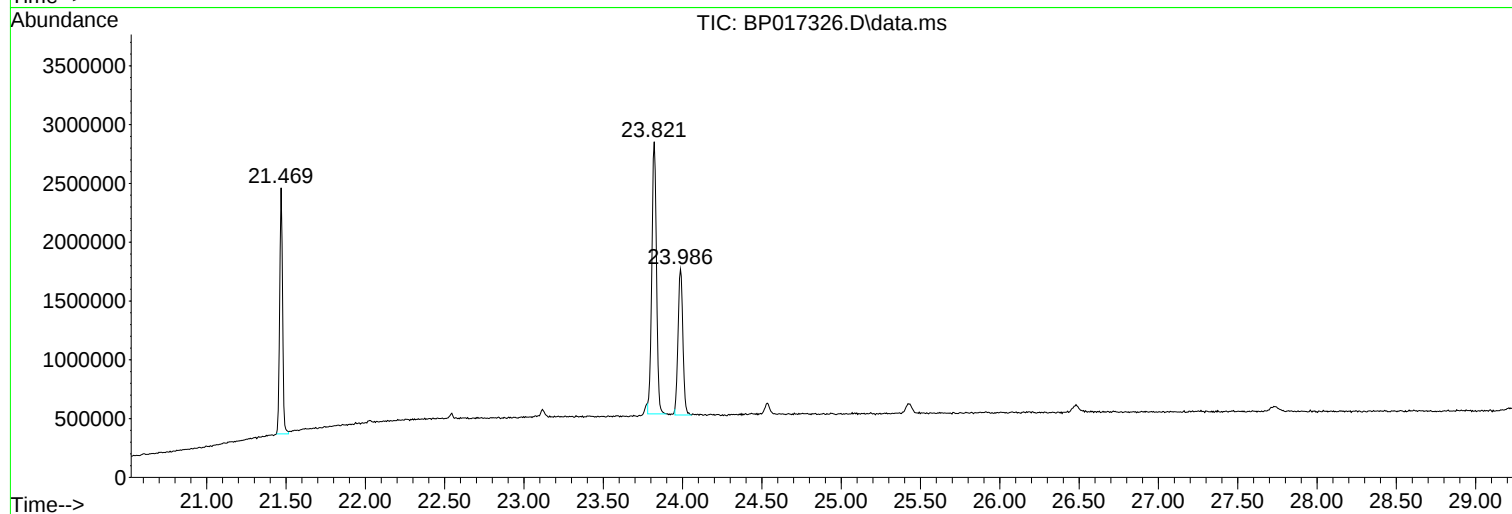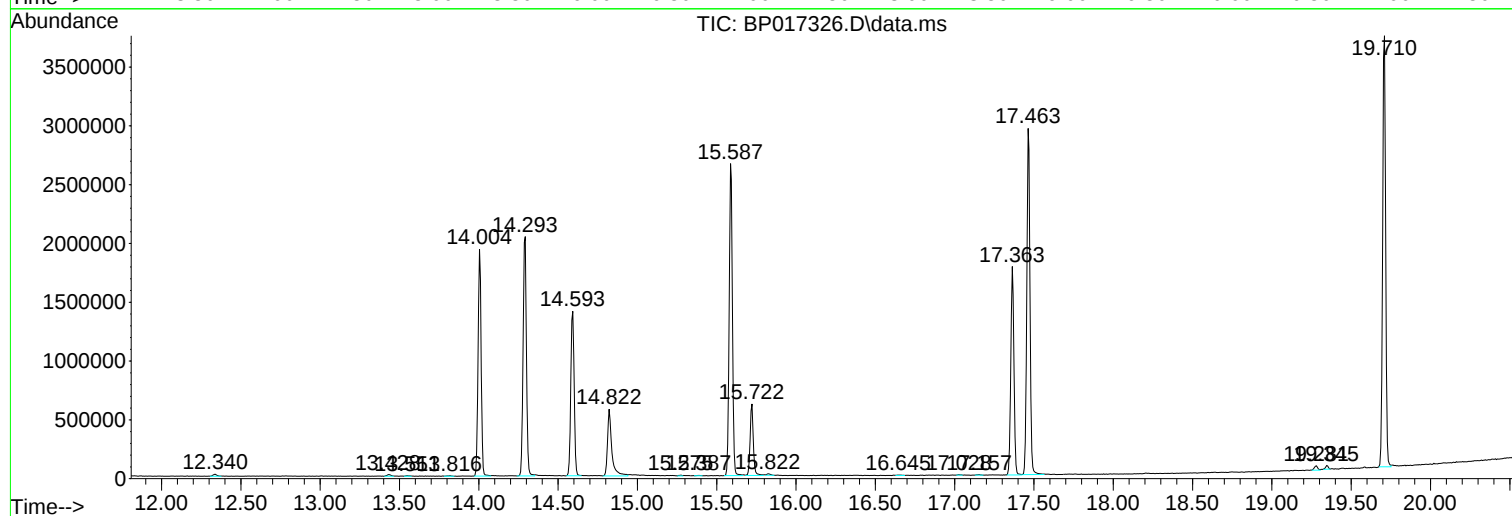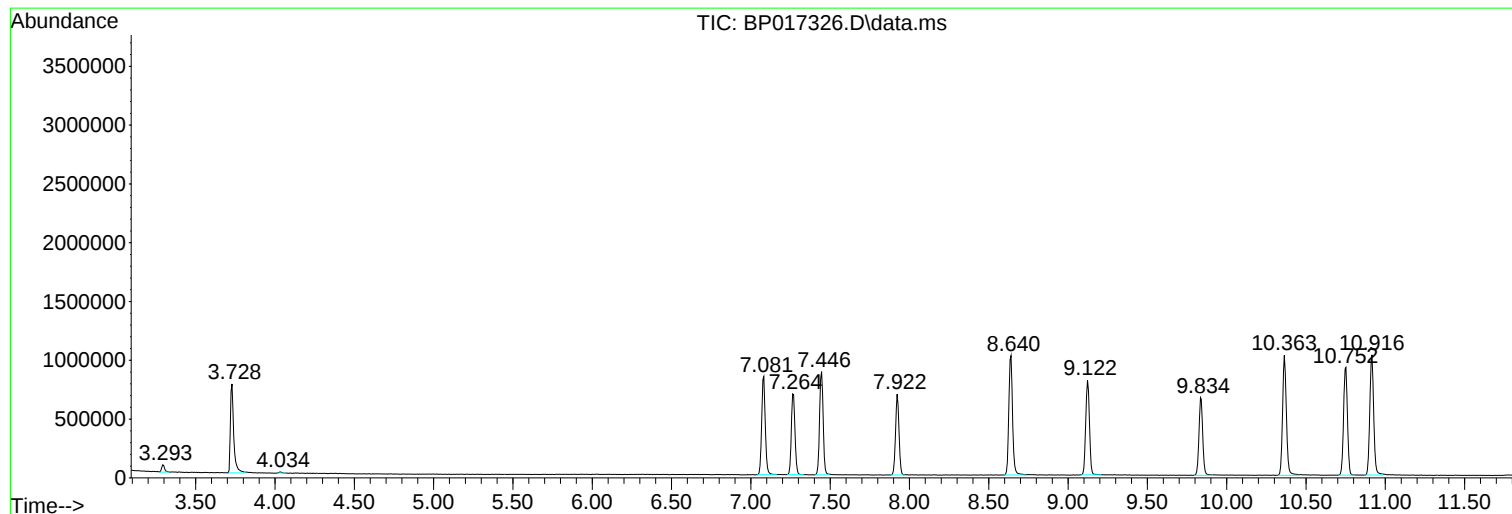

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP092523\
Data File : BP017326.D
Acq On : 25 Sep 2023 18:09
Operator : MA/JU
Sample : PB155714BL
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK714

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP092023.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP092523\
Data File : BP017326.D
Acq On : 25 Sep 2023 18:09
Operator : MA/JU
Sample : PB155714BL
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK714

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP092023.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------