

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP092523\
 Data File : BP017330.D
 Acq On : 25 Sep 2023 20:26
 Operator : MA/JU
 Sample : 04450-01
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BBJ39

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP092023.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP017330.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.252	23	28	33	rBV	475518	598074	6.61%	0.763%
2	3.299	33	36	40	rVB	53331	68591	0.76%	0.088%
3	3.734	107	110	125	rBV	351842	524755	5.80%	0.670%
4	3.928	138	143	152	rVB	44236	71352	0.79%	0.091%
5	4.040	159	162	166	rVB2	10385	13570	0.15%	0.017%
6	4.181	183	186	192	rVB3	14856	24196	0.27%	0.031%
7	4.428	225	228	236	rVB5	15944	26105	0.29%	0.033%
8	4.564	245	251	273	rVB	3803443	5594539	61.82%	7.141%
9	4.975	317	321	325	rBV2	7075	9885	0.11%	0.013%
10	5.558	417	420	426	rVB6	6458	10074	0.11%	0.013%
11	6.169	519	524	530	rVB9	5292	11750	0.13%	0.015%
12	6.334	546	552	556	rBV	15002	22505	0.25%	0.029%
13	6.893	644	647	654	rVB7	8416	14770	0.16%	0.019%
14	7.087	673	680	690	rBV	208760	349005	3.86%	0.445%
15	7.269	703	711	721	rBV	991370	1497511	16.55%	1.911%
16	7.452	735	742	754	rBV	872859	1415322	15.64%	1.807%
17	7.928	816	823	833	rBV	771883	1204063	13.31%	1.537%
18	8.640	937	944	953	rBV	663662	1057914	11.69%	1.350%
19	9.128	1019	1027	1035	rBV	1165863	1887947	20.86%	2.410%
20	9.287	1050	1054	1058	rBV6	5340	9115	0.10%	0.012%
21	9.840	1141	1148	1161	rBV	945297	1513960	16.73%	1.932%
22	10.363	1230	1237	1253	rBV	1321597	2254145	24.91%	2.877%
23	10.510	1259	1262	1269	rVB8	4278	9113	0.10%	0.012%
24	10.752	1296	1303	1310	rBV	1122538	1832904	20.25%	2.340%
25	10.916	1322	1331	1342	rBV	1169617	1983468	21.92%	2.532%
26	11.575	1438	1443	1450	rVB3	15241	28646	0.32%	0.037%
27	12.334	1566	1572	1578	rVB2	23764	39364	0.43%	0.050%
28	13.428	1752	1758	1765	rBV2	28239	49792	0.55%	0.064%
29	14.004	1849	1856	1866	rBV	2962845	3927667	43.40%	5.013%
30	14.204	1885	1890	1896	rBV10	5339	12870	0.14%	0.016%
31	14.287	1896	1904	1915	rBV	3176581	4589017	50.71%	5.857%
32	14.587	1948	1955	1962	rBV	1794650	2551430	28.19%	3.257%
33	14.822	1989	1995	2006	rBV	130143	273270	3.02%	0.349%
34	14.981	2018	2022	2028	rVV9	7195	17106	0.19%	0.022%
35	15.398	2092	2093	2101	rVB8	6747	11028	0.12%	0.014%
36	15.587	2118	2125	2132	rBV	4283226	6039683	66.74%	7.709%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP092523\
 Data File : BP017330.D
 Acq On : 25 Sep 2023 20:26
 Operator : MA/JU
 Sample : 04450-01
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BBJ39

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP092023.MA.M
 Title : SVOA CALIBRATION

37	15.657	2132	2137	2141	rVV	89741	143906	1.59%	0.184%
38	15.716	2141	2147	2158	rVV	1309231	1757636	19.42%	2.243%
39	15.822	2161	2165	2170	rVB	21357	35227	0.39%	0.045%
40	16.122	2211	2216	2222	rBV	108791	152262	1.68%	0.194%
41	16.245	2233	2237	2243	rVB9	5942	10352	0.11%	0.013%
42	16.457	2268	2273	2277	rBV	13294	19830	0.22%	0.025%
43	16.640	2300	2304	2310	rBV	58247	82505	0.91%	0.105%
44	16.863	2338	2342	2346	rBV6	8676	13475	0.15%	0.017%
45	17.022	2365	2369	2375	rBV9	7796	16424	0.18%	0.021%
46	17.145	2388	2390	2395	rVB5	6985	10298	0.11%	0.013%
47	17.357	2420	2426	2437	rBV	2272952	3230605	35.70%	4.124%
48	17.463	2437	2444	2461	rVV	5116053	7148590	78.99%	9.124%
49	17.751	2491	2493	2498	rBV4	7102	9682	0.11%	0.012%
50	18.204	2565	2570	2576	rBV	201871	304936	3.37%	0.389%
51	19.275	2748	2752	2757	rBV3	69958	97602	1.08%	0.125%
52	19.339	2760	2763	2768	rVB	61018	84771	0.94%	0.108%
53	19.439	2777	2780	2786	rBV2	83344	107002	1.18%	0.137%
54	19.704	2819	2825	2833	rBV	6793500	8938240	98.77%	11.409%
55	21.133	3065	3068	3075	rBV3	133616	209900	2.32%	0.268%
56	21.463	3119	3124	3132	rBV	2823110	3624646	40.05%	4.626%
57	23.816	3517	3524	3536	rVB2	4494997	9049505	100.00%	11.551%
58	23.980	3545	3552	3562	rVB	1831683	3753574	41.48%	4.791%




Sum of corrected areas: 78345474

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP092523\
Data File : BP017330.D
Acq On : 25 Sep 2023 20:26
Operator : MA/JU
Sample : 04450-01
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BBJ39

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP092023.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

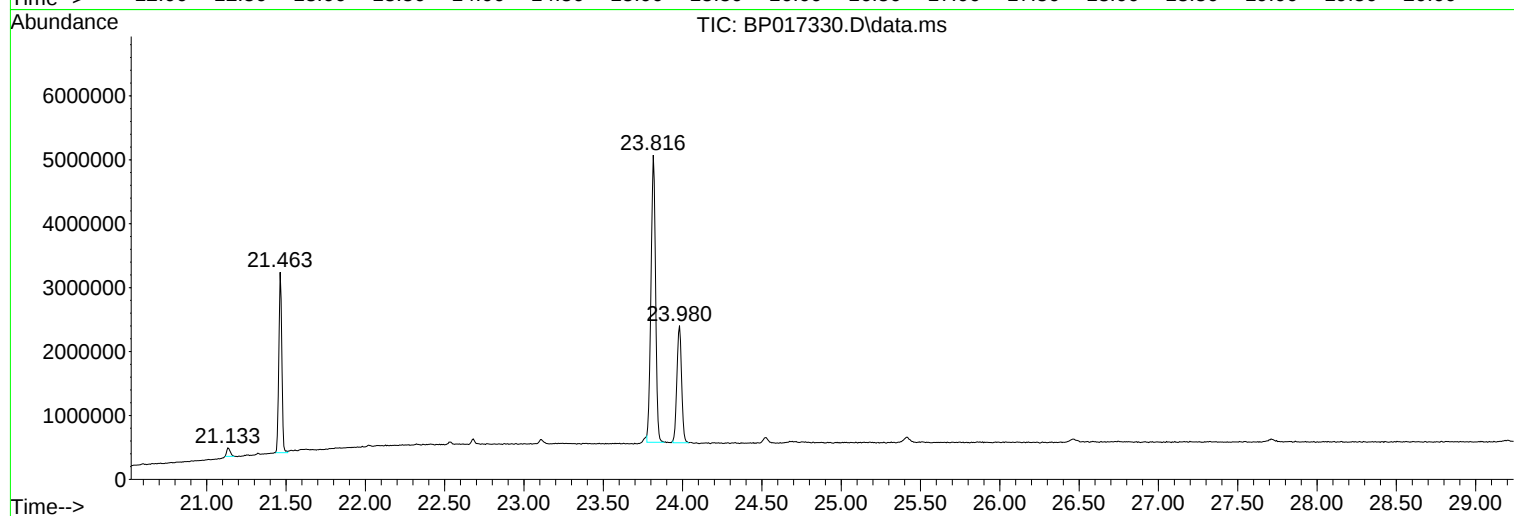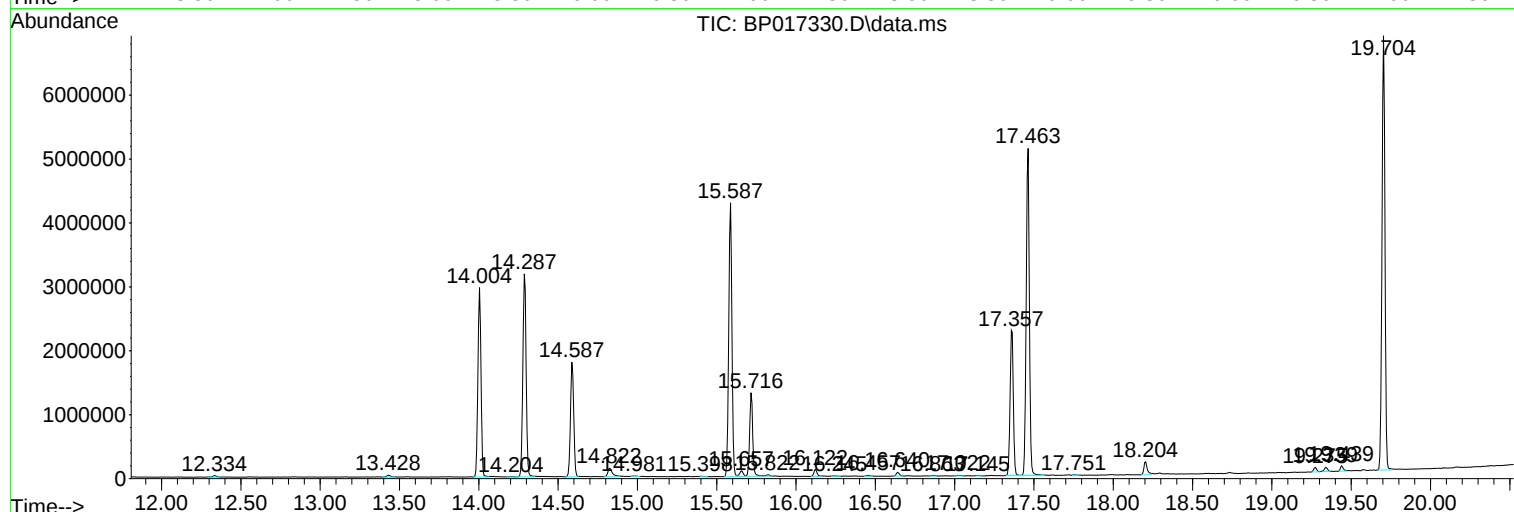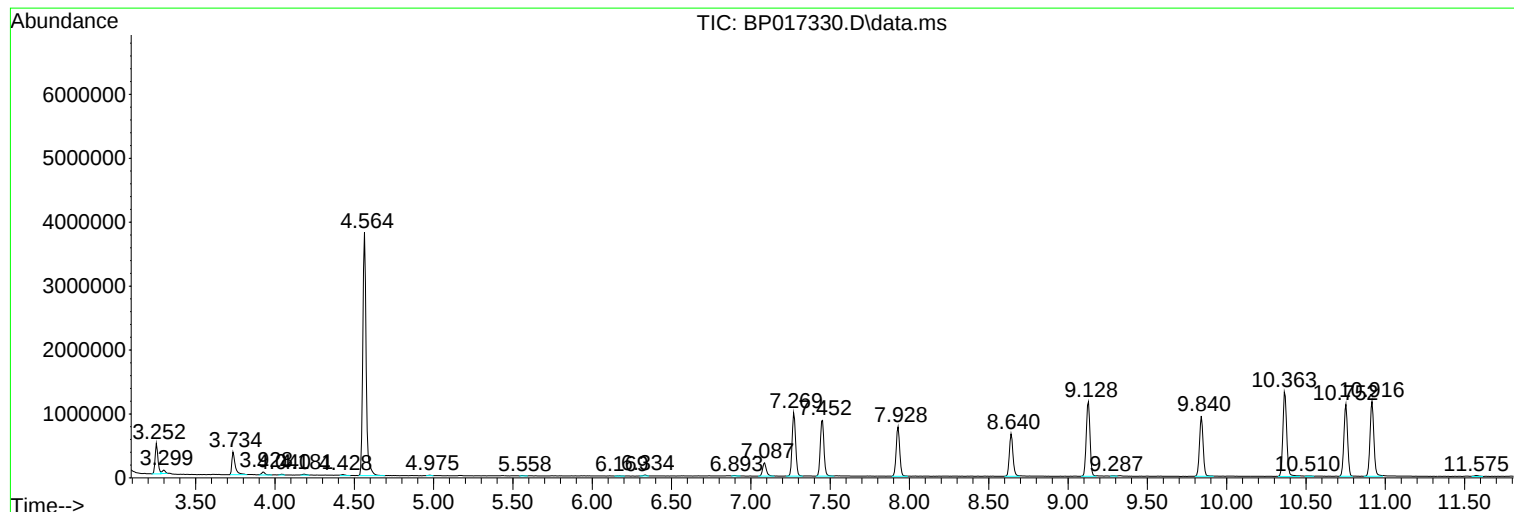

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP092523\
Data File : BP017330.D
Acq On : 25 Sep 2023 20:26
Operator : MA/JU
Sample : 04450-01
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BBJ39










Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP092023.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Tetrachloroethylene Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
4.564	92.93 ng/ul	5594540	1,4-Dichlorobenzene-d4	7.928

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Tetrachloroethylene	164	C2Cl4	000127-18-4	98
2			Tetrachloroethylene	164	C2Cl4	000127-18-4	98
3			Tetrachloroethylene	164	C2Cl4	000127-18-4	97
4			Tetrachloroethylene	164	C2Cl4	000127-18-4	96
5			Pyrimidine, 5-fluoro-2,4-dichloro-	166	C4HC12FN2	002927-71-1	38

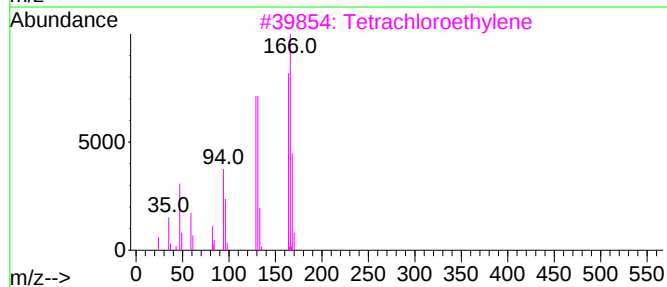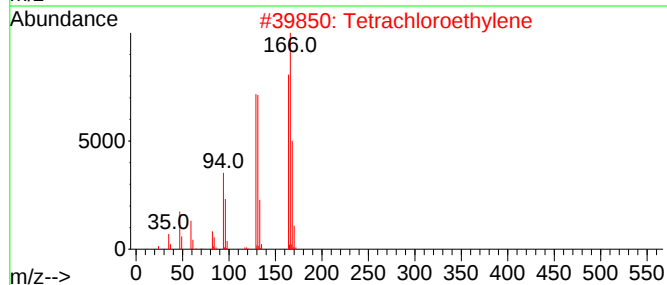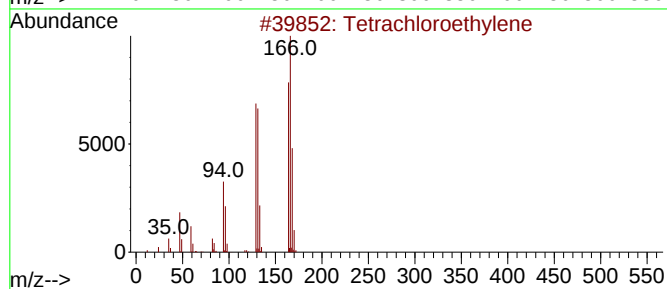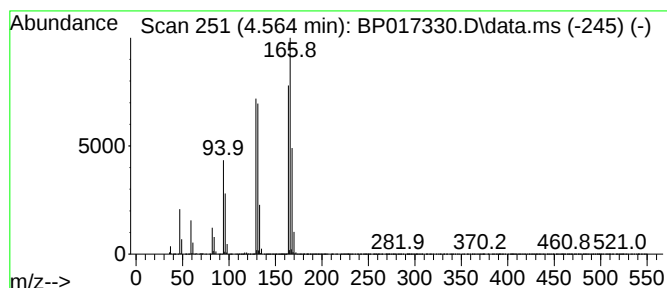

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP092523\
Data File : BP017330.D
Acq On : 25 Sep 2023 20:26
Operator : MA/JU
Sample : 04450-01
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BBJ39

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP092023.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Tetrachloroethy...	4.564	92.9	ng/ul	5594540	1	7.928	1204060	20.0