

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP092523\
 Data File : BP017338.D
 Acq On : 26 Sep 2023 00:58
 Operator : MA/JU
 Sample : 04472-17
 Misc :
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 EZYM6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP092023.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP017338.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.299	32	36	40	rVB	27539	35911	1.17%	0.113%
2	3.746	108	112	125	rBV	38249	73009	2.39%	0.229%
3	3.840	126	128	134	rVV2	15106	19235	0.63%	0.060%
4	3.922	137	142	149	rVB	83619	117107	3.83%	0.367%
5	4.040	160	162	164	rVB3	9205	7784	0.25%	0.024%
6	4.181	182	186	193	rVB4	30266	44663	1.46%	0.140%
7	4.428	224	228	235	rVB3	26673	39920	1.30%	0.125%
8	4.858	298	301	306	rBV6	4274	6222	0.20%	0.020%
9	4.975	316	321	325	rBV	49942	67793	2.21%	0.213%
10	5.428	396	398	403	rVB2	5085	7050	0.23%	0.022%
11	5.540	411	417	425	rBV3	20477	45544	1.49%	0.143%
12	6.334	546	552	558	rBV	23709	37099	1.21%	0.116%
13	6.546	584	588	591	rBV6	2255	4170	0.14%	0.013%
14	6.599	595	597	601	rBV5	2785	3983	0.13%	0.012%
15	6.893	644	647	653	rVB4	14529	22777	0.74%	0.071%
16	7.081	673	679	691	rBV	338110	564878	18.46%	1.771%
17	7.269	704	711	721	rBV	400979	603462	19.72%	1.892%
18	7.358	723	726	730	rVB6	3713	6149	0.20%	0.019%
19	7.446	733	741	749	rBV	288879	465429	15.21%	1.459%
20	7.540	754	757	760	rVV5	6727	8950	0.29%	0.028%
21	7.593	764	766	771	rVB6	4100	5363	0.18%	0.017%
22	7.734	785	790	795	rBV3	7832	14026	0.46%	0.044%
23	7.928	815	823	834	rBV	597527	942972	30.81%	2.956%
24	8.640	936	944	955	rBV	379174	615792	20.12%	1.931%
25	8.716	955	957	960	rVB4	4416	4861	0.16%	0.015%
26	8.775	960	967	976	rBV	101749	170281	5.56%	0.534%
27	9.122	1019	1026	1034	rBV	431415	693669	22.66%	2.175%
28	9.234	1043	1045	1051	rVB7	6334	9955	0.33%	0.031%
29	9.328	1056	1061	1065	rVB5	5963	9681	0.32%	0.030%
30	9.840	1138	1148	1162	rBV	182774	316490	10.34%	0.992%
31	9.987	1165	1173	1177	rBV4	12812	27805	0.91%	0.087%
32	10.022	1177	1179	1185	rVB7	5450	9132	0.30%	0.029%
33	10.204	1204	1210	1216	rVB5	10276	18020	0.59%	0.056%
34	10.363	1229	1237	1246	rBV	290735	500154	16.34%	1.568%
35	10.746	1295	1302	1311	rVV	850308	1410761	46.09%	4.423%
36	10.822	1311	1315	1318	rVB5	4138	6129	0.20%	0.019%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP092523\
 Data File : BP017338.D
 Acq On : 26 Sep 2023 00:58
 Operator : MA/JU
 Sample : 04472-17
 Misc :
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 EZYM6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP092023.MA.M
 Title : SVOA CALIBRATION

37	10.916	1323	1331	1346	rBV	458057	806467	26.35%	2.528%
38	11.310	1393	1398	1399	rBV5	3561	5122	0.17%	0.016%
39	11.510	1427	1432	1435	rBV7	5224	8229	0.27%	0.026%
40	11.581	1438	1444	1447	rVV6	6140	11444	0.37%	0.036%

41	11.728	1466	1469	1472	rBV4	3512	5542	0.18%	0.017%
42	11.793	1476	1480	1481	rVV4	3970	5819	0.19%	0.018%
43	11.816	1481	1484	1488	rVB5	5174	8907	0.29%	0.028%
44	12.098	1524	1532	1535	rBV9	4613	9737	0.32%	0.031%
45	12.234	1552	1555	1558	rBV5	2676	4187	0.14%	0.013%

46	12.334	1567	1572	1580	rVB3	10159	19497	0.64%	0.061%
47	12.781	1643	1648	1649	rBV4	3638	5763	0.19%	0.018%
48	12.846	1655	1659	1661	rVB5	2627	3600	0.12%	0.011%
49	12.904	1664	1669	1670	rBV5	3841	5309	0.17%	0.017%
50	13.040	1688	1692	1697	rBV7	2764	3967	0.13%	0.012%

51	13.157	1707	1712	1717	rBV7	6463	9983	0.33%	0.031%
52	13.340	1739	1743	1747	rBV6	6545	8673	0.28%	0.027%
53	13.428	1752	1758	1766	rVV2	43733	73598	2.40%	0.231%
54	13.504	1766	1771	1773	rVV6	2380	4595	0.15%	0.014%
55	13.545	1775	1778	1782	rVB5	2632	3553	0.12%	0.011%

56	13.775	1812	1817	1820	rBV6	3903	6888	0.23%	0.022%
57	13.816	1822	1824	1828	rVB5	4415	4897	0.16%	0.015%
58	13.998	1849	1855	1863	rBV	1034986	1423058	46.49%	4.461%
59	14.204	1886	1890	1893	rBV6	4107	6428	0.21%	0.020%
60	14.287	1897	1904	1915	rBV	1154663	1640905	53.61%	5.144%

61	14.416	1922	1926	1933	rVB8	11332	18739	0.61%	0.059%
62	14.587	1948	1955	1970	rBV	1324446	1896657	61.97%	5.946%
63	14.828	1990	1996	2009	rBV	59389	145738	4.76%	0.457%
64	14.969	2016	2020	2021	rBV4	4832	5837	0.19%	0.018%
65	14.987	2021	2023	2027	rVV5	7843	13939	0.46%	0.044%

66	15.028	2027	2030	2037	rVB8	18134	28909	0.94%	0.091%
67	15.328	2076	2081	2084	rBV4	7757	11003	0.36%	0.034%
68	15.369	2084	2088	2091	rVV3	14170	18974	0.62%	0.059%
69	15.404	2091	2094	2096	rVB3	3738	4366	0.14%	0.014%
70	15.581	2116	2124	2136	rBV	1528437	2225310	72.71%	6.976%

71	15.716	2142	2147	2153	rBV2	56387	78397	2.56%	0.246%
72	15.822	2161	2165	2169	rVB7	6472	8913	0.29%	0.028%
73	16.004	2194	2196	2201	rVB6	3617	4858	0.16%	0.015%
74	16.104	2209	2213	2217	rBV7	2751	5811	0.19%	0.018%
75	16.239	2232	2236	2241	rBV2	23324	36240	1.18%	0.114%

76	16.581	2289	2294	2295	rBV5	3244	4388	0.14%	0.014%
----	--------	------	------	------	------	------	------	-------	--------

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP092523\
 Data File : BP017338.D
 Acq On : 26 Sep 2023 00:58
 Operator : MA/JU
 Sample : 04472-17
 Misc :
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 EZYM6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP092023.MA.M
 Title : SVOA CALIBRATION

77	16.710	2313	2316	2320	rVB6	4309	5132	0.17%	0.016%
78	16.881	2340	2345	2352	rVB2	26680	38601	1.26%	0.121%
79	17.039	2368	2372	2376	rVB2	20263	24088	0.79%	0.076%
80	17.081	2376	2379	2383	rVB4	10094	13098	0.43%	0.041%
81	17.234	2399	2405	2410	rBV10	6019	13813	0.45%	0.043%
82	17.357	2420	2426	2437	rBV	1702639	2317546	75.72%	7.266%
83	17.457	2437	2443	2455	rVV	1598643	2257115	73.75%	7.076%
84	17.545	2455	2458	2462	rVB6	15018	20608	0.67%	0.065%
85	17.786	2496	2499	2502	rVB	20042	21349	0.70%	0.067%
86	17.845	2507	2509	2515	rBV7	4728	6475	0.21%	0.020%
87	17.981	2530	2532	2538	rVB7	9454	12156	0.40%	0.038%
88	18.198	2565	2569	2578	rBV2	132045	212643	6.95%	0.667%
89	18.463	2610	2614	2621	rVB6	20264	26383	0.86%	0.083%
90	18.798	2668	2671	2675	rBV6	12974	16064	0.52%	0.050%
91	19.022	2705	2709	2713	rBV2	24974	37684	1.23%	0.118%
92	19.269	2742	2751	2759	rBV2	53680	174329	5.70%	0.547%
93	19.369	2766	2768	2772	rVB	35694	36825	1.20%	0.115%
94	19.439	2776	2780	2786	rBV3	60858	83837	2.74%	0.263%
95	19.698	2819	2824	2834	rBV	2323683	3060675	100.00%	9.595%
96	20.157	2900	2902	2908	rBV3	29471	42199	1.38%	0.132%
97	20.645	2983	2985	2989	rBV2	39162	44872	1.47%	0.141%
98	21.463	3119	3124	3132	rBV	1903201	2503333	81.79%	7.848%
99	23.804	3517	3522	3535	rVB2	1419821	2821155	92.17%	8.844%
100	23.974	3544	3551	3562	rVB	1225668	2577150	84.20%	8.079%




Sum of corrected areas: 31897603

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP092523\
Data File : BP017338.D
Acq On : 26 Sep 2023 00:58
Operator : MA/JU
Sample : 04472-17
Misc :
ALS Vial : 29 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
EZY6

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP092023.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

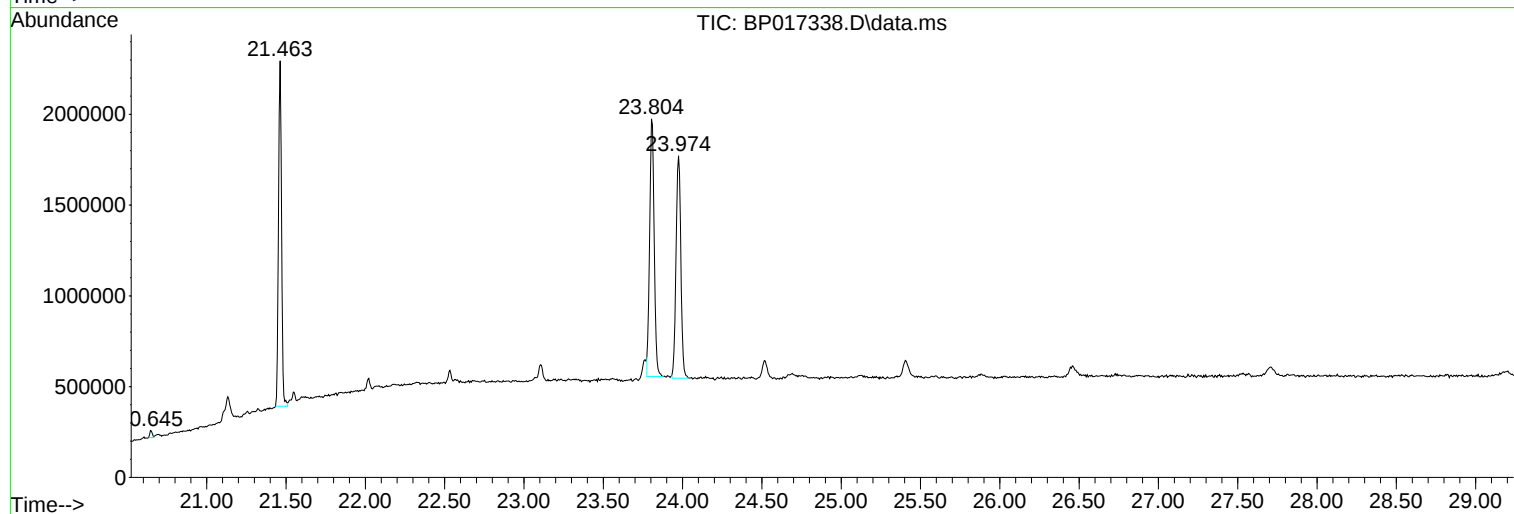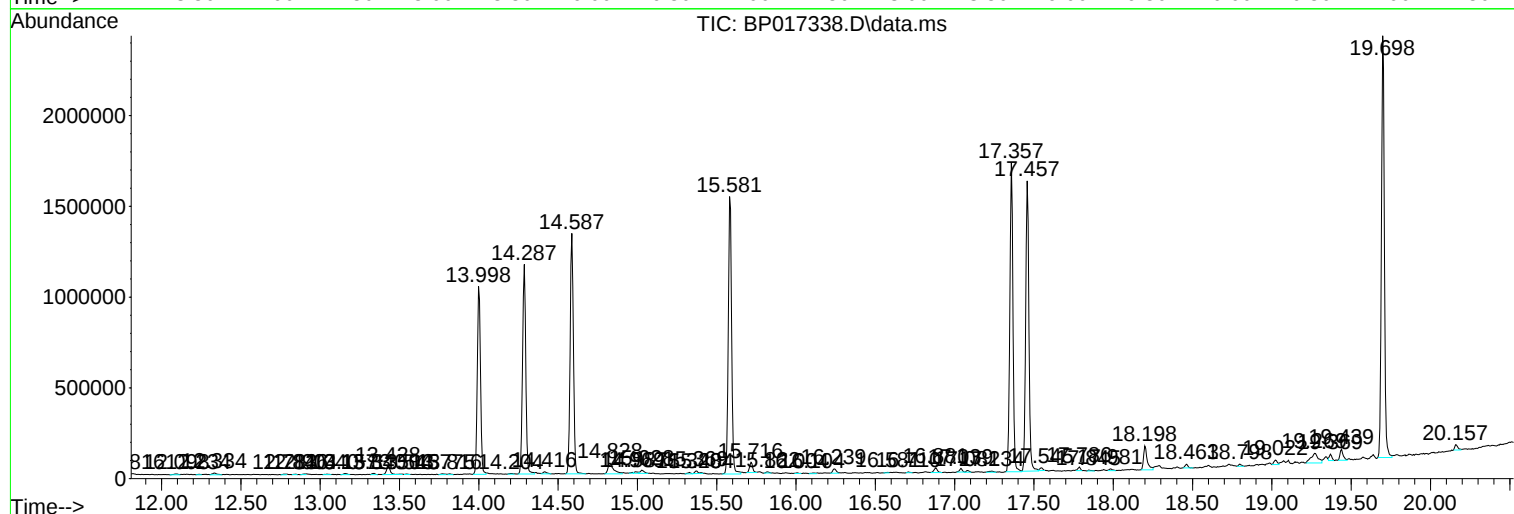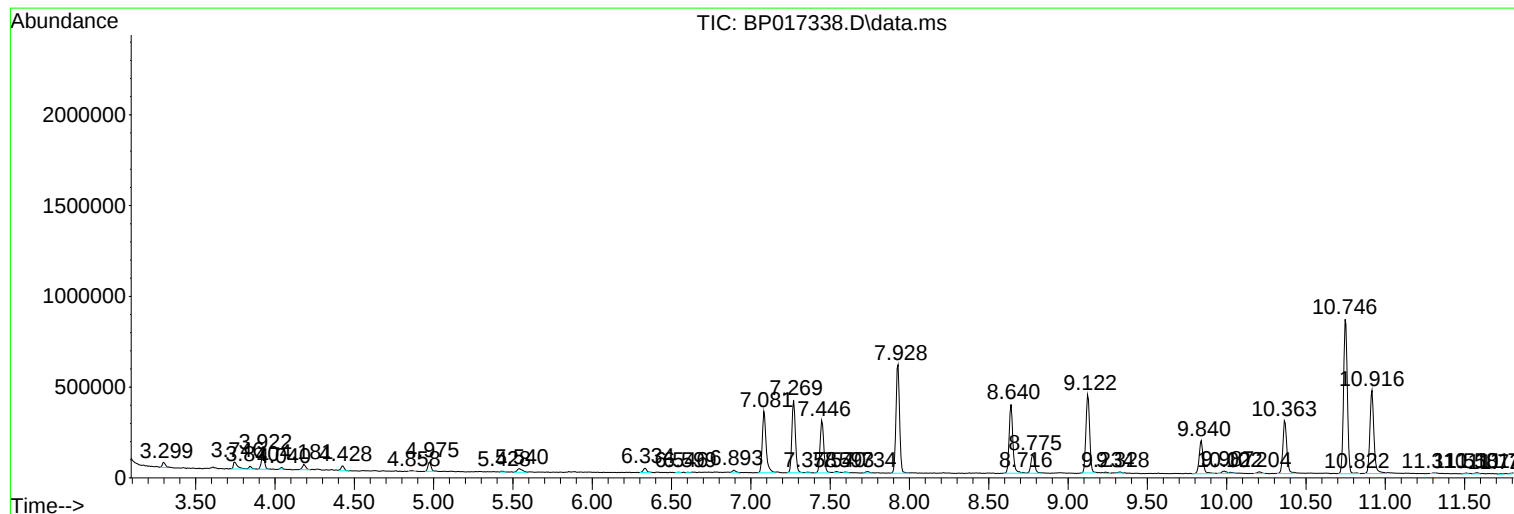

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP092523\
Data File : BP017338.D
Acq On : 26 Sep 2023 00:58
Operator : MA/JU
Sample : 04472-17
Misc :
ALS Vial : 29 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
EZY6










Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP092023.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Butane, 2,3-dimethoxy-2-met... Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
3.922	2.48 ng/ul	117107	1,4-Dichlorobenzene-d4	7.928

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Butane, 2,3-dimethoxy-2-methyl-	132	C7H16O2	074421-00-4	50
2			1-(2-Methoxyethoxy)-2-methyl-2-p...	162	C8H18O3	1000364-24-4	38
3			3-Heptanol, 3-methyl-	130	C8H18O	005582-82-1	25
4			Octanoic acid, 7-methoxy-3,7-dim...	216	C12H24O3	069687-76-9	25
5			Silane, trimethyl(1-methyl-1-pro...	128	C7H16Si	010111-13-4	25

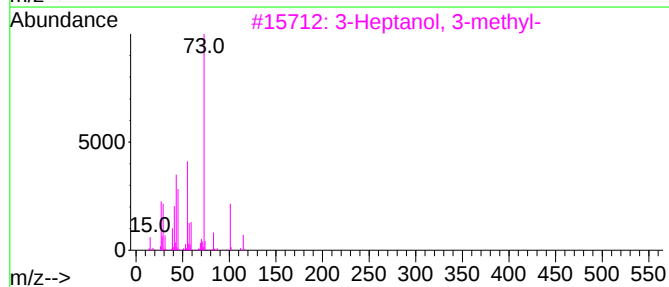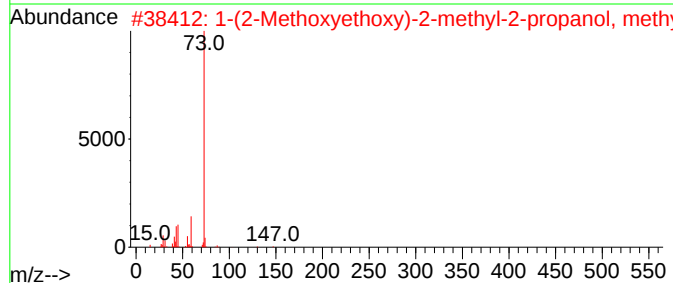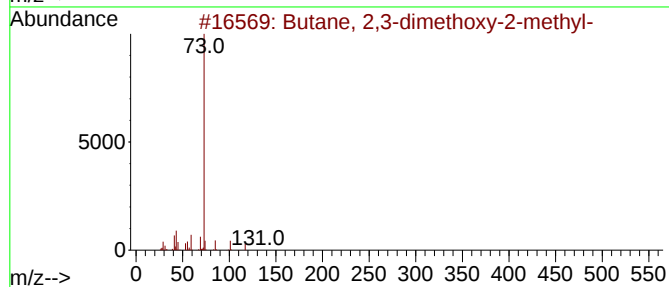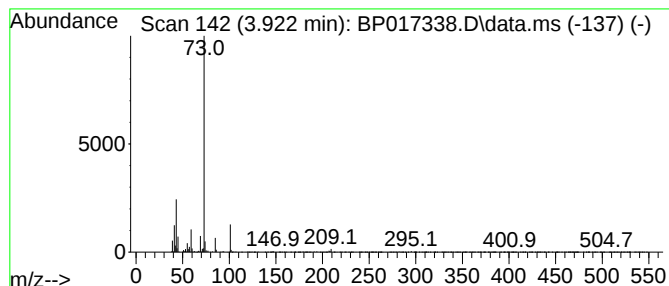

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP092523\
Data File : BP017338.D
Acq On : 26 Sep 2023 00:58
Operator : MA/JU
Sample : 04472-17
Misc :
ALS Vial : 29 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
EZYM6

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP092023.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Butane, 2,3-dim...	3.922	2.5	ng/u1	117107	1	7.928	942972	20.0