

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP092523\
 Data File : BP017353.D
 Acq On : 26 Sep 2023 10:00
 Operator : MA/JU
 Sample : 04472-14
 Misc :
 ALS Vial : 45 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 EZYM3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP092023.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP017353.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.299	33	36	44	rVB	35746	45001	1.48%	0.130%
2	3.746	109	112	124	rVB2	48437	82708	2.71%	0.239%
3	3.846	125	129	133	rVV	35482	43997	1.44%	0.127%
4	3.922	137	142	150	rVB	93614	135636	4.45%	0.391%
5	4.034	159	161	167	rVB2	14518	22655	0.74%	0.065%
6	4.181	182	186	193	rVB3	29887	49875	1.64%	0.144%
7	4.428	224	228	236	rVB2	32023	47161	1.55%	0.136%
8	4.622	258	261	264	rVB5	6889	8891	0.29%	0.026%
9	4.969	316	320	327	rBV	56653	81700	2.68%	0.236%
10	5.099	339	342	348	rBV7	6288	9510	0.31%	0.027%
11	5.287	368	374	375	rBV6	4998	7510	0.25%	0.022%
12	5.434	396	399	403	rVB2	5856	7181	0.24%	0.021%
13	5.540	408	417	426	rBV2	37391	71063	2.33%	0.205%
14	5.852	466	470	472	rBV4	9016	12171	0.40%	0.035%
15	5.975	489	491	498	rVB8	4590	8532	0.28%	0.025%
16	6.334	546	552	557	rBV	29513	45363	1.49%	0.131%
17	6.487	575	578	583	rVB7	6202	9305	0.31%	0.027%
18	6.769	622	626	631	rVB8	5978	11643	0.38%	0.034%
19	6.887	642	646	653	rVB4	12031	21480	0.70%	0.062%
20	6.993	660	664	671	rVB10	3859	7216	0.24%	0.021%
21	7.081	673	679	692	rBV	463081	774559	25.39%	2.235%
22	7.269	701	711	721	rBV	455619	692486	22.70%	1.998%
23	7.446	735	741	752	rBV	398122	638720	20.94%	1.843%
24	7.534	752	756	763	rBV9	6786	14093	0.46%	0.041%
25	7.734	783	790	798	rBV	9376	21645	0.71%	0.062%
26	7.816	801	804	808	rVB6	5971	8452	0.28%	0.024%
27	7.922	815	822	835	rBV	806314	1289060	42.26%	3.719%
28	8.016	835	838	843	rVB7	4025	6882	0.23%	0.020%
29	8.504	916	921	923	rBV6	4851	7448	0.24%	0.021%
30	8.640	936	944	954	rBV	303006	516448	16.93%	1.490%
31	8.775	961	967	976	rVB	134448	215271	7.06%	0.621%
32	8.934	988	994	999	rBV10	4748	12428	0.41%	0.036%
33	9.081	1015	1019	1020	rBV4	10678	13480	0.44%	0.039%
34	9.122	1020	1026	1037	rVV	505202	806205	26.43%	2.326%
35	9.240	1041	1046	1050	rVB8	8934	17272	0.57%	0.050%
36	9.322	1055	1060	1069	rVB9	9531	19233	0.63%	0.055%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP092523\
 Data File : BP017353.D
 Acq On : 26 Sep 2023 10:00
 Operator : MA/JU
 Sample : 04472-14
 Misc :
 ALS Vial : 45 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 EZYM3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP092023.MA.M
 Title : SVOA CALIBRATION

37	9.522	1091	1094	1100	rVB8	4572	8737	0.29%	0.025%
38	9.840	1138	1148	1155	rVV	206481	359171	11.78%	1.036%
39	9.981	1166	1172	1179	rBV7	14018	32879	1.08%	0.095%
40	10.110	1191	1194	1199	rVB5	8003	9810	0.32%	0.028%
41	10.204	1205	1210	1215	rVB2	11883	19195	0.63%	0.055%
42	10.363	1230	1237	1250	rBV	345598	587479	19.26%	1.695%
43	10.634	1279	1283	1289	rBV6	6993	11778	0.39%	0.034%
44	10.745	1295	1302	1311	rBV	1149178	1880880	61.66%	5.426%
45	10.916	1323	1331	1342	rBV	394725	719538	23.59%	2.076%
46	11.310	1391	1398	1399	rBV6	5726	10611	0.35%	0.031%
47	11.575	1438	1443	1449	rBV3	7297	14662	0.48%	0.042%
48	11.681	1457	1461	1465	rBV7	4756	7209	0.24%	0.021%
49	11.816	1480	1484	1490	rVB9	7432	14307	0.47%	0.041%
50	12.086	1526	1530	1534	rBV7	9089	13898	0.46%	0.040%
51	12.228	1549	1554	1560	rBV9	3768	8003	0.26%	0.023%
52	12.328	1568	1571	1576	rVB3	11300	16944	0.56%	0.049%
53	12.404	1579	1584	1590	rVB6	5600	9236	0.30%	0.027%
54	12.628	1617	1622	1626	rBV7	4608	8169	0.27%	0.024%
55	13.033	1688	1691	1699	rVB10	4429	8568	0.28%	0.025%
56	13.333	1735	1742	1746	rVB5	11784	18257	0.60%	0.053%
57	13.428	1750	1758	1766	rBV2	51575	91299	2.99%	0.263%
58	13.822	1822	1825	1829	rVB6	5296	6958	0.23%	0.020%
59	13.904	1833	1839	1841	rBV6	8245	13301	0.44%	0.038%
60	13.998	1849	1855	1872	rVB	1063937	1453521	47.65%	4.193%
61	14.286	1897	1904	1921	rVV	1180274	1738970	57.01%	5.017%
62	14.416	1921	1926	1934	rVB4	14955	26045	0.85%	0.075%
63	14.586	1945	1955	1965	rBV	1636471	2373956	77.83%	6.849%
64	14.969	2016	2020	2022	rBV5	7651	9784	0.32%	0.028%
65	15.004	2022	2026	2028	rVV5	9694	16778	0.55%	0.048%
66	15.033	2028	2031	2038	rVB8	10705	19532	0.64%	0.056%
67	15.186	2051	2057	2062	rBV10	5687	12470	0.41%	0.036%
68	15.245	2064	2067	2072	rVB7	4586	7511	0.25%	0.022%
69	15.327	2076	2081	2084	rBV6	6540	11480	0.38%	0.033%
70	15.369	2085	2088	2092	rBV6	10109	14011	0.46%	0.040%
71	15.580	2118	2124	2131	rBV	1502865	2175216	71.31%	6.275%
72	15.769	2151	2156	2160	rVB8	5914	8809	0.29%	0.025%
73	15.822	2161	2165	2169	rVB7	6208	8993	0.29%	0.026%
74	16.245	2232	2237	2243	rBV2	14601	27512	0.90%	0.079%
75	16.292	2243	2245	2252	rVB8	6111	11884	0.39%	0.034%
76	16.392	2255	2262	2266	rBV3	10706	21347	0.70%	0.062%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP092523\
 Data File : BP017353.D
 Acq On : 26 Sep 2023 10:00
 Operator : MA/JU
 Sample : 04472-14
 Misc :
 ALS Vial : 45 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 EZYM3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP092023.MA.M
 Title : SVOA CALIBRATION

77	16.451	2269	2272	2278	rVB6	8908	17430	0.57%	0.050%
78	16.516	2279	2283	2288	rVB5	8885	11585	0.38%	0.033%
79	16.639	2302	2304	2311	rVB8	7273	10646	0.35%	0.031%
80	16.716	2311	2317	2322	rBV10	8634	19715	0.65%	0.057%
81	16.792	2326	2330	2332	rBV2	8930	12911	0.42%	0.037%
82	16.880	2339	2345	2352	rVB	33566	51694	1.69%	0.149%
83	17.004	2362	2366	2367	rBV4	4986	7060	0.23%	0.020%
84	17.039	2370	2372	2376	rVV2	12443	16000	0.52%	0.046%
85	17.080	2376	2379	2385	rVB7	9194	15908	0.52%	0.046%
86	17.357	2420	2426	2437	rBV	1953251	2709526	88.83%	7.817%
87	17.457	2437	2443	2455	rVV2	1456006	2035159	66.72%	5.871%
88	17.845	2507	2509	2515	rVB6	6688	7096	0.23%	0.020%
89	17.980	2530	2532	2536	rVB4	9613	9892	0.32%	0.029%
90	18.198	2565	2569	2577	rBV2	118532	185908	6.09%	0.536%
91	18.727	2657	2659	2662	rBV4	13864	18543	0.61%	0.053%
92	18.910	2686	2690	2696	rBV	117597	149293	4.89%	0.431%
93	19.021	2706	2709	2712	rBV	29378	33270	1.09%	0.096%
94	19.298	2754	2756	2757	rBV2	20267	13807	0.45%	0.040%
95	19.327	2758	2761	2770	rVB5	136891	217633	7.14%	0.628%
96	19.439	2776	2780	2786	rBV2	73049	91219	2.99%	0.263%
97	19.698	2819	2824	2833	rBV	2187998	2840282	93.12%	8.194%
98	21.462	3119	3124	3130	rBV	2240660	2878216	94.36%	8.303%
99	23.803	3517	3522	3531	rVB2	1341935	2669617	87.52%	7.702%
100	23.974	3544	3551	3563	rVB	1467796	3050178	100.00%	8.799%




Sum of corrected areas: 34663576

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP092523\
Data File : BP017353.D
Acq On : 26 Sep 2023 10:00
Operator : MA/JU
Sample : 04472-14
Misc :
ALS Vial : 45 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
EZY3

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP092023.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

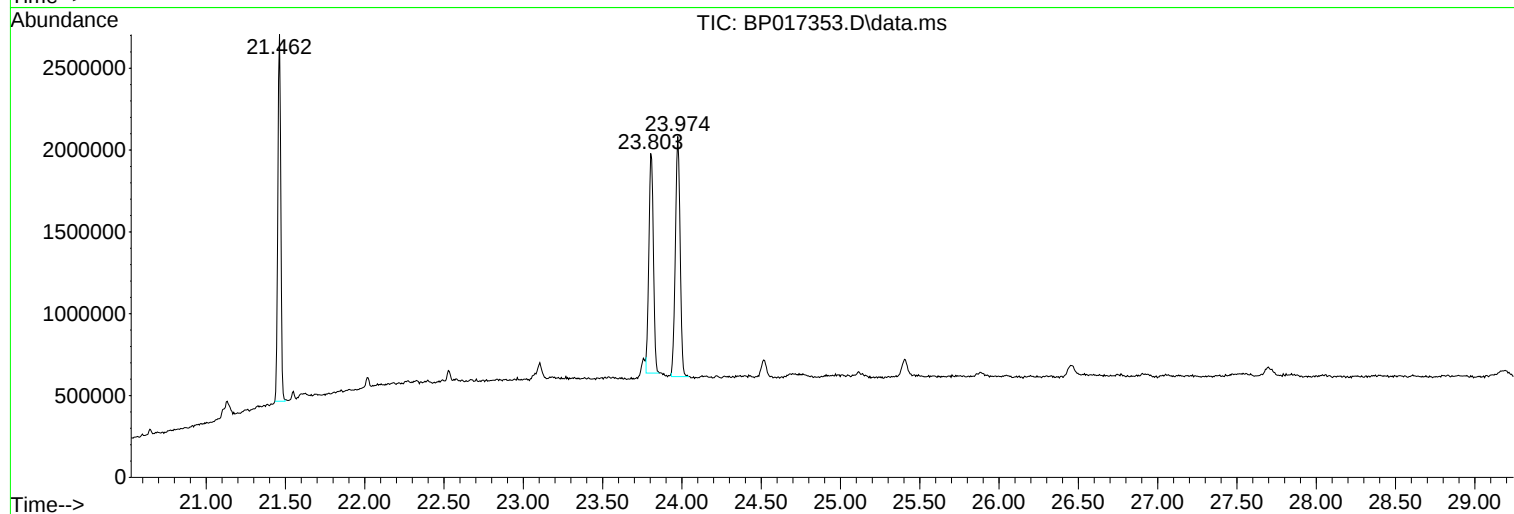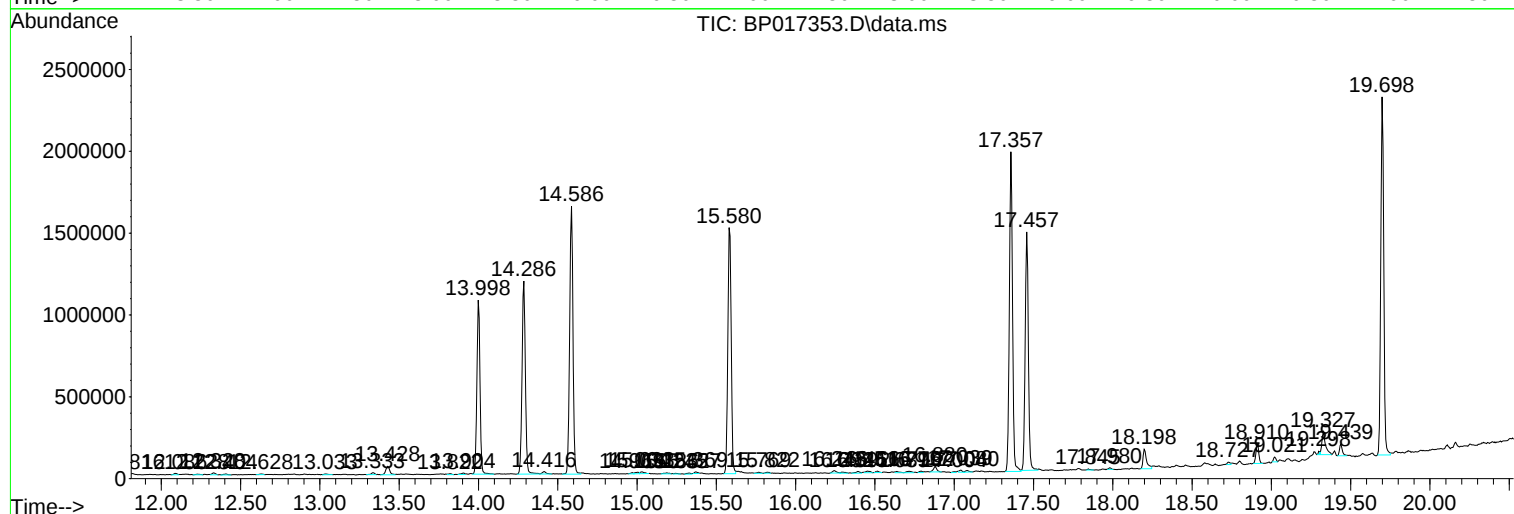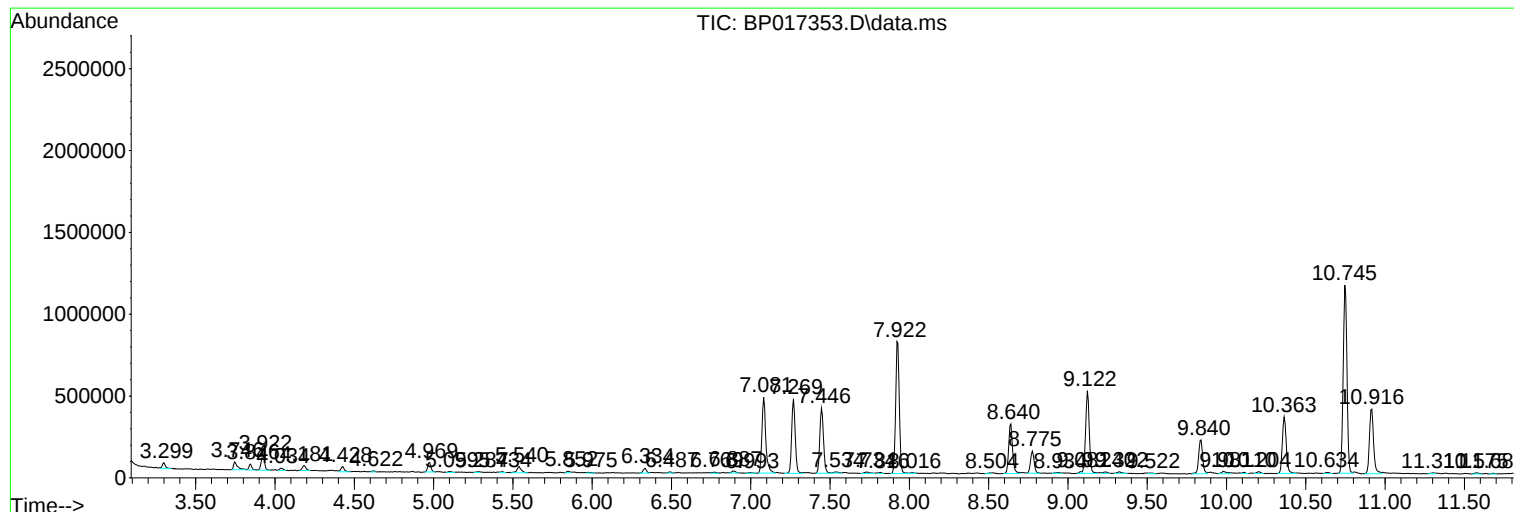

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP092523\
Data File : BP017353.D
Acq On : 26 Sep 2023 10:00
Operator : MA/JU
Sample : 04472-14
Misc :
ALS Vial : 45 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
EZY3










Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP092023.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Butane, 2,3-dimethoxy-2-met... Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
3.922	2.10 ng/ul	135636	1,4-Dichlorobenzene-d4	7.928

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Butane, 2,3-dimethoxy-2-methyl-	132	C7H16O2	074421-00-4	59
2			Octanal, 7-methoxy-3,7-dimethyl-	186	C11H22O2	003613-30-7	37
3			3-Hexanol, 3,5-dimethyl-	130	C8H18O	004209-91-0	36
4			Valproic Acid	144	C8H16O2	000099-66-1	33
5			3-Heptanol, 3-methyl-	130	C8H18O	005582-82-1	28

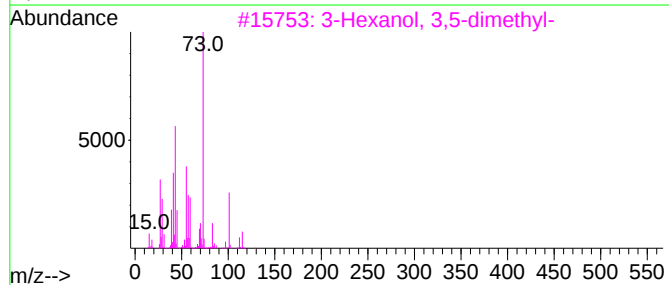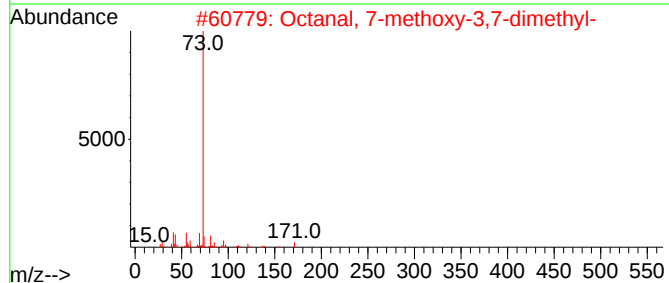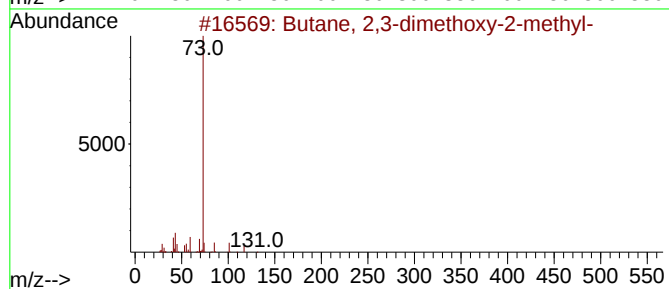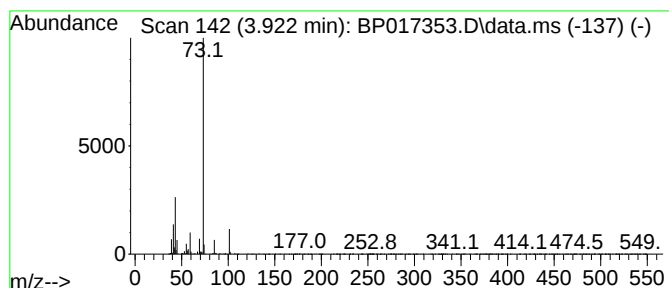

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP092523\
Data File : BP017353.D
Acq On : 26 Sep 2023 10:00
Operator : MA/JU
Sample : 04472-14
Misc :
ALS Vial : 45 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
EZYM3

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP092023.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Butane, 2,3-dim...	3.922	2.1	ng/ul	135636	1	7.928	1289060	20.0