

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP092523\
 Data File : BP017359.D
 Acq On : 26 Sep 2023 13:37
 Operator : MA/JU
 Sample : PB155787BL
 Misc :
 ALS Vial : 51 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK787

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP092023.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP017359.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.293	32	35	46	rVB	55870	77080	1.46%	0.146%
2	3.728	105	109	136	rBV	710203	1030671	19.48%	1.954%
3	4.040	159	162	166	rVB2	10650	10926	0.21%	0.021%
4	7.081	670	679	694	rBV	799460	1290234	24.38%	2.447%
5	7.269	704	711	719	rBV	645226	1007459	19.04%	1.910%
6	7.446	734	741	754	rBV	848234	1316620	24.88%	2.497%
7	7.922	815	822	830	rVB	643692	991201	18.73%	1.880%
8	8.634	933	943	956	rBV	985232	1624033	30.69%	3.080%
9	9.122	1019	1026	1034	rBV	787278	1255410	23.72%	2.381%
10	9.834	1139	1147	1162	rBV	661848	1094345	20.68%	2.075%
11	10.357	1228	1236	1254	rBV	973249	1701117	32.15%	3.226%
12	10.745	1295	1302	1311	rBV	946283	1544462	29.19%	2.929%
13	10.910	1323	1330	1344	rBV	1009292	1749301	33.06%	3.317%
14	11.781	1470	1478	1479	rBV8	3171	6868	0.13%	0.013%
15	12.328	1564	1571	1580	rBV3	17853	35638	0.67%	0.068%
16	13.428	1752	1758	1763	rBV2	17421	28119	0.53%	0.053%
17	13.998	1847	1855	1865	rBV	1907093	2567702	48.52%	4.869%
18	14.286	1897	1904	1916	rBV	2147062	3036540	57.38%	5.758%
19	14.586	1947	1955	1965	rBV	1459580	2172502	41.06%	4.120%
20	14.816	1987	1994	2014	rBV	619223	1173756	22.18%	2.226%
21	15.580	2115	2124	2135	rBV	2809198	3924439	74.16%	7.442%
22	15.716	2140	2147	2158	rVV	744522	1004266	18.98%	1.904%
23	15.816	2160	2164	2171	rVB3	13611	25226	0.48%	0.048%
24	17.139	2385	2389	2395	rBV7	6110	12245	0.23%	0.023%
25	17.357	2420	2426	2436	rBV	1976656	2753900	52.04%	5.222%
26	17.457	2436	2443	2457	rVV	3329593	4477739	84.62%	8.491%
27	19.268	2748	2751	2755	rBV2	37296	45778	0.87%	0.087%
28	19.339	2759	2763	2767	rVB	37976	53275	1.01%	0.101%
29	19.698	2819	2824	2833	rBV	4109840	5278631	99.76%	10.009%
30	21.462	3119	3124	3130	rBV	2329859	2970621	56.14%	5.633%
31	23.809	3516	3523	3535	rVB2	2648776	5291541	100.00%	10.034%
32	23.974	3544	3551	3566	rVB	1562017	3184899	60.19%	6.039%




Sum of corrected areas: 52736544

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP092523\
Data File : BP017359.D
Acq On : 26 Sep 2023 13:37
Operator : MA/JU
Sample : PB155787BL
Misc :
ALS Vial : 51 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK787

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP092023.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

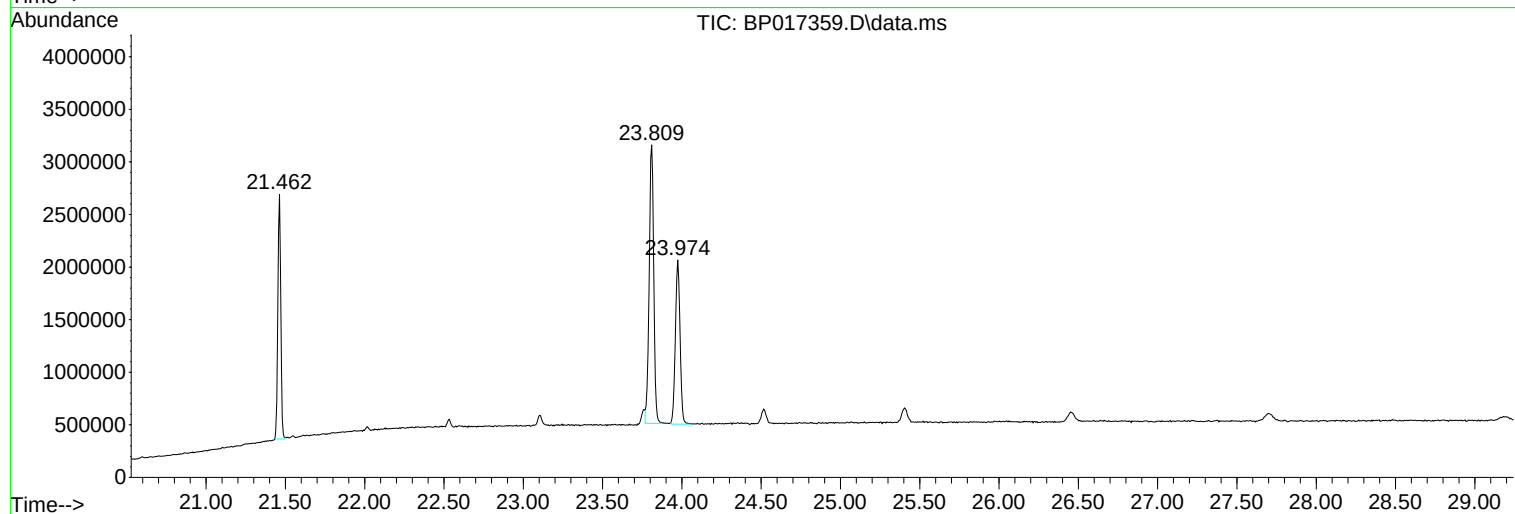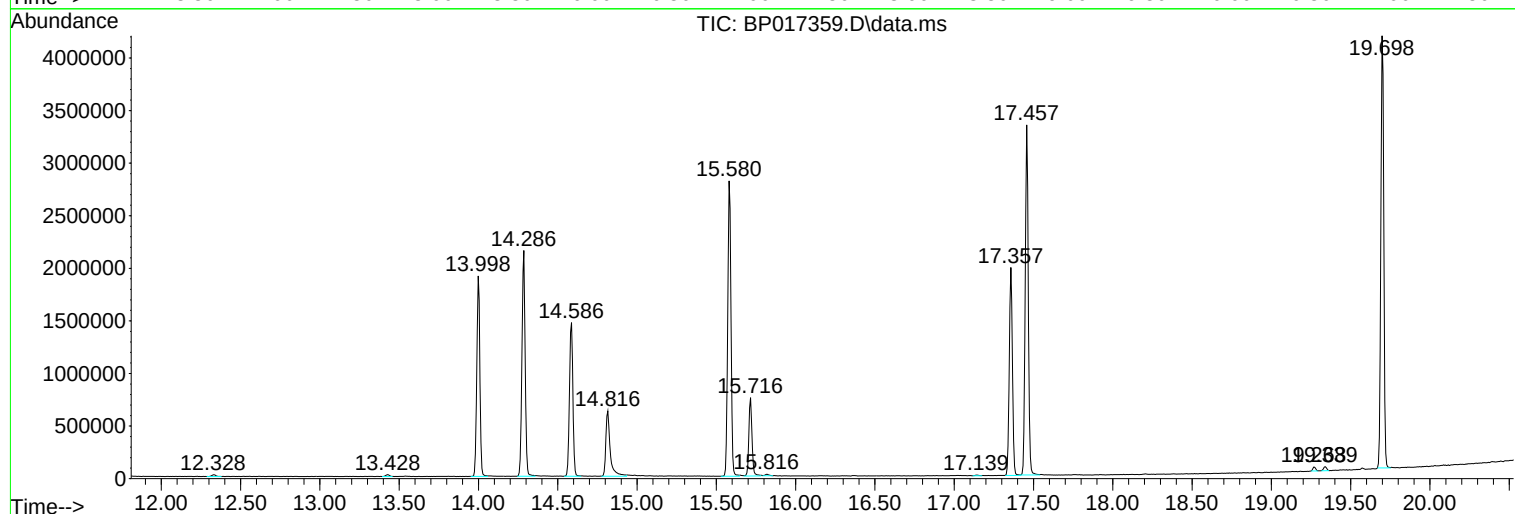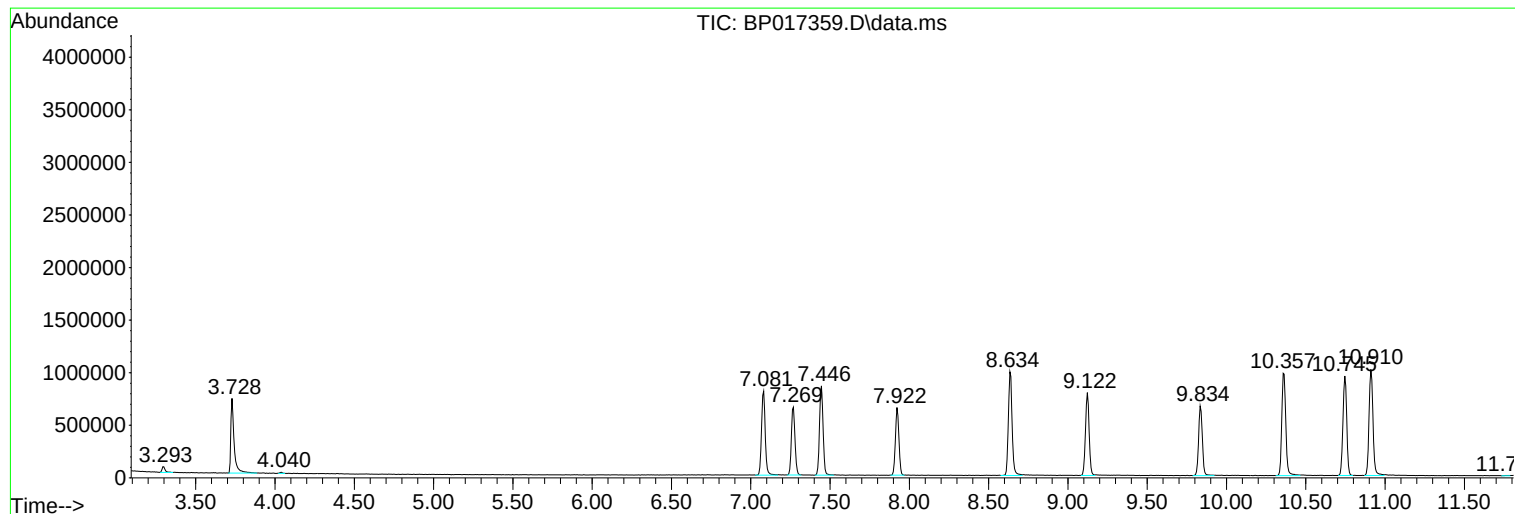

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP092523\
Data File : BP017359.D
Acq On : 26 Sep 2023 13:37
Operator : MA/JU
Sample : PB155787BL
Misc :
ALS Vial : 51 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK787

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP092023.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP092523\
Data File : BP017359.D
Acq On : 26 Sep 2023 13:37
Operator : MA/JU
Sample : PB155787BL
Misc :
ALS Vial : 51 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK787

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP092023.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------