
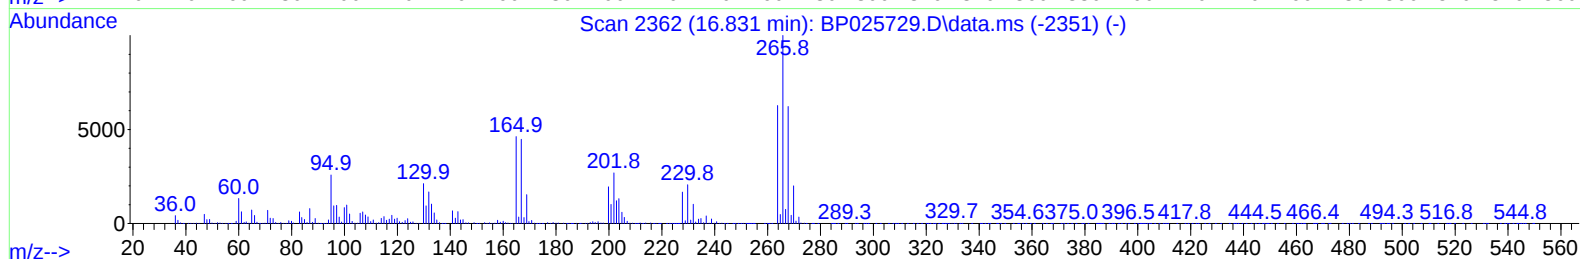
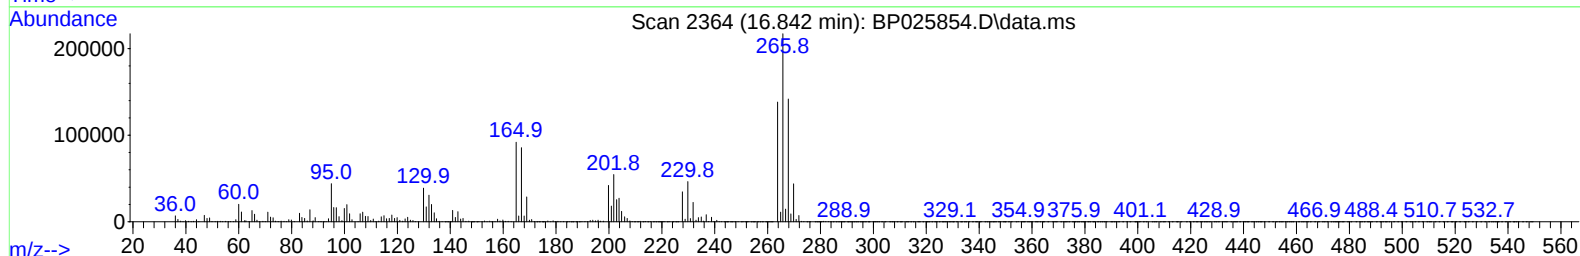


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP092525\
Data File : BP025854.D
Acq On : 25 Sep 2025 10:53
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 25 12:45:57 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP091225.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Sep 11 16:45:04 2025
Response via : Initial Calibration

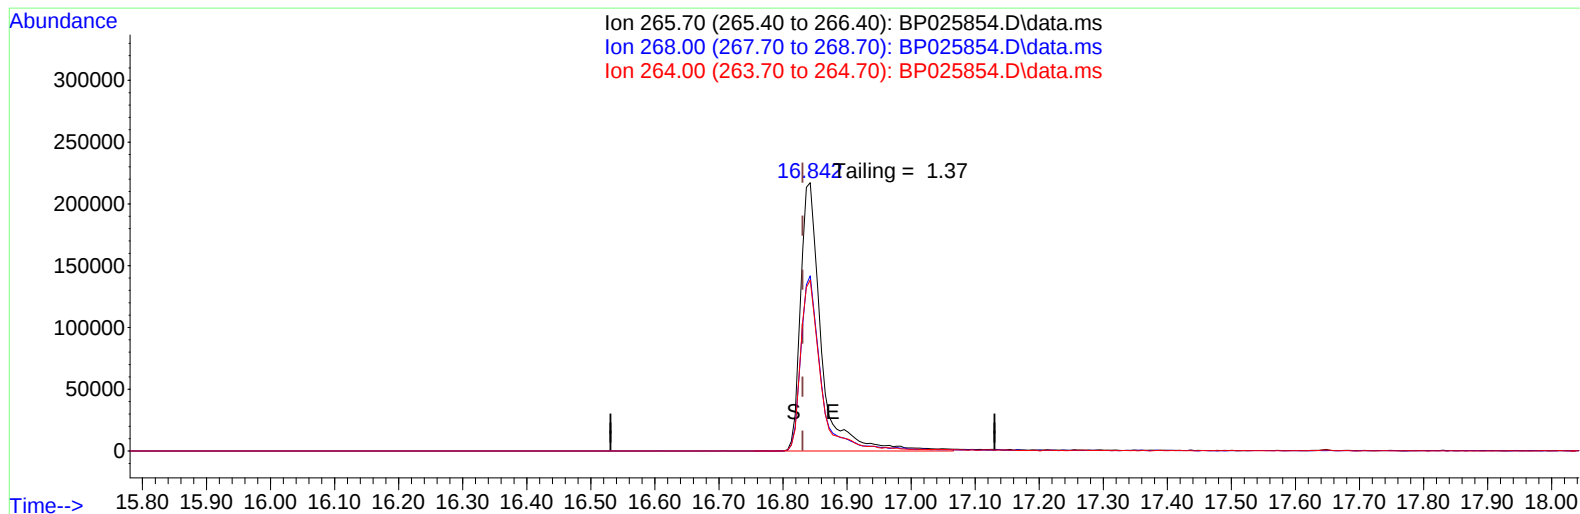

TIC: BP025854.D\data.ms

(70) Pentachlorophenol (C)




16.842min (+ 0.012) 381324.51 ng

response 487157

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.30	65.29
264.00	62.70	63.67
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP092525\
Data File : BP025854.D
Acq On : 25 Sep 2025 10:53
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 25 12:45:57 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP091225.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Sep 11 16:45:04 2025
Response via : Initial Calibration

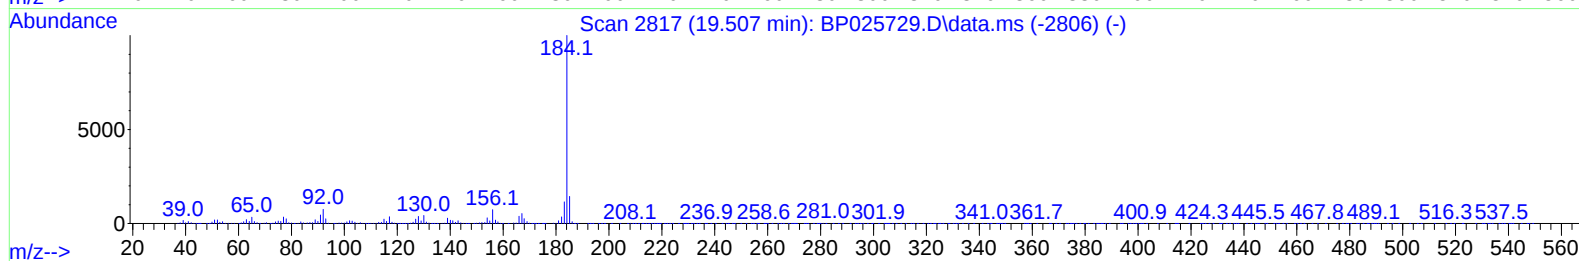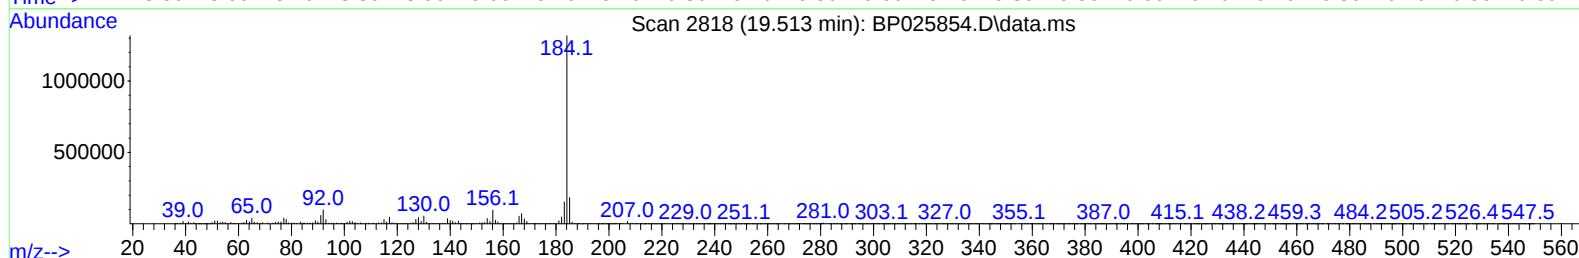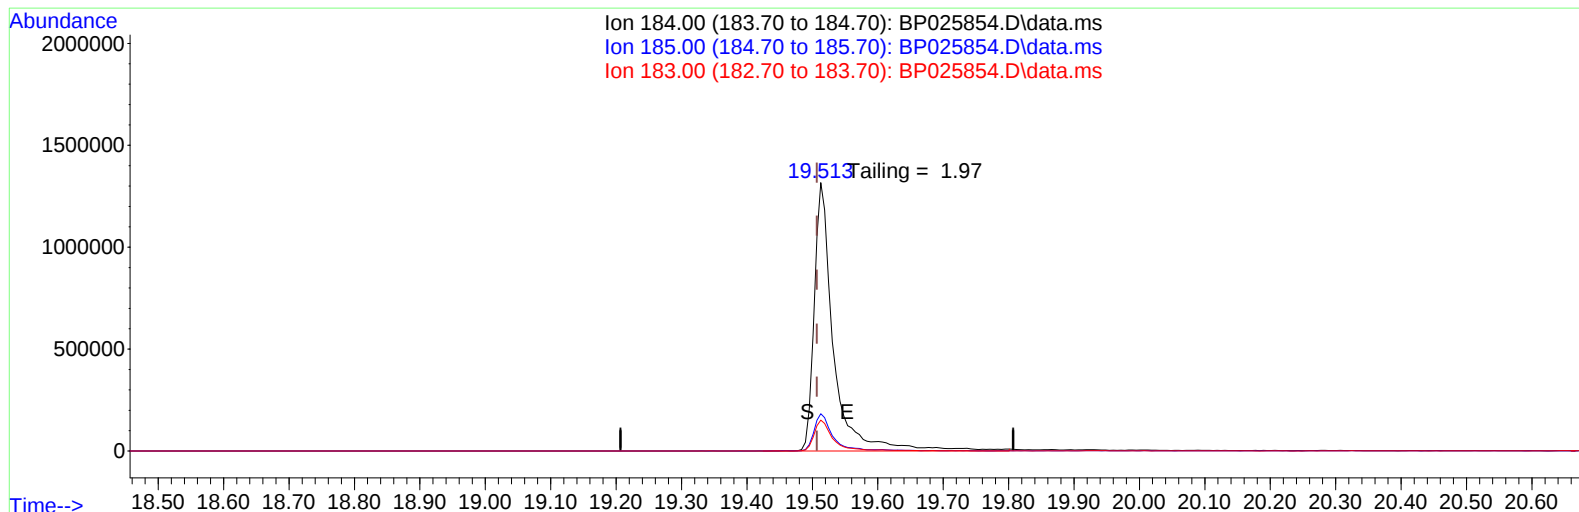

TIC: BP025854.D\data.ms

(77) Benzidine

19.513min (+ 0.006) 616938.90 ng

response 2647900

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.40	13.92
183.00	11.50	11.55
0.00	0.00	0.00