

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP092525\
 Data File : BP025861.D
 Acq On : 25 Sep 2025 16:06
 Operator : CG/JU
 Sample : PB169834BL
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 PB169834BL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP091225.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BP025861.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.373	408	414	436	rBV	1690763	2972527	41.21%	10.454%
2	6.949	674	682	703	rBV	1304557	2783222	38.59%	9.789%
3	7.743	810	817	828	rBV	321701	546295	7.57%	1.921%
4	8.890	1004	1012	1033	rBV	908394	1863487	25.84%	6.554%
5	10.513	1279	1288	1307	rBV	323433	733267	10.17%	2.579%
6	12.978	1699	1707	1721	rBV	2400706	4282500	59.38%	15.062%
7	14.372	1937	1944	1962	rBV	464205	969854	13.45%	3.411%
8	15.901	2196	2204	2224	rBV	1661845	3501809	48.55%	12.316%
9	17.178	2415	2421	2435	rBV2	576606	1172493	16.26%	4.124%
10	19.895	2878	2883	2898	rBV	5038724	7212337	100.00%	25.366%
11	21.648	3176	3181	3192	rBV	600826	1268048	17.58%	4.460%
12	25.019	3750	3754	3772	rVB2	347708	1127341	15.63%	3.965%




Sum of corrected areas: 28433180

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP092525\
Data File : BP025861.D
Acq On : 25 Sep 2025 16:06
Operator : CG/JU
Sample : PB169834BL
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB169834BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP091225.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

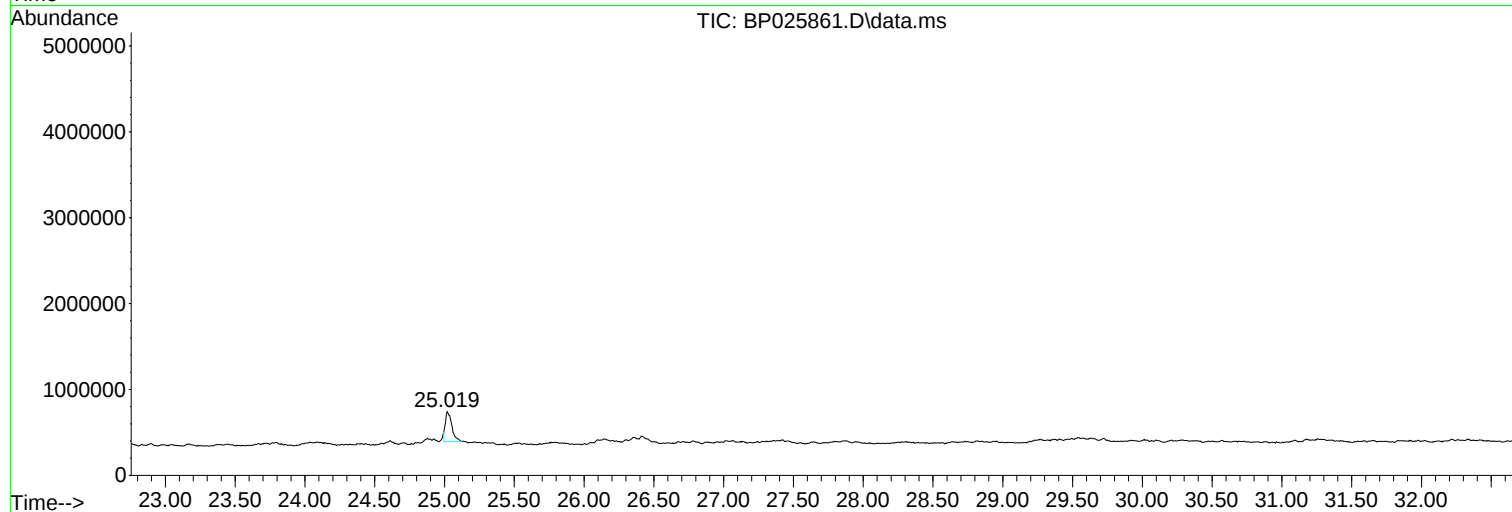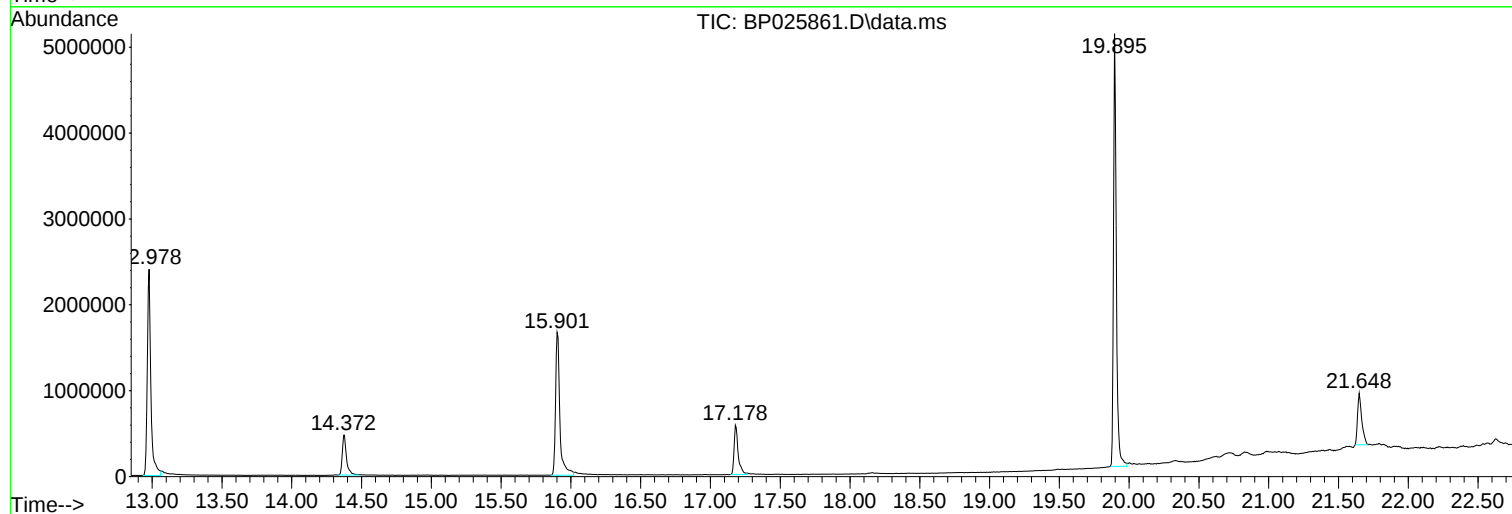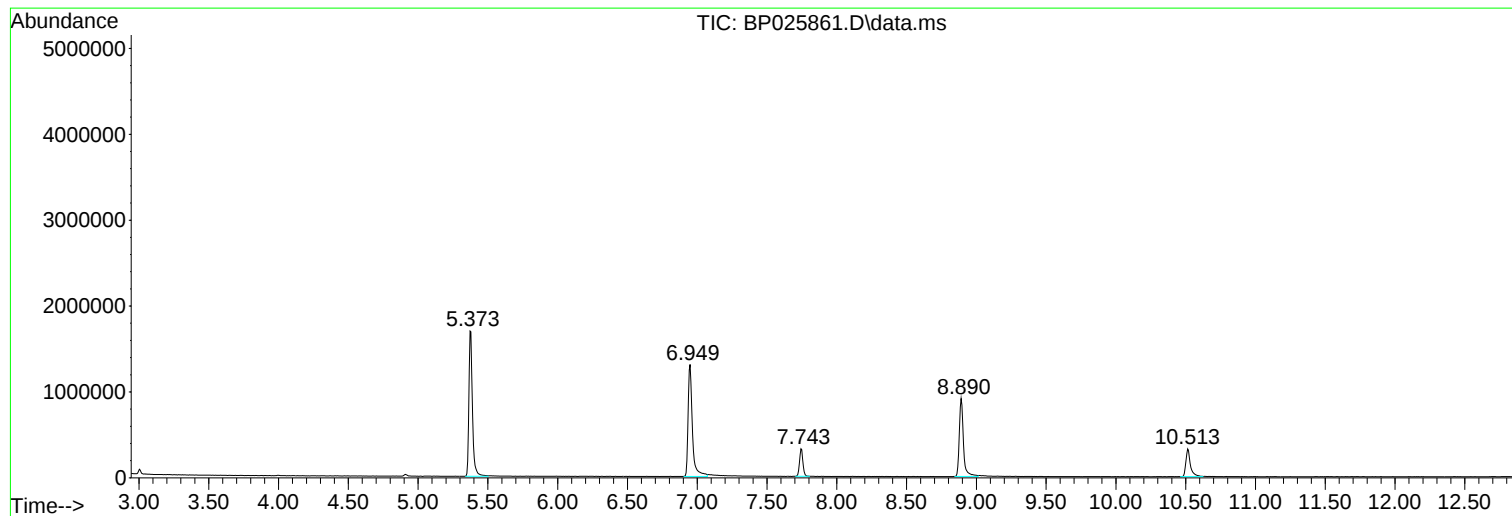

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP092525\
Data File : BP025861.D
Acq On : 25 Sep 2025 16:06
Operator : CG/JU
Sample : PB169834BL
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB169834BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP091225.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP092525\
Data File : BP025861.D
Acq On : 25 Sep 2025 16:06
Operator : CG/JU
Sample : PB169834BL
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB169834BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP091225.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------