
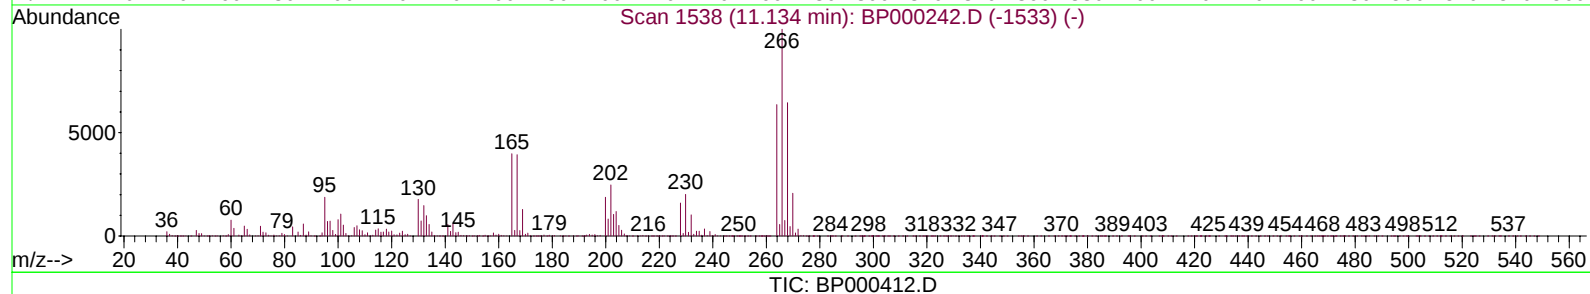
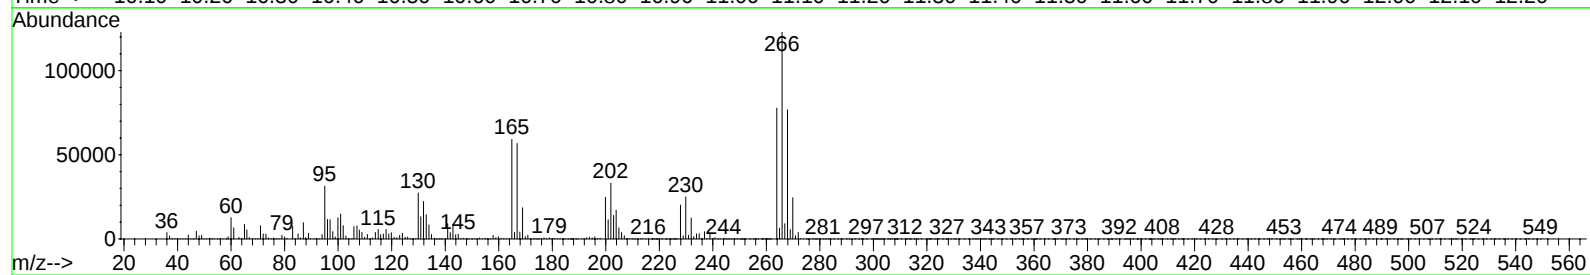


Data Path : Z:\svoasrv\HPCHEM1\BNA P\Data\BP092619\
Data File : BP000412.D
Acq On : 26 Sep 2019 10:18
Operator : JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 26 18:58:02 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA P\METHODS\8270-BP091619.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Sep 19 14:44:51 2019
Response via : Initial Calibration

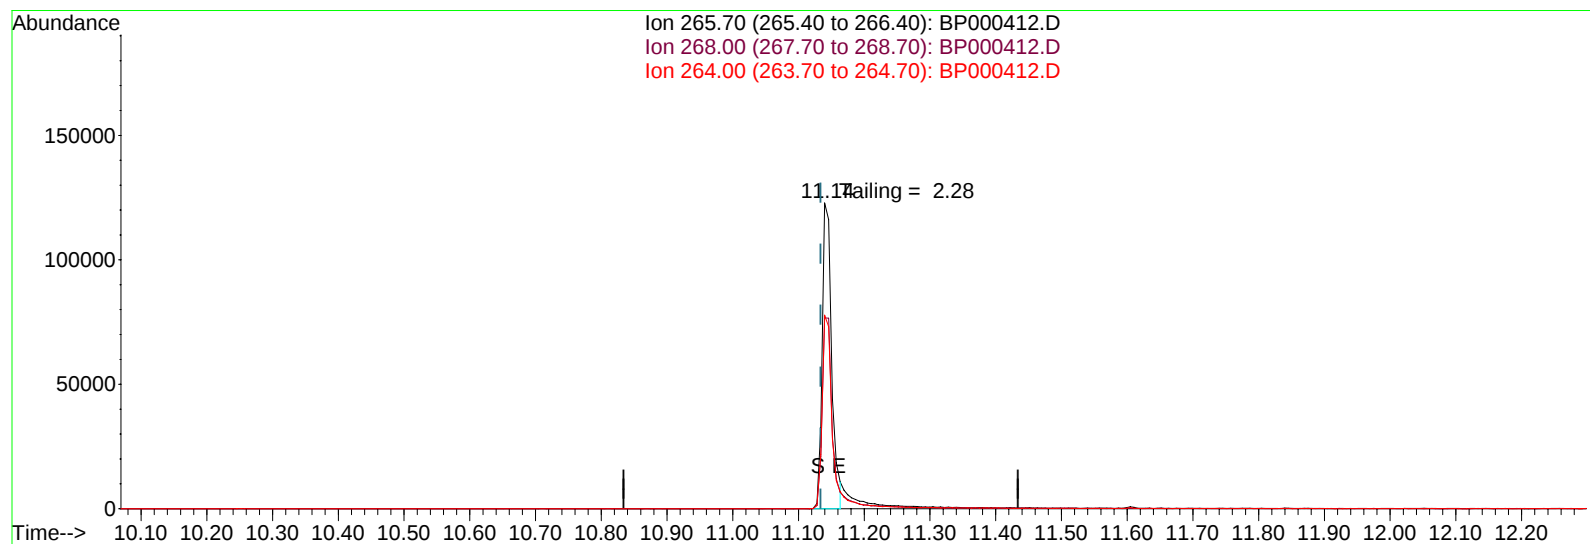

(70) Pentachlorophenol (C)




11.140min (+0.006) 2385.50ng

response 139368

Ion	Exp%	Act%
265.70	100	100
268.00	64.50	62.44
264.00	63.50	63.33
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA P\Data\BP092619\
Data File : BP000412.D
Acq On : 26 Sep 2019 10:18
Operator : JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 26 18:58:02 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA P\METHODS\8270-BP091619.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Sep 19 14:44:51 2019
Response via : Initial Calibration

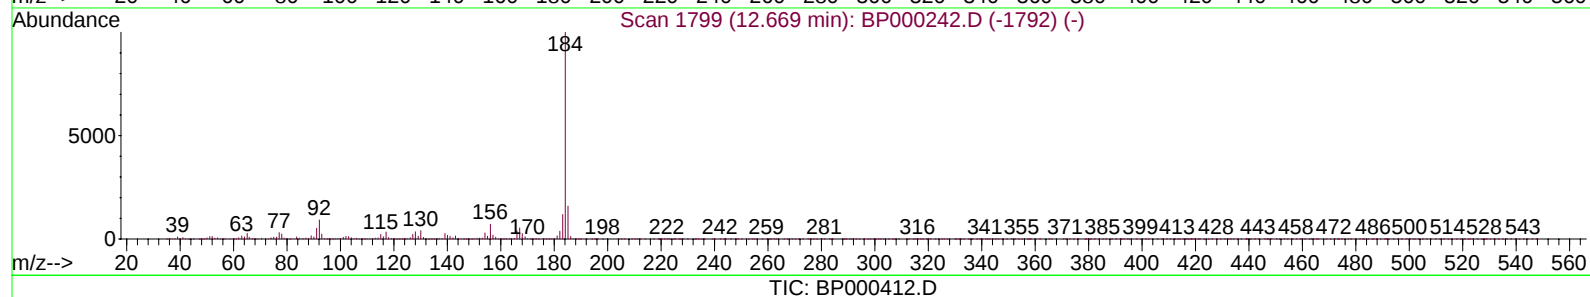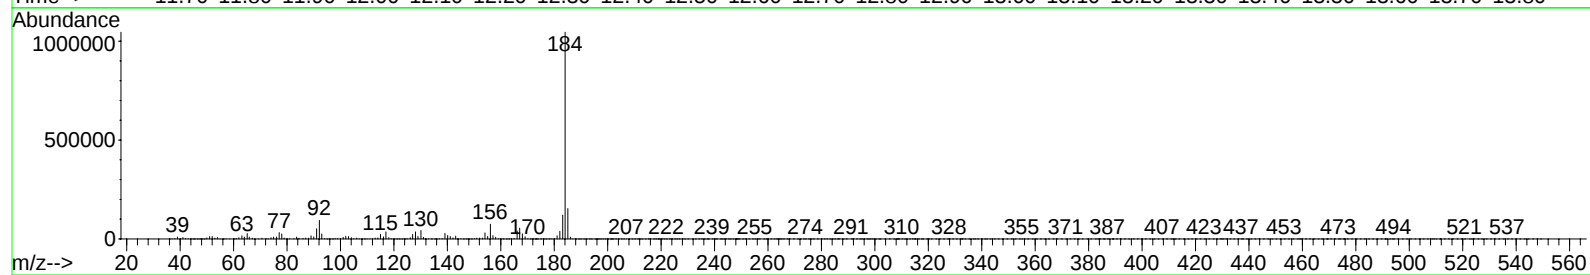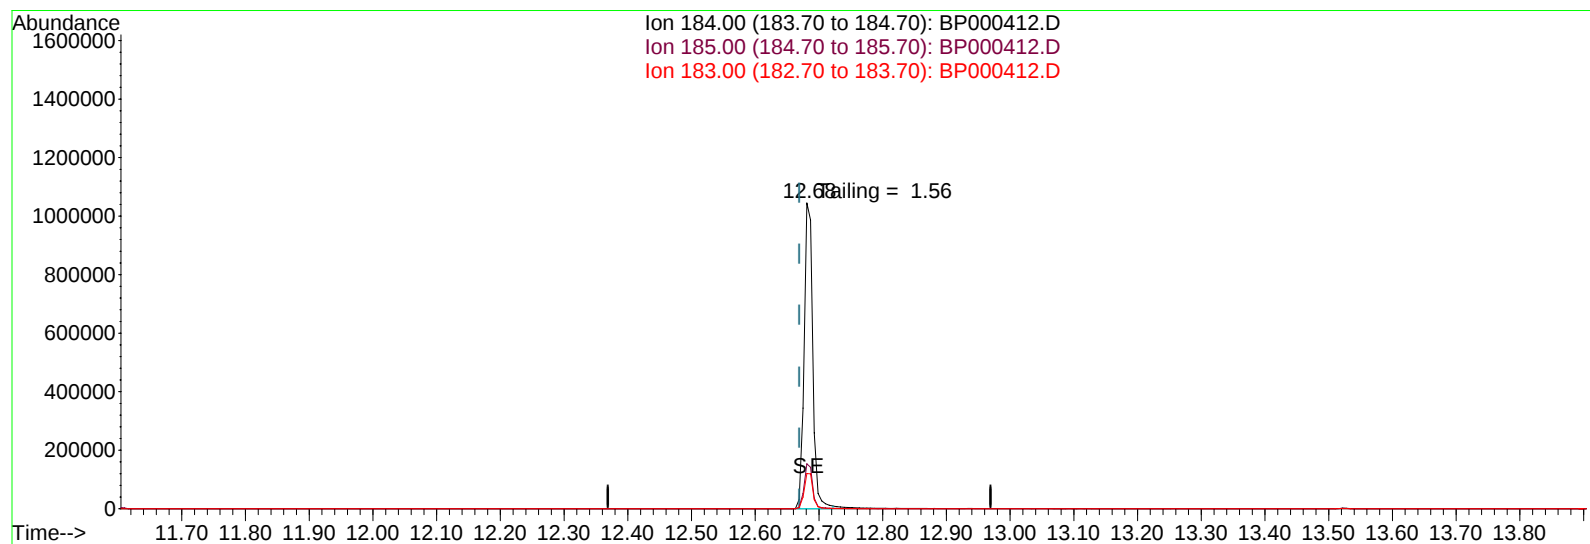

(77) Benzidine

12.681min (+0.012) 2518.96ng

response 1005241

Ion	Exp%	Act%
184.00	100	100
185.00	15.90	14.71
183.00	11.90	11.52
0.00	0.00	0.00