


Data Path : Z:\SVOASRV\HPCHEM1\BNA_P\DATA\BP092619\
 Data File : BP000412.D
 Acq On : 26 Sep 2019 10:18
 Operator : JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP091619.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Sep 19 14:44:51 2019

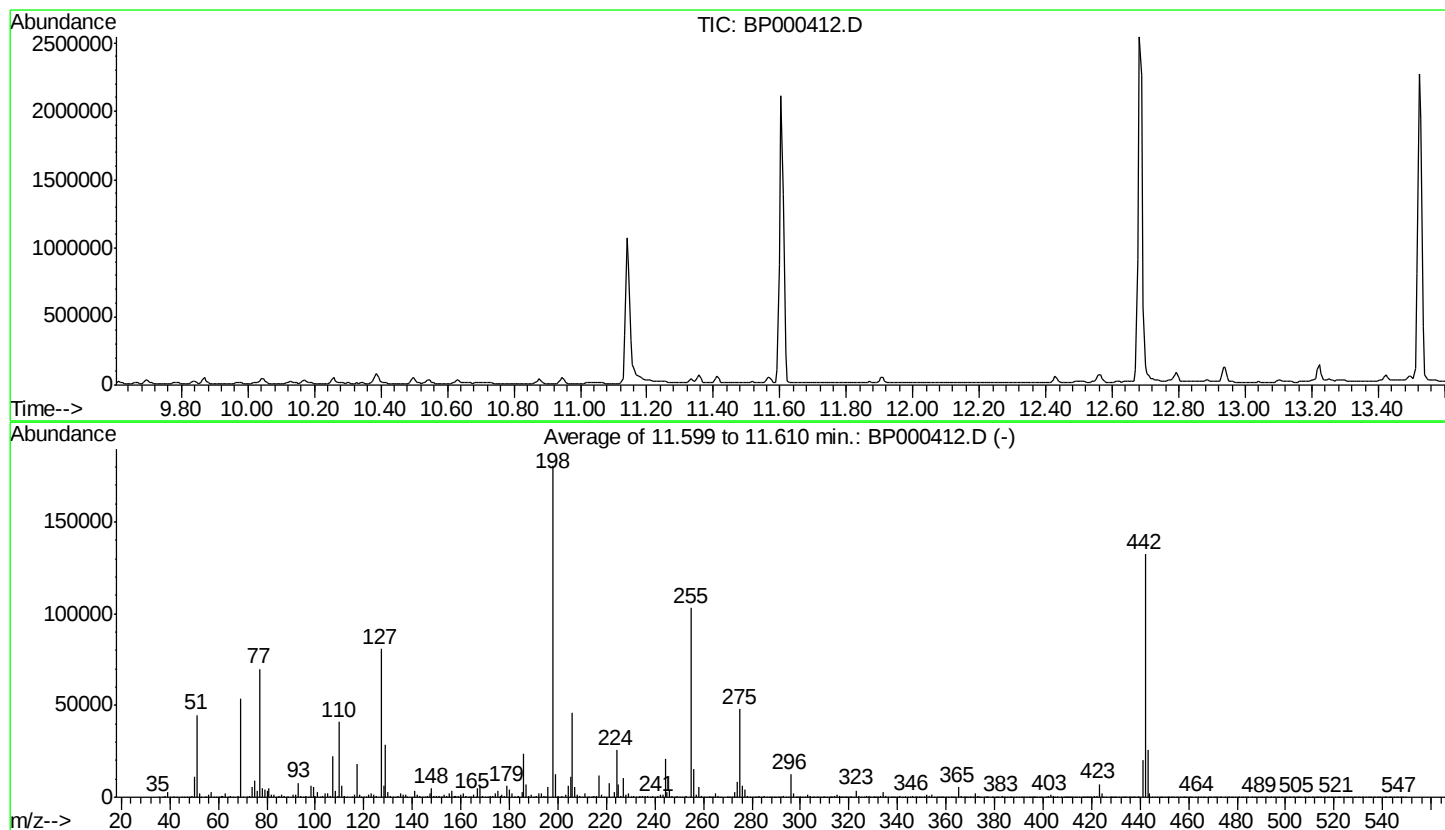

AutoFind: Scans 1617, 1618, 1619; Background Corrected with Scan 1610

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	24.8	44806	PASS
68	69	0.00	2	1.8	996	PASS
69	198	0.00	100	29.8	53842	PASS
70	69	0.00	2	0.7	372	PASS
127	198	10	80	44.6	80594	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	180682	PASS
199	198	5	9	6.8	12336	PASS
275	198	10	60	26.5	47957	PASS
365	198	1	100	2.9	5325	PASS
441	198	0.01	100	11.4	20543	PASS
442	198	50	100	73.3	132432	PASS
443	442	15	24	19.4	25633	PASS