


Data Path : Z:\SVOASRV\HPCHEM1\BNA_P\DATA\BP092619\
 Data File : BP000436.D
 Acq On : 26 Sep 2019 22:00
 Operator : JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP091619.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Sep 19 14:44:51 2019

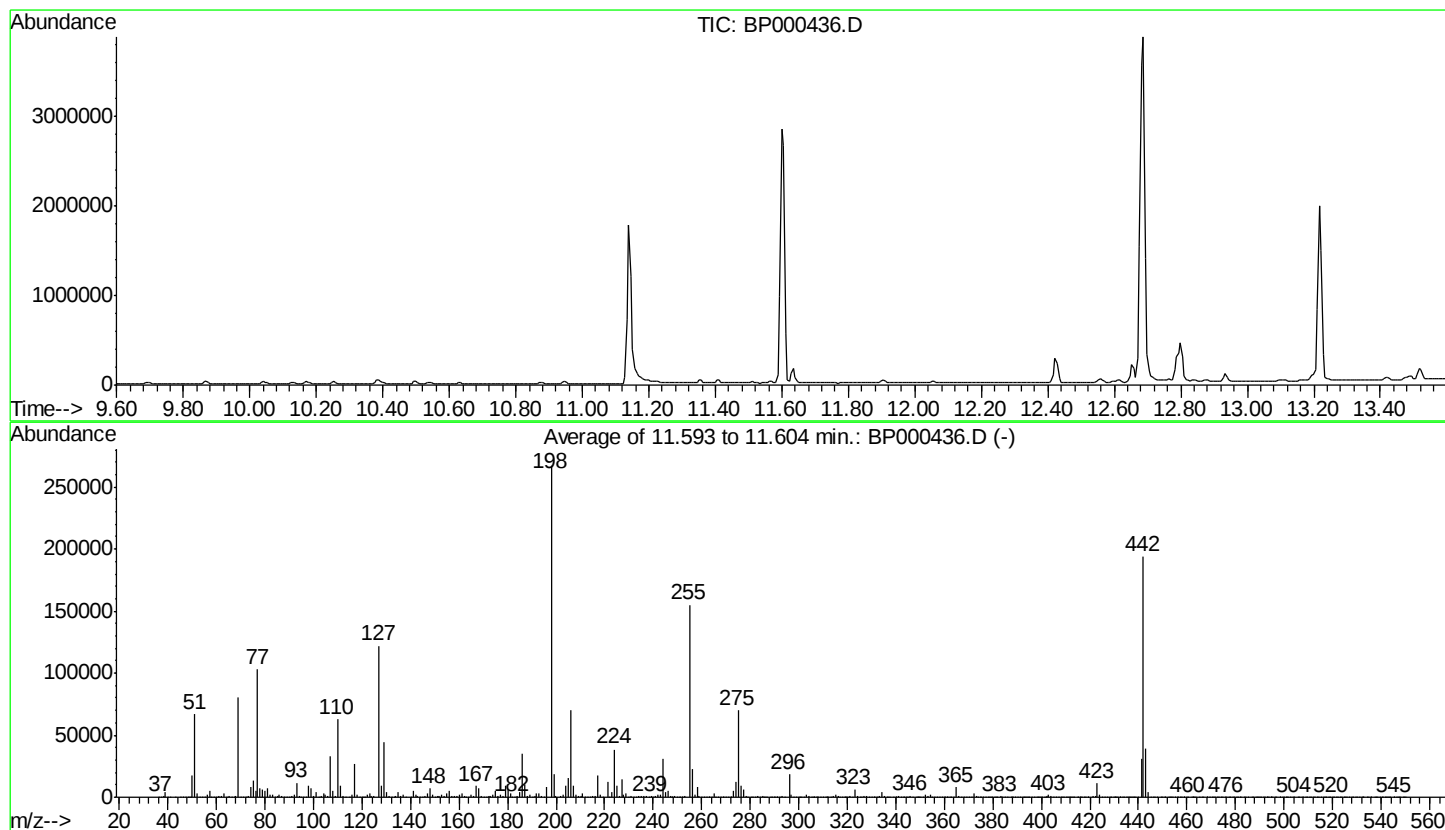

AutoFind: Scans 1616, 1617, 1618; Background Corrected with Scan 1610

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	25.0	66865	PASS
68	69	0.00	2	1.9	1501	PASS
69	198	0.00	100	30.0	80072	PASS
70	69	0.00	2	0.4	353	PASS
127	198	10	80	45.6	121963	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	267191	PASS
199	198	5	9	7.1	18891	PASS
275	198	10	60	26.2	70055	PASS
365	198	1	100	3.0	7986	PASS
441	198	0.01	100	11.5	30723	PASS
442	198	50	100	72.4	193489	PASS
443	442	15	24	20.2	39141	PASS