
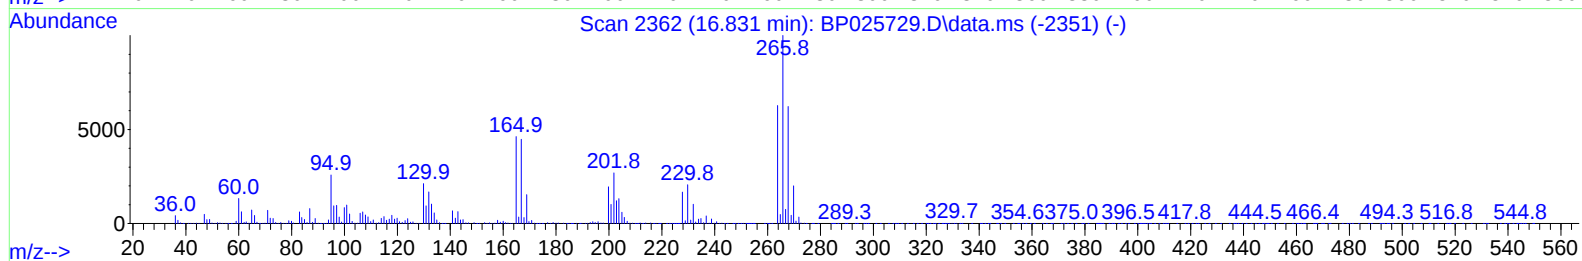
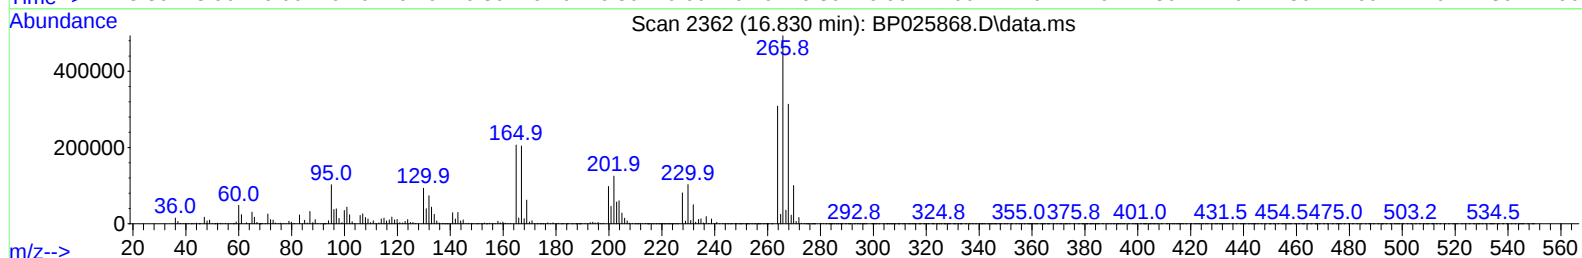


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP092625\
Data File : BP025868.D
Acq On : 26 Sep 2025 11:45
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 26 12:46:19 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP091225.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Sep 11 16:45:04 2025
Response via : Initial Calibration

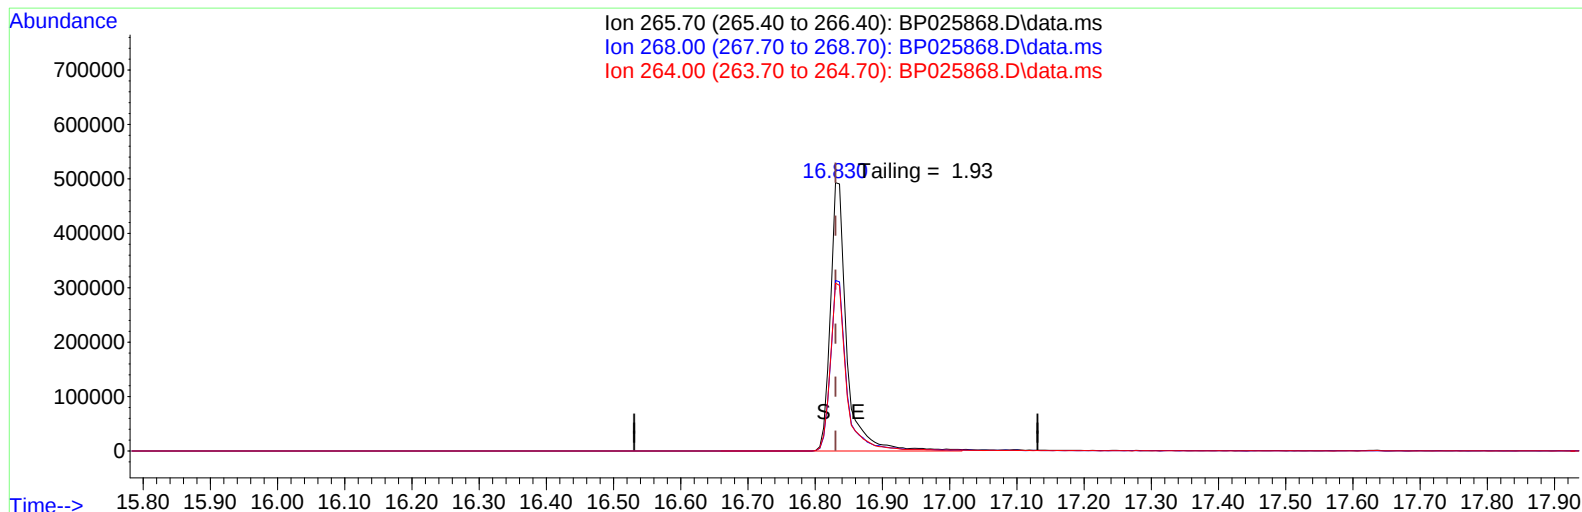

TIC: BP025868.D\data.ms

(70) Pentachlorophenol (C)




16.830min (-0.000) 86438.90 ng

response 820530

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.30	63.53
264.00	62.70	62.57
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP092625\
Data File : BP025868.D
Acq On : 26 Sep 2025 11:45
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 26 12:46:19 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP091225.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Sep 11 16:45:04 2025
Response via : Initial Calibration

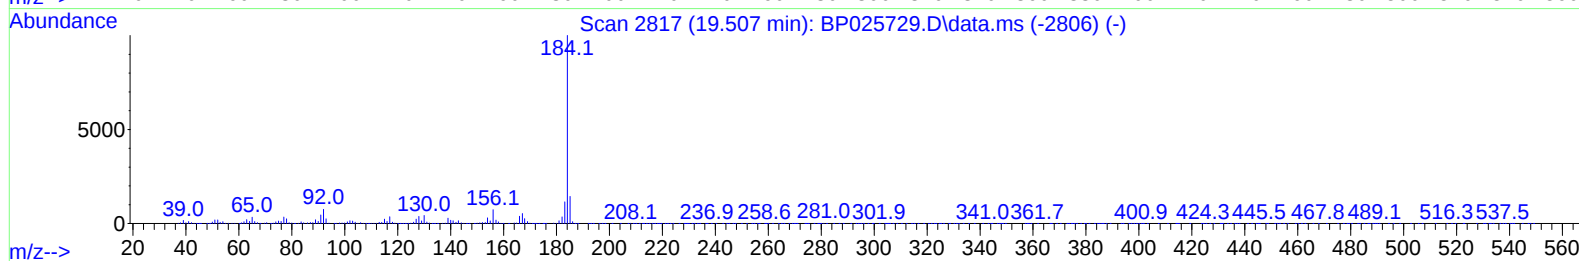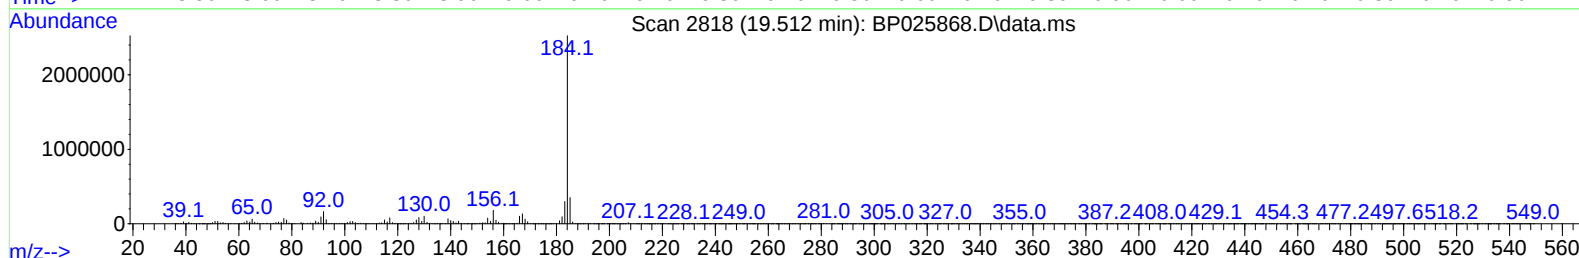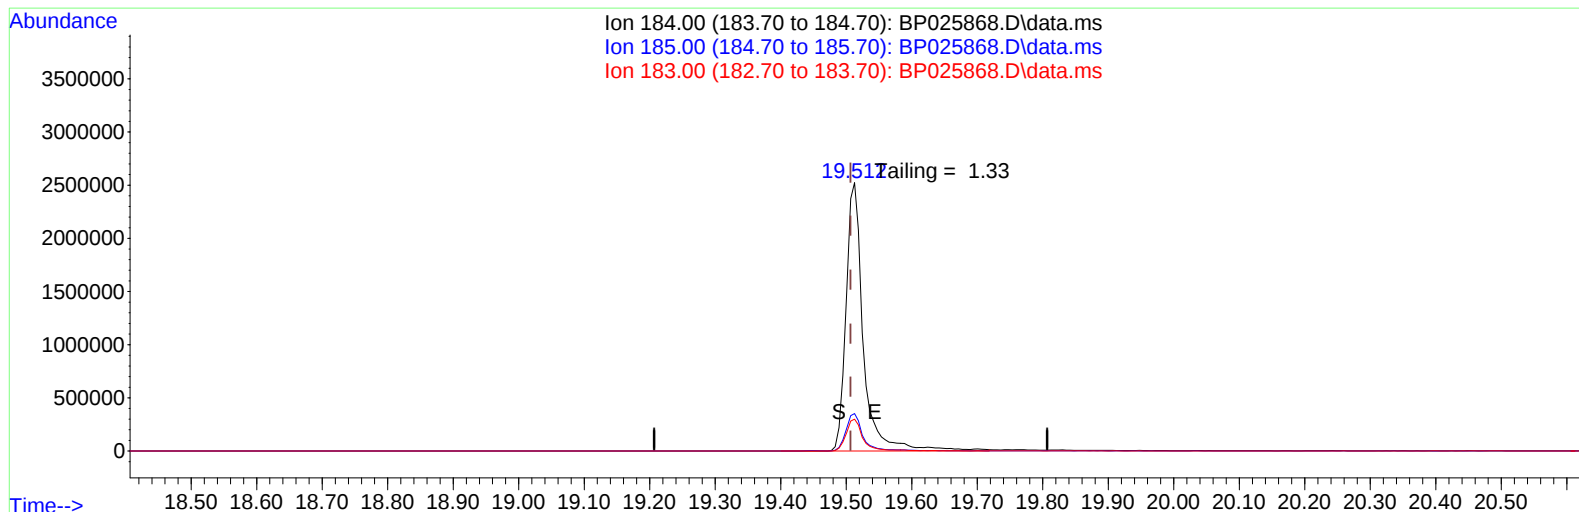

TIC: BP025868.D\data.ms

(77) Benzidine

19.512min (+ 0.006) 20581.93 ng

response 4520632

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.40	13.95
183.00	11.50	11.87
0.00	0.00	0.00