


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP092625\
Data File : BP025868.D
Acq On : 26 Sep 2025 11:45
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP091225.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Thu Sep 11 16:45:04 2025

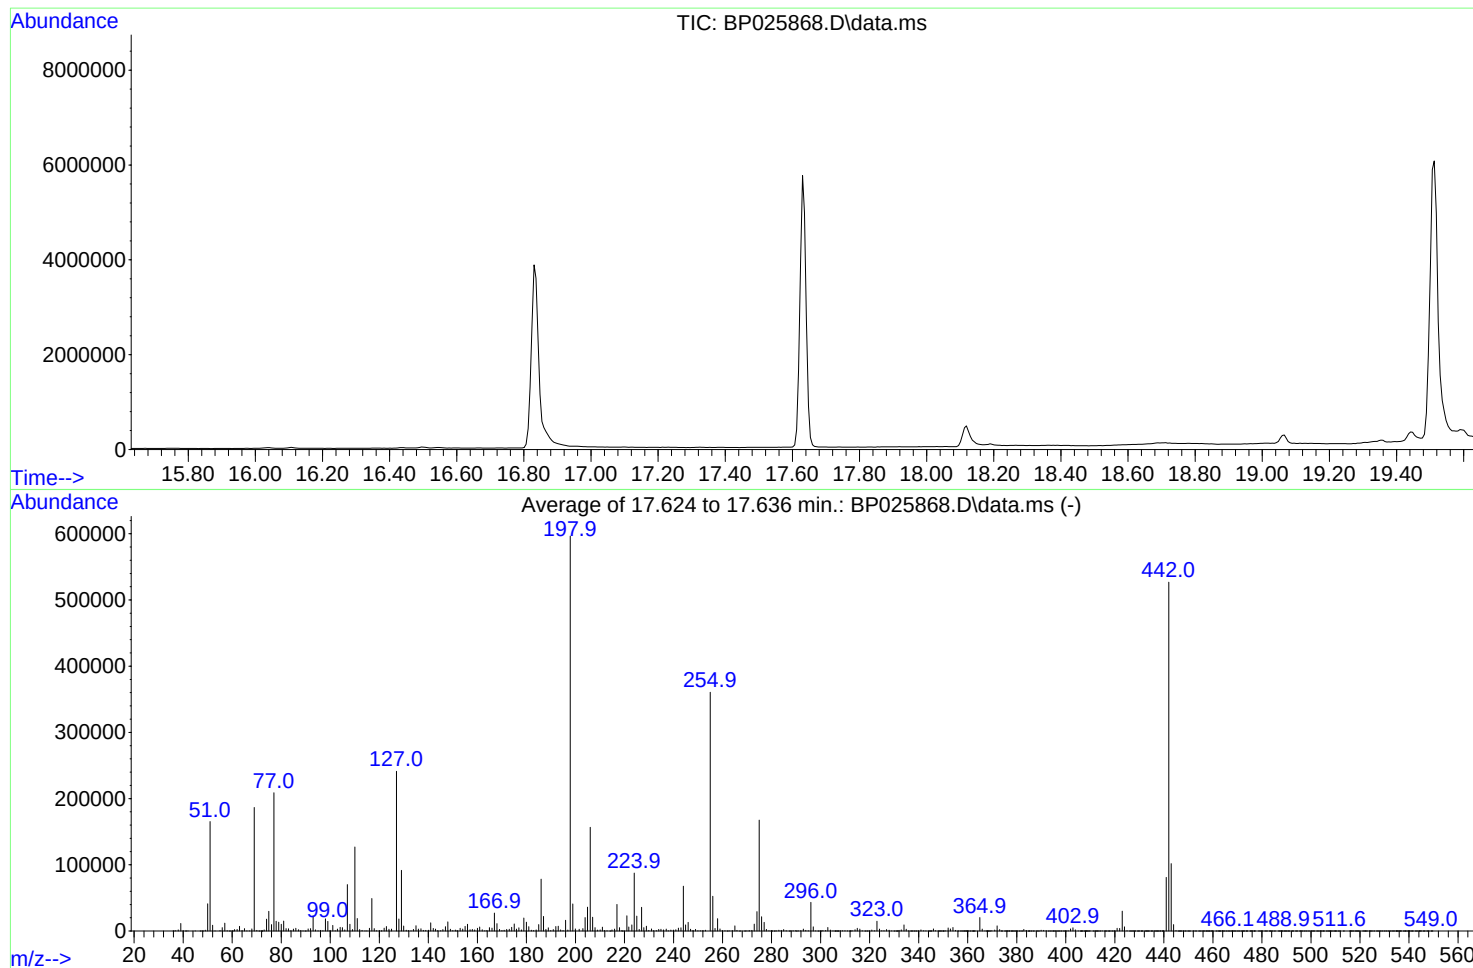

AutoFind: Scans 2497, 2498, 2499; Background Corrected with Scan 2483

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
68	69	0.00	2	1.7	3180	PASS
69	69	100	100	100.0	186622	PASS
70	69	0.00	2	0.5	915	PASS
197	198	0.00	2	0.2	1437	PASS
198	198	100	100	100.0	596418	PASS
199	198	5	9	6.8	40769	PASS
365	198	1	100	3.4	20211	PASS
441	443	0.01	150	79.6	80995	PASS
442	442	100	100	100.0	526912	PASS
443	442	15	24	19.3	101755	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
9/26/2025	BNA_P	<u>BP025868.D</u>
Compound Name	Response	Retention Time
DDT	2411381	20.807
DDD	44551	20.342
DDE	2064	19.907
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
46615	2457996	1.90

Instrument :
BNA_P
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP092625\
Data File : BP025868.D
Acq On : 26 Sep 2025 11:45
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: Sep 26 12:46:19 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP091225.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Sep 11 16:45:04 2025
Response via : Initial Calibration

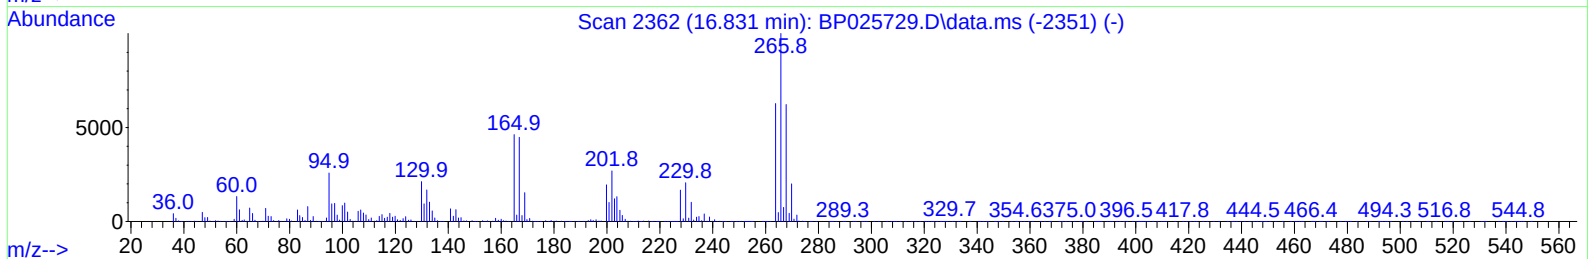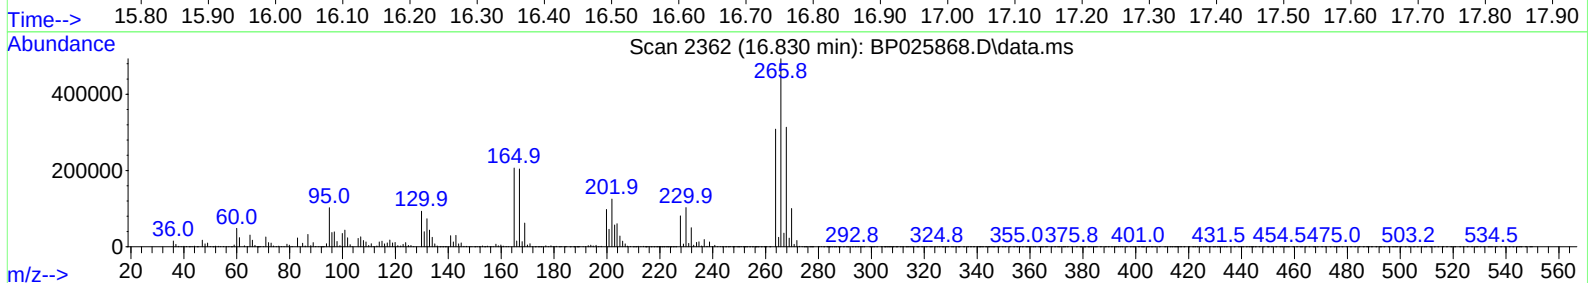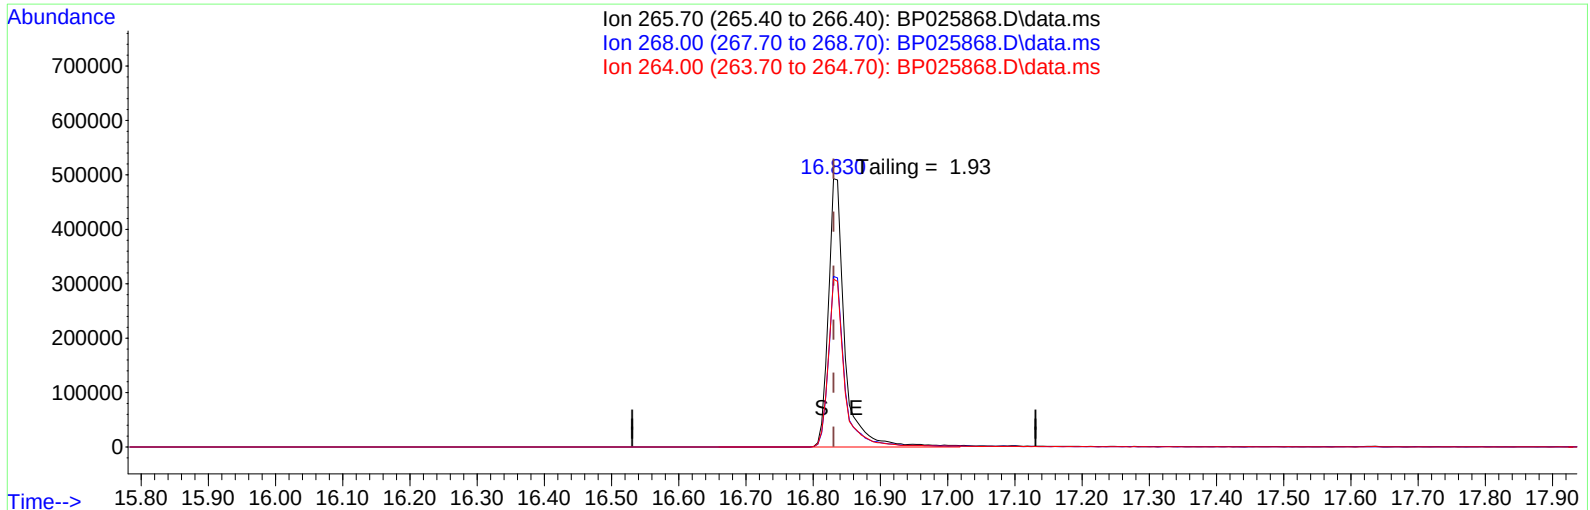

TIC: BP025868.D\data.ms

(70) Pentachlorophenol (C)

16.830min (-0.000) 86438.90 ng




response 820530

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.30	63.53
264.00	62.70	62.57
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP092625\
Data File : BP025868.D
Acq On : 26 Sep 2025 11:45
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: Sep 26 12:46:19 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP091225.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Sep 11 16:45:04 2025
Response via : Initial Calibration

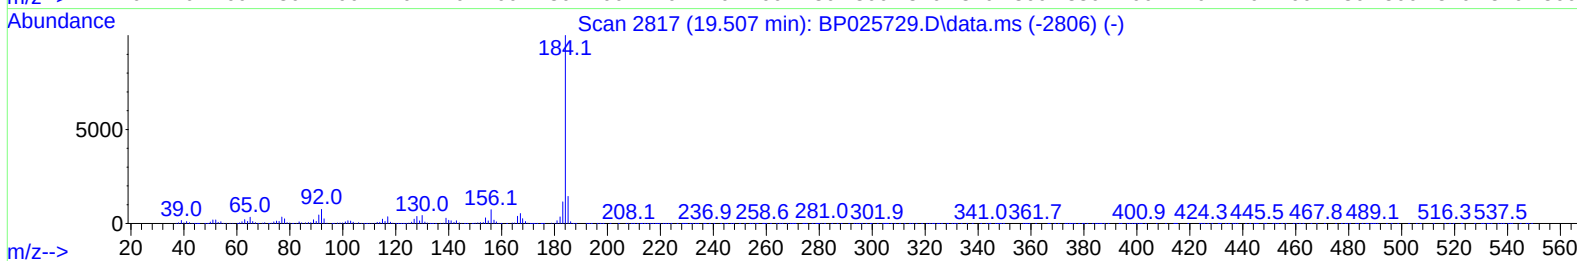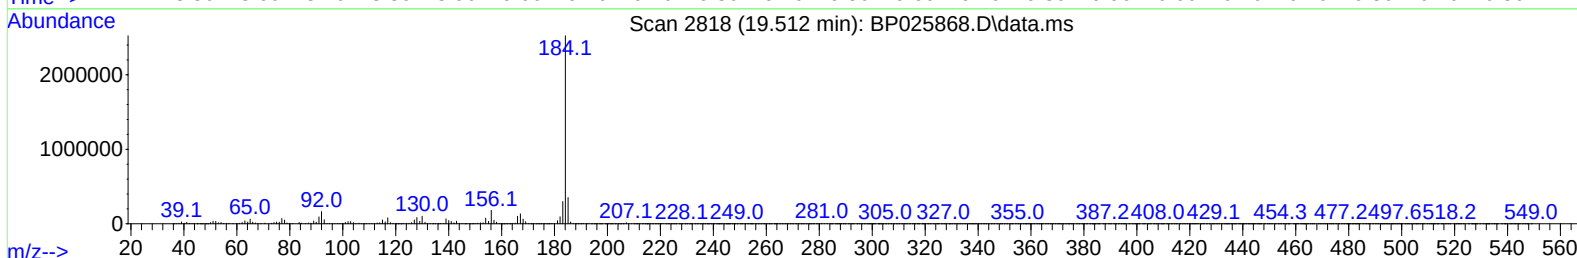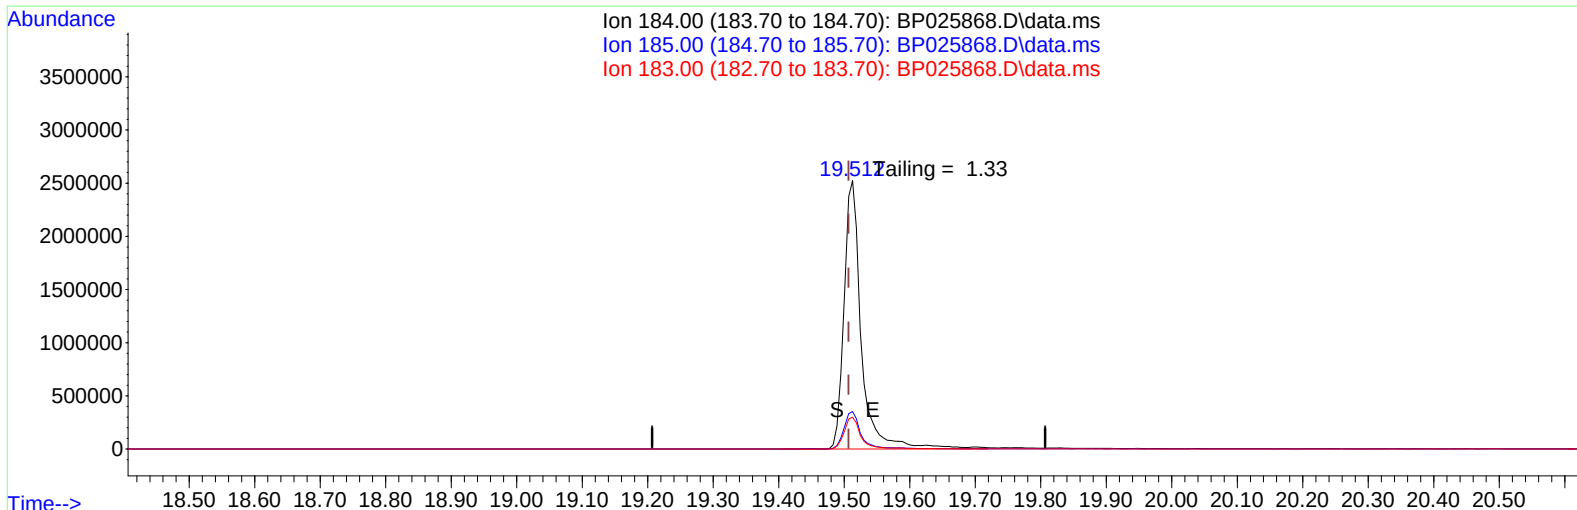

TIC: BP025868.D\data.ms

(77) Benzidine

19.512min (+ 0.006) 20581.93 ng

response 4520632

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.40	13.95
183.00	11.50	11.87
0.00	0.00	0.00