


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP092719\
 Data File : BP000448.D
 Acq On : 27 Sep 2019 11:05
 Operator : JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP091619.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Sep 19 14:44:51 2019

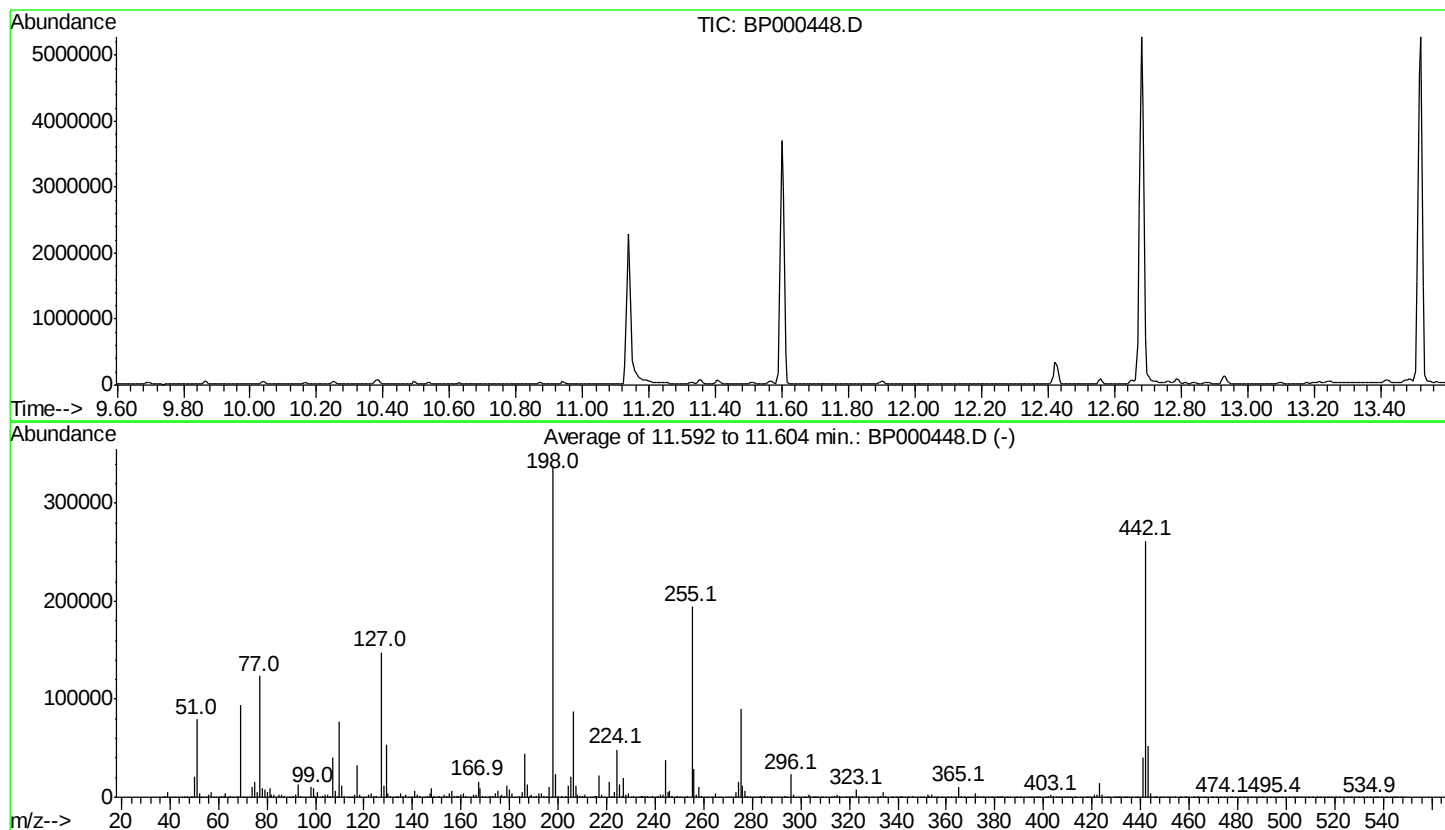

AutoFind: Scans 1616, 1617, 1618; Background Corrected with Scan 1606

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	23.4	79084	PASS
68	69	0.00	2	1.9	1793	PASS
69	198	0.00	100	27.9	94485	PASS
70	69	0.00	2	0.5	456	PASS
127	198	10	80	43.8	148207	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	338342	PASS
199	198	5	9	6.8	23067	PASS
275	198	10	60	26.5	89653	PASS
365	198	1	100	3.1	10564	PASS
441	198	0.01	100	12.1	40843	PASS
442	198	50	100	77.3	261484	PASS
443	442	15	24	20.1	52542	PASS