
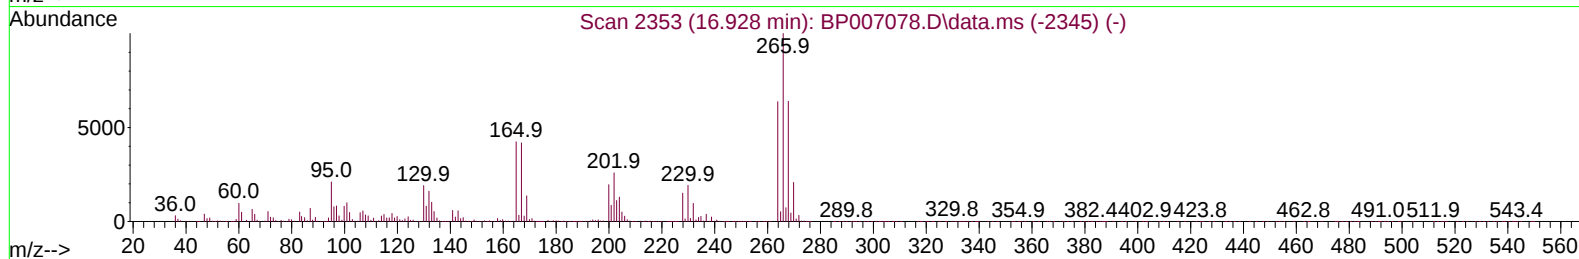
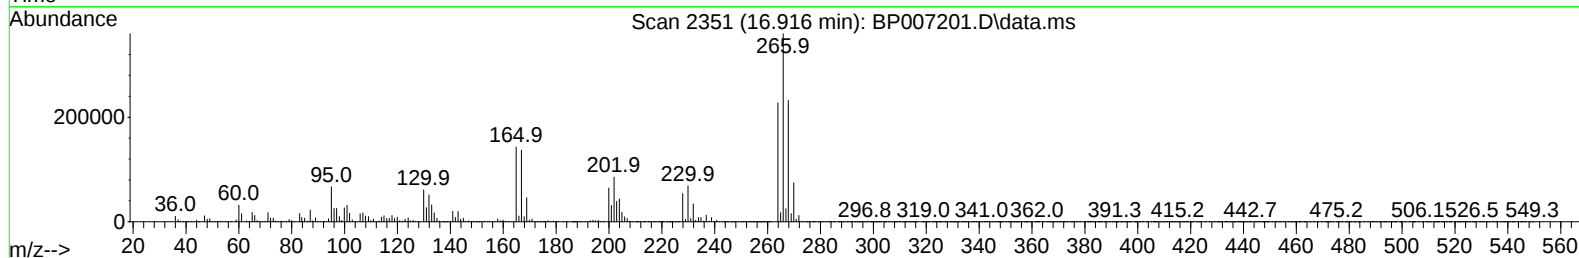


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP092721\
Data File : BP007201.D
Acq On : 27 Sep 2021 12:26
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 27 13:29:44 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP092121.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Sep 23 11:17:25 2021
Response via : Initial Calibration

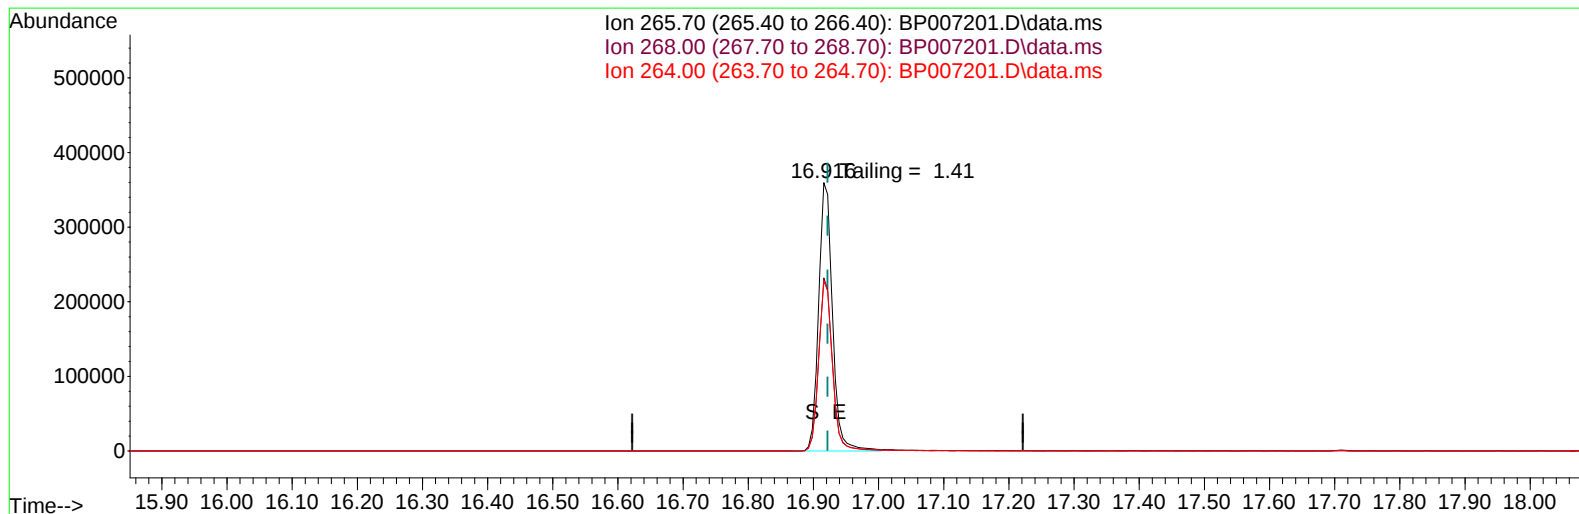




TIC: BP007201.D\data.ms

(70) Pentachlorophenol (C)**16.916min (-0.006) 1428218.80 ng****response 537177**

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.50	64.54
264.00	62.90	63.26
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP092721\
 Data File : BP007201.D
 Acq On : 27 Sep 2021 12:26
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 27 13:29:44 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP092121.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Sep 23 11:17:25 2021
 Response via : Initial Calibration

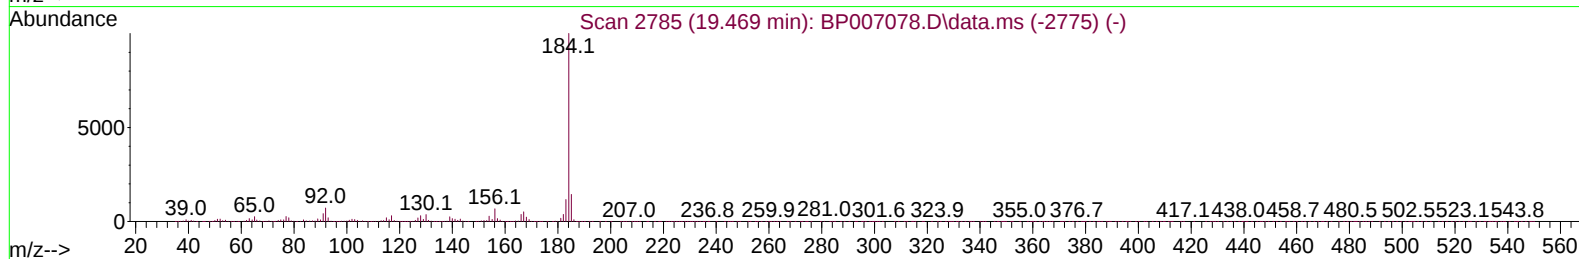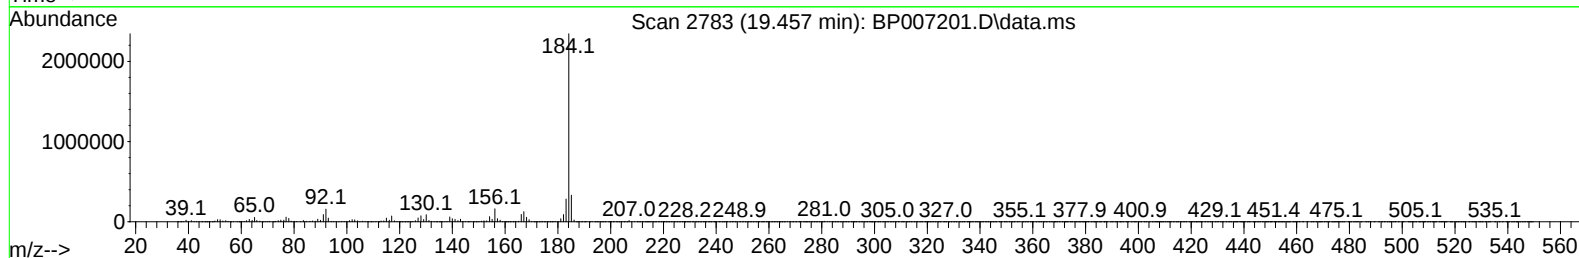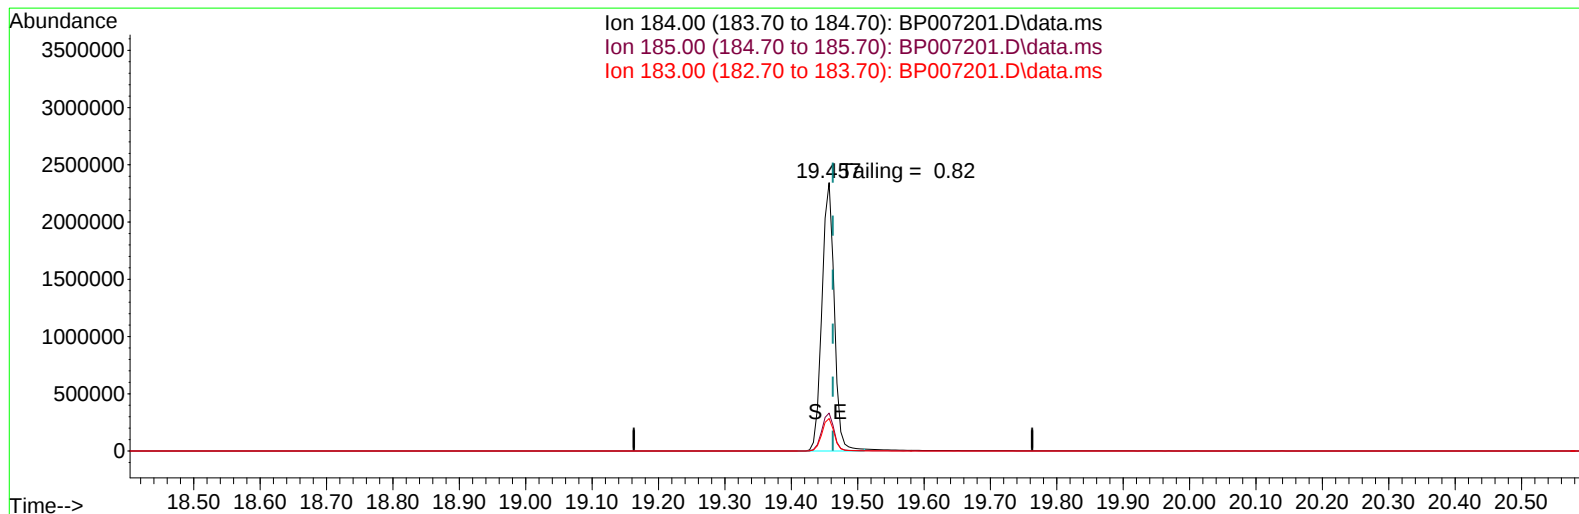

TIC: BP007201.D\data.ms

(77) Benzidine**19.457min (-0.006) 743834.38 ng****response 3063132**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.70	14.16
183.00	11.90	12.09
0.00	0.00	0.00