

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP092721\
 Data File : BP007203.D
 Acq On : 27 Sep 2021 13:39
 Operator : CG/JU
 Sample : PB139374BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 PB139374BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP092121.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BP007203.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.458	396	403	420	rBV	2420688	3618281	22.95%	5.943%
2	7.052	666	674	686	rBV	2786071	4548023	28.84%	7.470%
3	7.881	807	815	823	rBV	938943	1487434	9.43%	2.443%
4	9.040	1004	1012	1031	rBV	1819967	3123951	19.81%	5.131%
5	10.681	1283	1291	1306	rBV	1199622	2043058	12.96%	3.356%
6	13.140	1701	1709	1723	rBV	6725513	10328934	65.50%	16.965%
7	14.516	1936	1943	1954	rBV	1806812	2665682	16.91%	4.378%
8	16.010	2189	2197	2217	rBV	6316990	9370550	59.43%	15.391%
9	17.269	2403	2411	2423	rBV	2015772	2949612	18.71%	4.845%
10	19.827	2840	2846	2851	rBV	12994339	15768243	100.00%	25.899%
11	21.357	3101	3106	3115	rBV	1996912	2644320	16.77%	4.343%
12	23.768	3510	3516	3525	rVB2	1133396	2335725	14.81%	3.836%




Sum of corrected areas: 60883813

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP092721\
Data File : BP007203.D
Acq On : 27 Sep 2021 13:39
Operator : CG/JU
Sample : PB139374BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB139374BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP092121.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

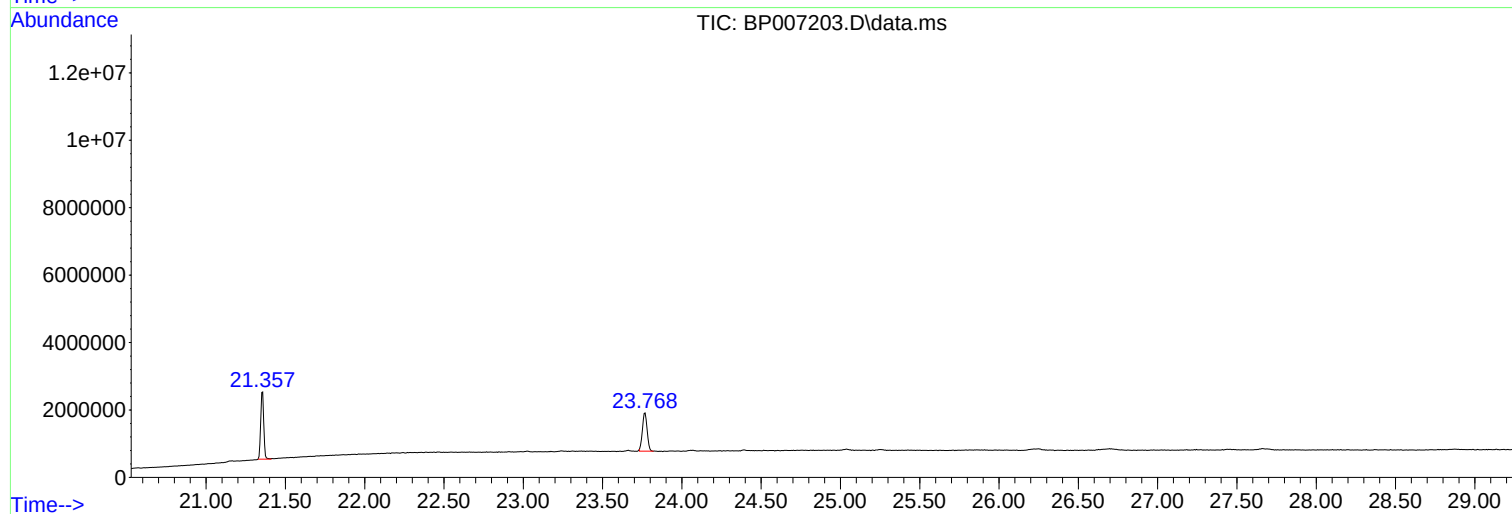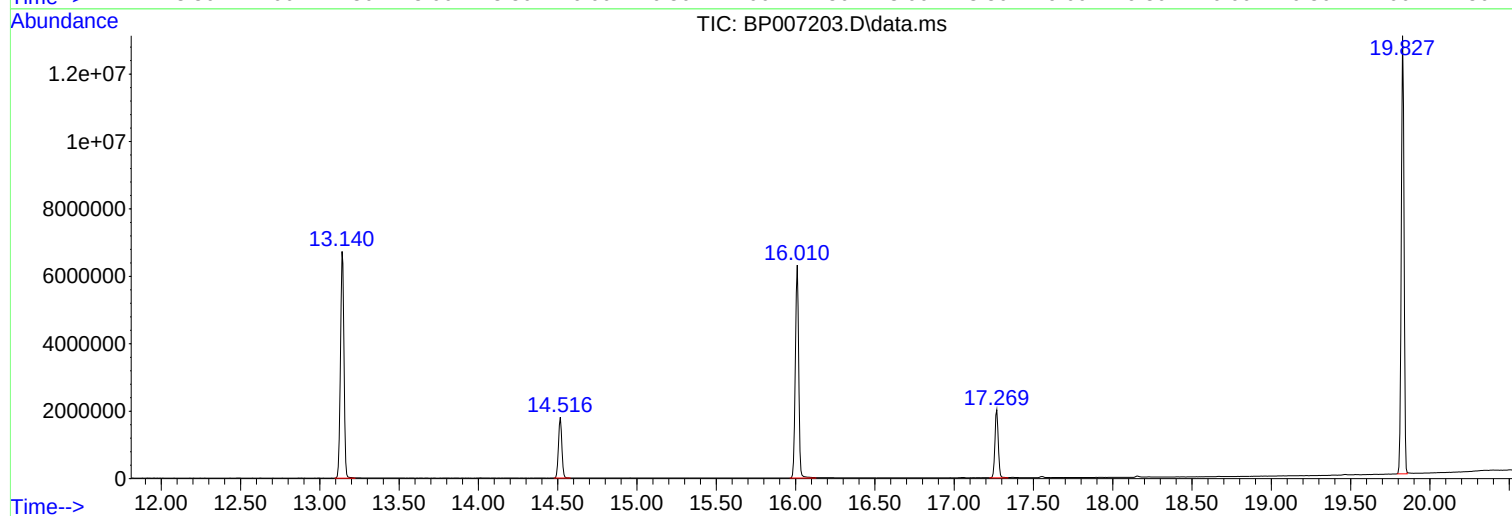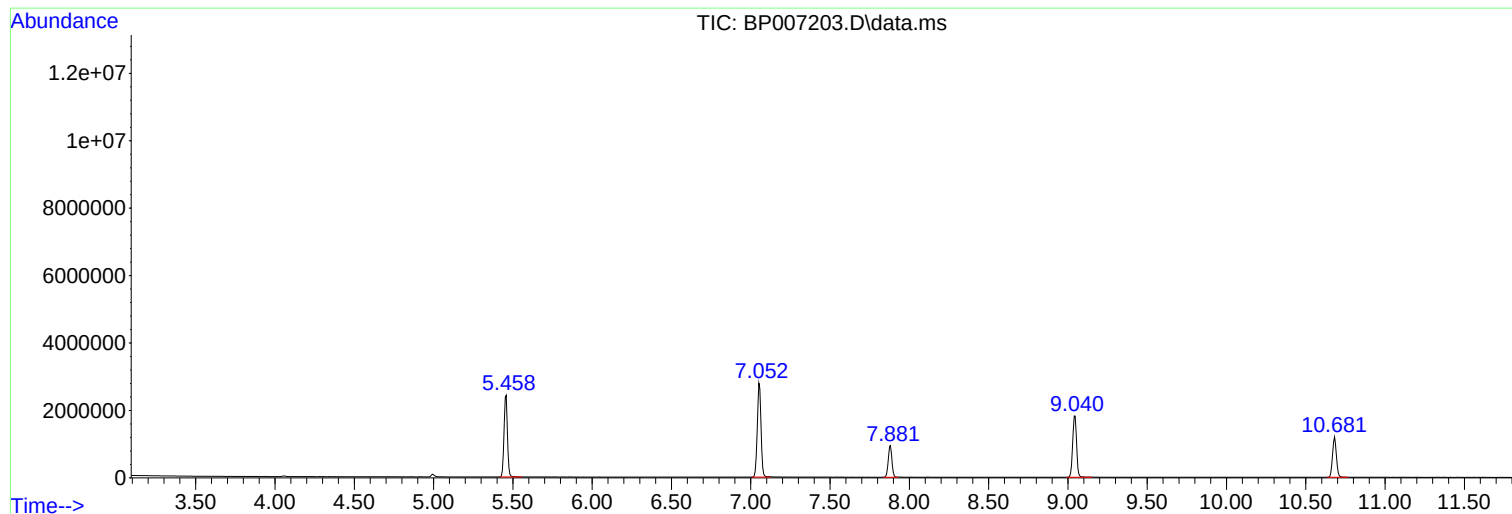

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP092721\
Data File : BP007203.D
Acq On : 27 Sep 2021 13:39
Operator : CG/JU
Sample : PB139374BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB139374BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP092121.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP092721\
Data File : BP007203.D
Acq On : 27 Sep 2021 13:39
Operator : CG/JU
Sample : PB139374BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB139374BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP092121.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------