

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP092721\
 Data File : BP007214.D
 Acq On : 27 Sep 2021 20:06
 Operator : CG/JU
 Sample : M3935-01 5X
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 TP-2

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP092121.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BP007214.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.458	397	403	416	rBV	647650	954136	27.07%	3.822%
2	7.058	667	675	688	rBV	591219	983308	27.90%	3.938%
3	7.881	808	815	824	rBV	1066642	1673582	47.49%	6.703%
4	9.046	1006	1013	1030	rBV	365336	628055	17.82%	2.516%
5	10.481	1250	1257	1272	rBV2	48989	130032	3.69%	0.521%
6	10.681	1283	1291	1306	rBV	1357926	2433586	69.05%	9.747%
7	13.140	1702	1709	1719	rBV	1152961	1719113	48.78%	6.886%
8	14.516	1935	1943	1950	rBV	2239268	3295515	93.51%	13.200%
9	14.581	1951	1954	1962	rVB2	28826	46178	1.31%	0.185%
10	15.563	2117	2121	2127	rBV2	23221	39442	1.12%	0.158%
11	16.010	2191	2197	2209	rBV	794085	1201559	34.09%	4.813%
12	17.269	2405	2411	2416	rBV	2388029	3524296	100.00%	14.116%
13	17.310	2416	2418	2424	rVB	194102	238542	6.77%	0.955%
14	17.404	2430	2434	2439	rVB	51789	70299	1.99%	0.282%
15	19.280	2749	2753	2758	rBV	235754	303661	8.62%	1.216%
16	19.627	2809	2812	2821	rVB	229654	349844	9.93%	1.401%
17	19.822	2841	2845	2850	rBV	1493693	1811569	51.40%	7.256%
18	21.351	3101	3105	3110	rVB	2022938	2679165	76.02%	10.731%
19	23.768	3511	3516	3524	rVB2	1407185	2884938	81.86%	11.555%




Sum of corrected areas: 24966820

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP092721\
Data File : BP007214.D
Acq On : 27 Sep 2021 20:06
Operator : CG/JU
Sample : M3935-01 5X
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
TP-2

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP092121.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

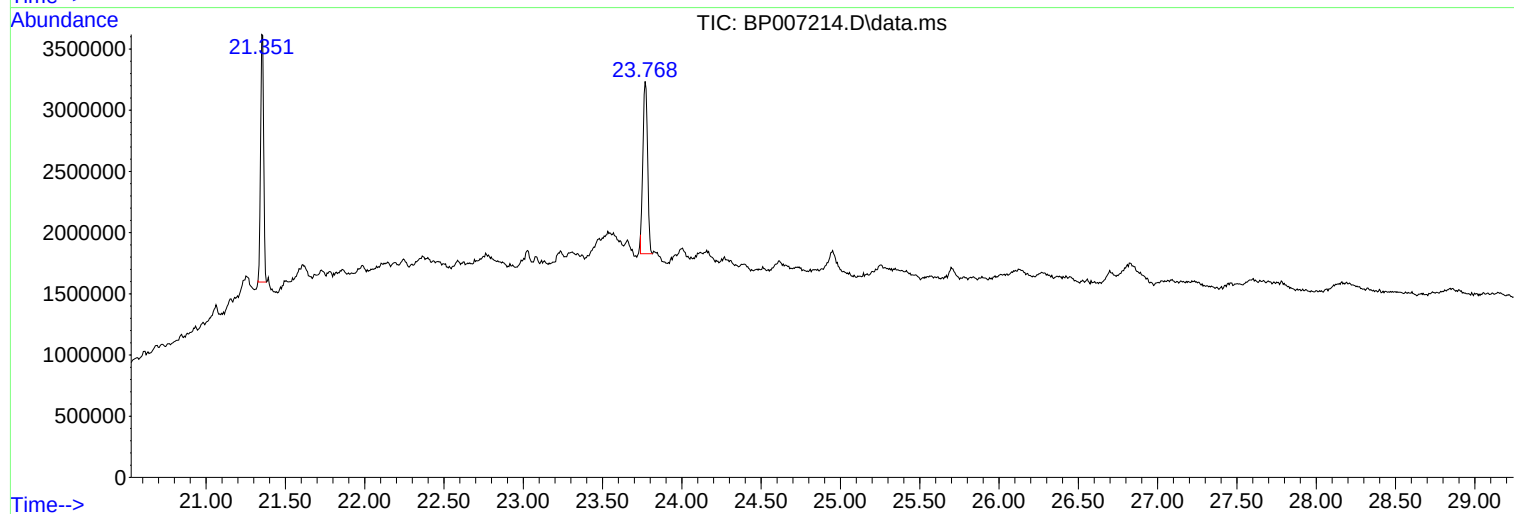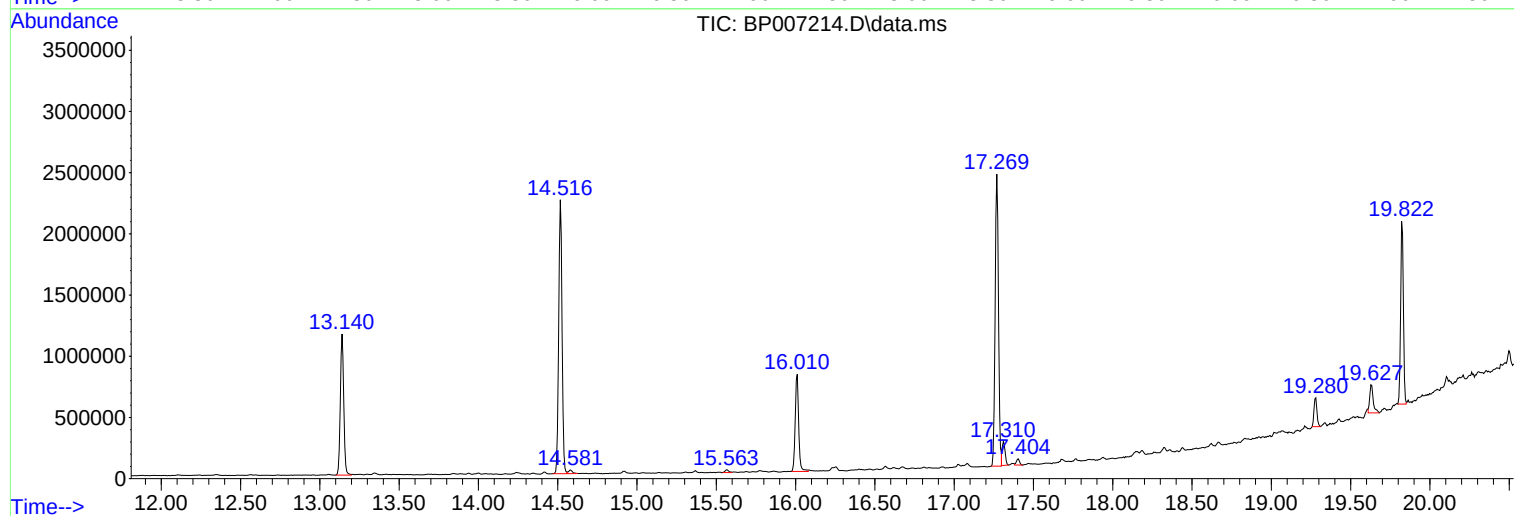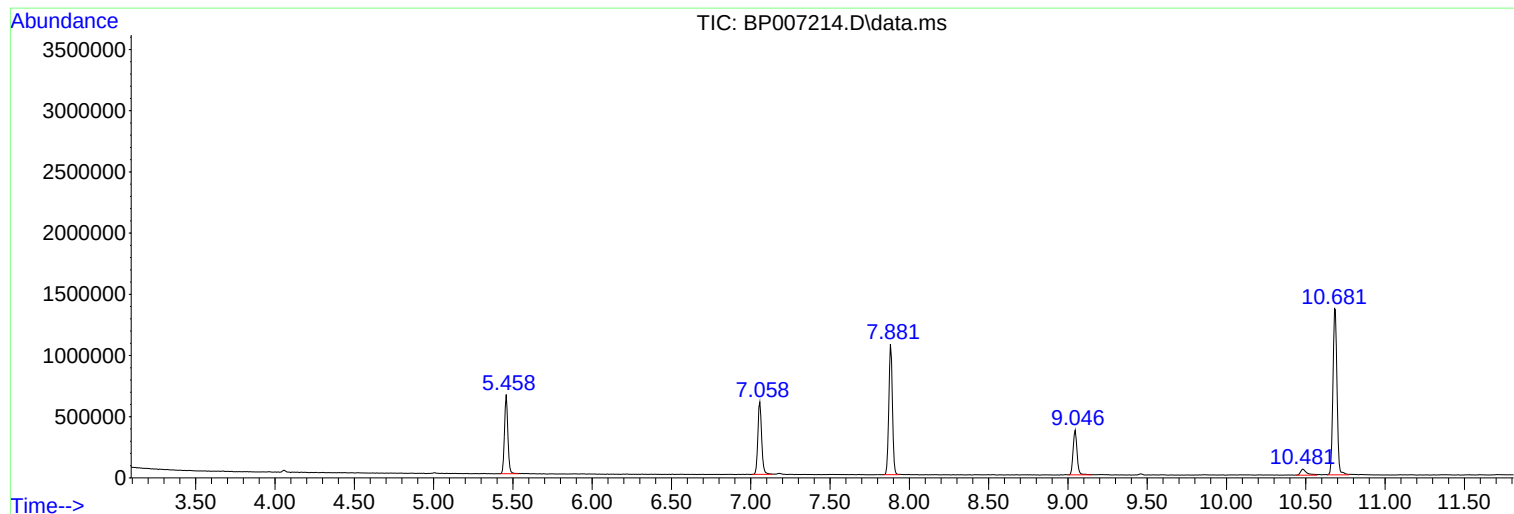

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP092721\
Data File : BP007214.D
Acq On : 27 Sep 2021 20:06
Operator : CG/JU
Sample : M3935-01 5X
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
TP-2

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP092121.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP092721\
Data File : BP007214.D
Acq On : 27 Sep 2021 20:06
Operator : CG/JU
Sample : M3935-01 5X
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
TP-2

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP092121.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
