

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP092721\
 Data File : BP007215.D
 Acq On : 27 Sep 2021 20:40
 Operator : CG/JU
 Sample : M3947-01 5X
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 CL-02-092421

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP092121.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BP007215.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.458	393	403	414	rBV	458723	716310	18.73%	3.082%
2	7.058	666	675	688	rBV	448040	763700	19.97%	3.286%
3	7.881	807	815	823	rBV	739451	1177410	30.78%	5.066%
4	9.046	1006	1013	1022	rBV	249857	428630	11.21%	1.844%
5	10.475	1250	1256	1271	rBV2	89180	203949	5.33%	0.878%
6	10.681	1283	1291	1304	rBV	1045435	1828279	47.80%	7.867%
7	13.140	1701	1709	1721	rBV	905384	1337462	34.97%	5.755%
8	14.516	1936	1943	1956	rBV	1972793	2882698	75.37%	12.404%
9	16.010	2190	2197	2204	rBV	792279	1185424	30.99%	5.101%
10	17.269	2404	2411	2422	rBV	2713643	3824663	100.00%	16.457%
11	17.934	2521	2524	2530	rBV3	37037	50738	1.33%	0.218%
12	19.063	2714	2716	2722	rVB5	65579	79513	2.08%	0.342%
13	19.822	2841	2845	2850	rBV	1892989	2254321	58.94%	9.700%
14	21.351	3101	3105	3111	rVB	2598771	3332097	87.12%	14.337%
15	23.769	3511	3516	3524	rVB2	1564837	3175358	83.02%	13.663%


Sum of corrected areas: 23240552

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP092721\
Data File : BP007215.D
Acq On : 27 Sep 2021 20:40
Operator : CG/JU
Sample : M3947-01 5X
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
CL-02-092421

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP092121.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

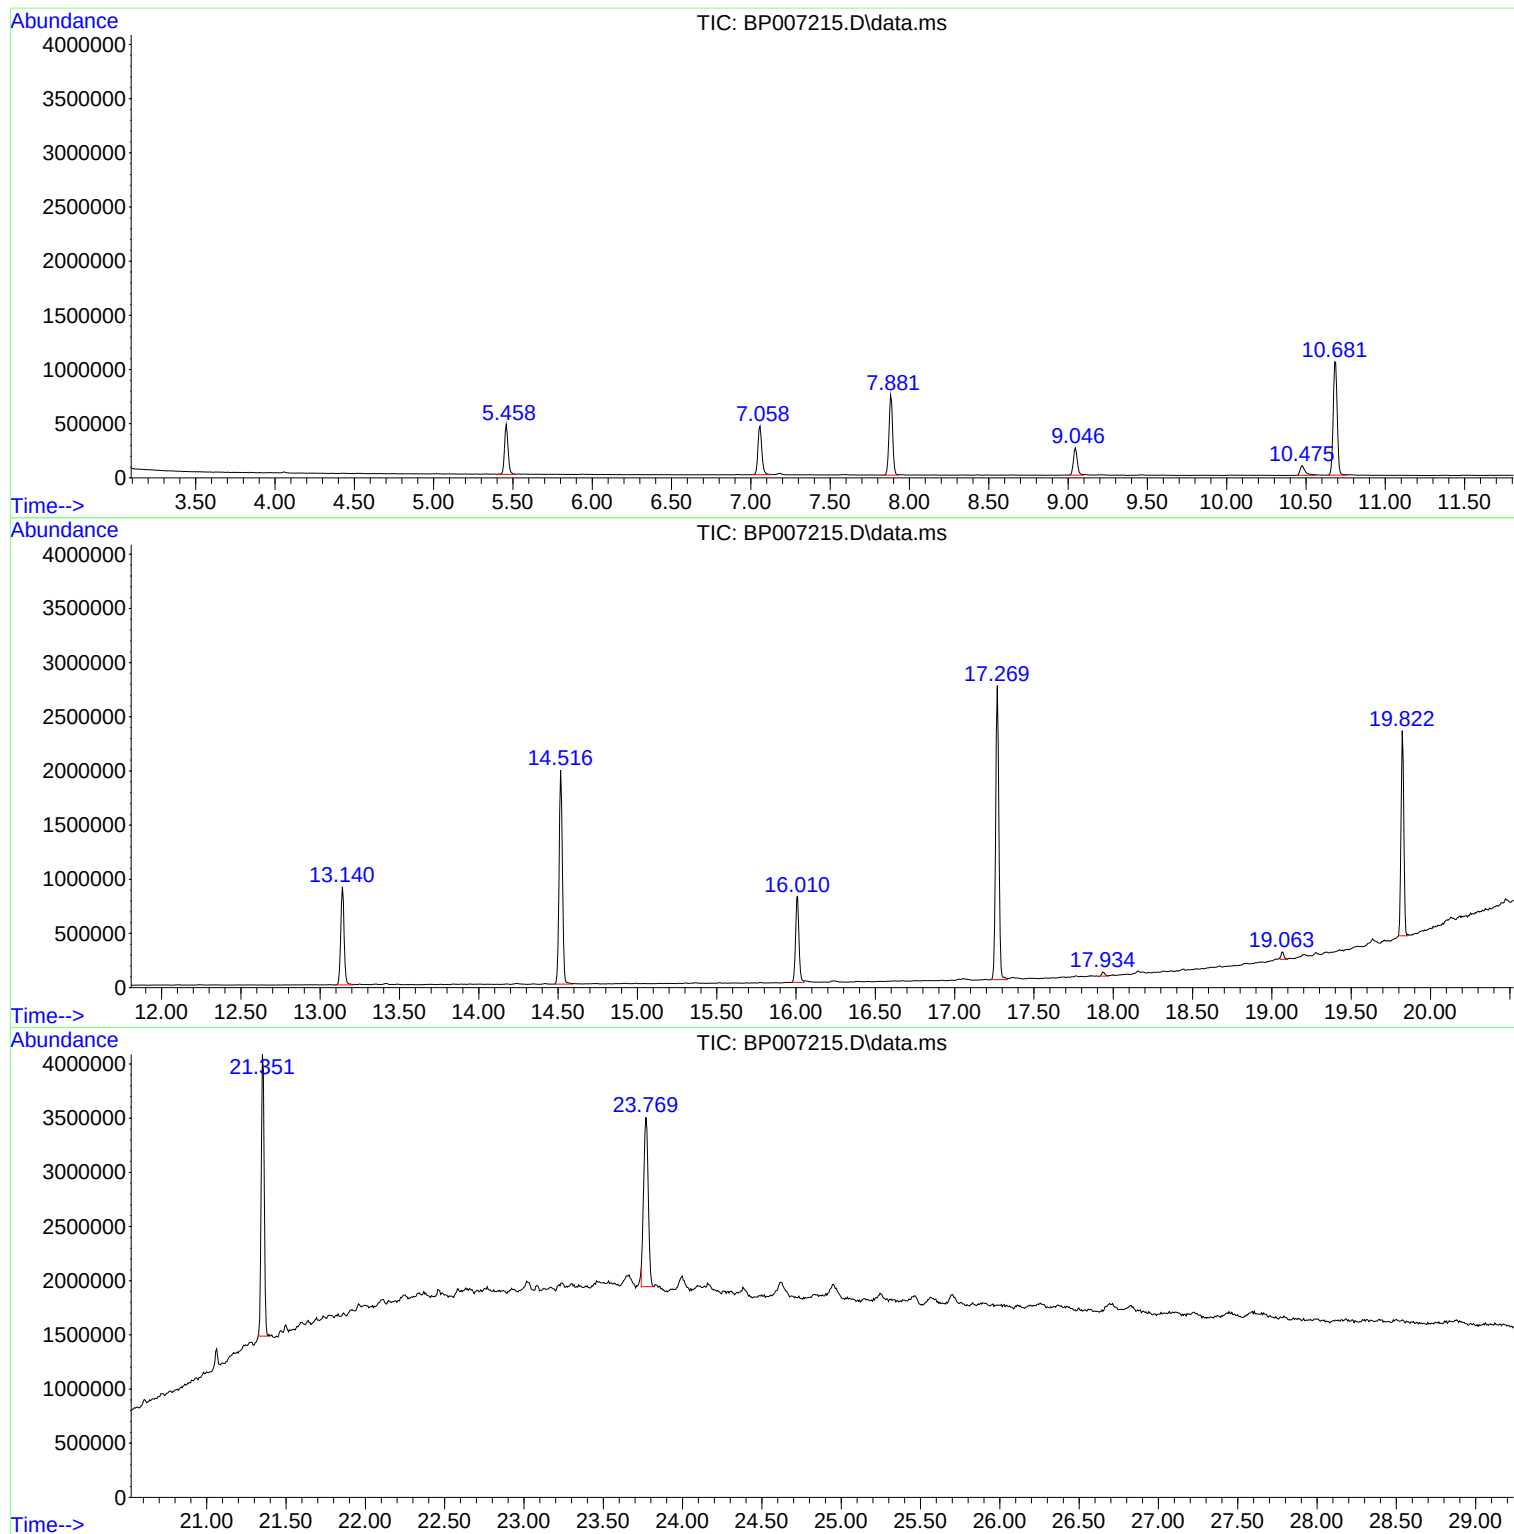

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP092721\
Data File : BP007215.D
Acq On : 27 Sep 2021 20:40
Operator : CG/JU
Sample : M3947-01 5X
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
CL-02-092421









Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP092121.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Ethanol, 2-(2-butoxyethoxy)- Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
10.475	2.23 ng	203949	Naphthalene-d8	10.687

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Ethanol, 2-(2-butoxyethoxy)-	162	C8H18O3	000112-34-5	91
2			Ethanol, 1-(2-butoxyethoxy)-	162	C8H18O3	054446-78-5	86
3			Ethylene glycol monoisobutyl ether	118	C6H14O2	004439-24-1	74
4			Di-sec-Butyl ether	130	C8H18O	006863-58-7	50
5			3,3-Dimethylbutane-2-ol	102	C6H14O	000464-07-3	50

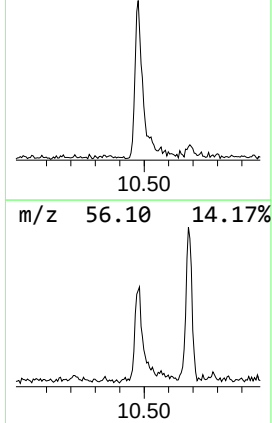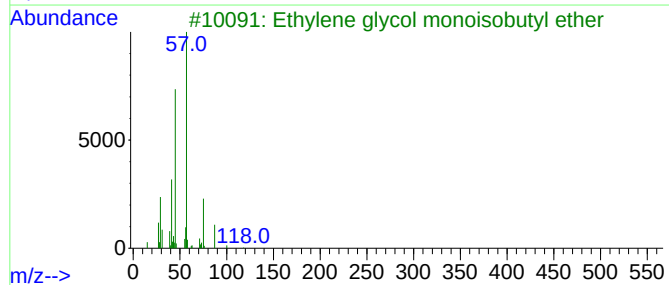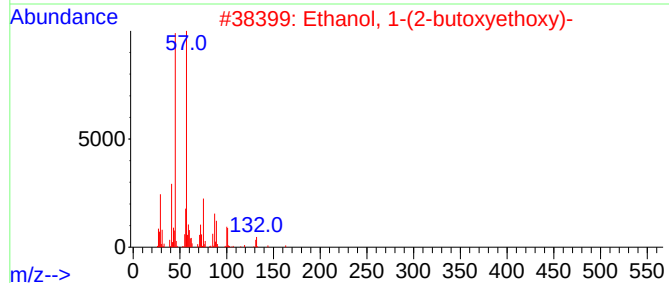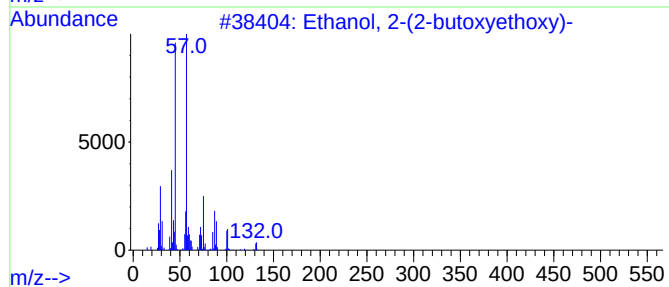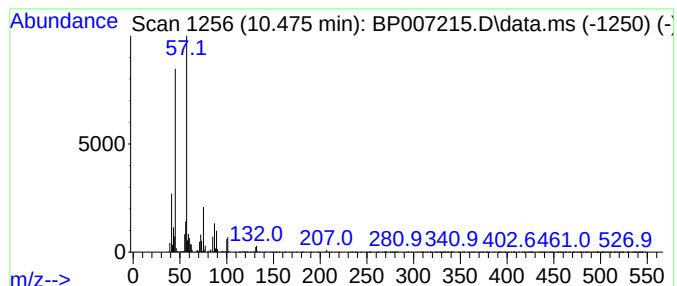

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP092721\
Data File : BP007215.D
Acq On : 27 Sep 2021 20:40
Operator : CG/JU
Sample : M3947-01 5X
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
CL-02-092421

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP092121.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Ethanol, 2-(2-b...	10.475	2.2	ng	203949	2	10.687	1828280	20.0