
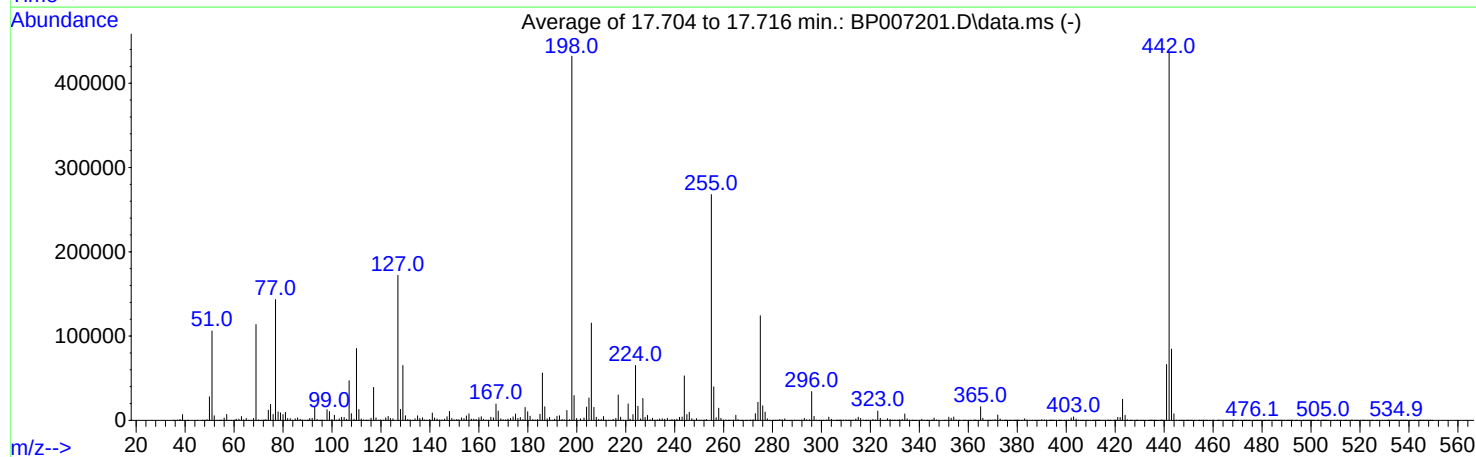


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP092721\
 Data File : BP007201.D
 Acq On : 27 Sep 2021 12:26
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP092121.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Sep 23 11:17:25 2021

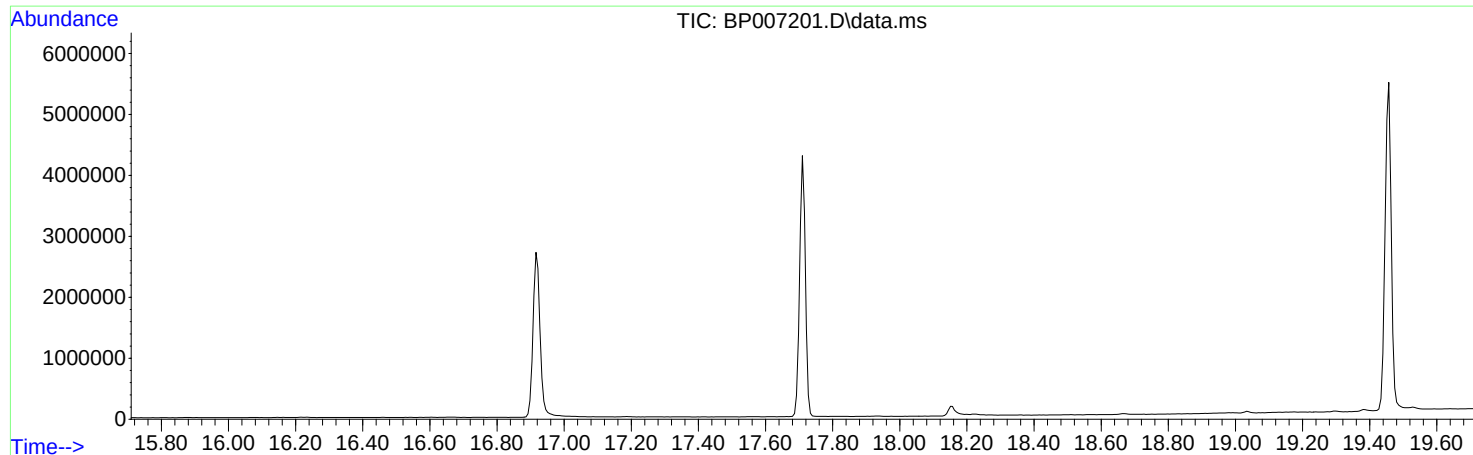




AutoFind: Scans 2485, 2486, 2487; Background Corrected with Scan 2478

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	24.6	106221	PASS
68	69	0.00	2	2.0	2222	PASS
69	198	0.00	100	26.3	113788	PASS
70	69	0.00	2	0.5	520	PASS
127	198	10	80	39.8	171981	PASS
197	198	0.00	2	0.2	869	PASS
198	198	100	100	100.0	432074	PASS
199	198	5	9	6.8	29360	PASS
275	198	10	60	28.7	124131	PASS
365	198	1	100	3.7	16093	PASS
441	198	0.01	100	15.3	66303	PASS
442	442	100	100	100.0	436455	PASS
443	442	15	24	19.4	84643	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP092721\
Data File : BP007201.D
Acq On : 27 Sep 2021 12:26
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: Sep 27 13:29:44 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP092121.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Sep 23 11:17:25 2021
Response via : Initial Calibration

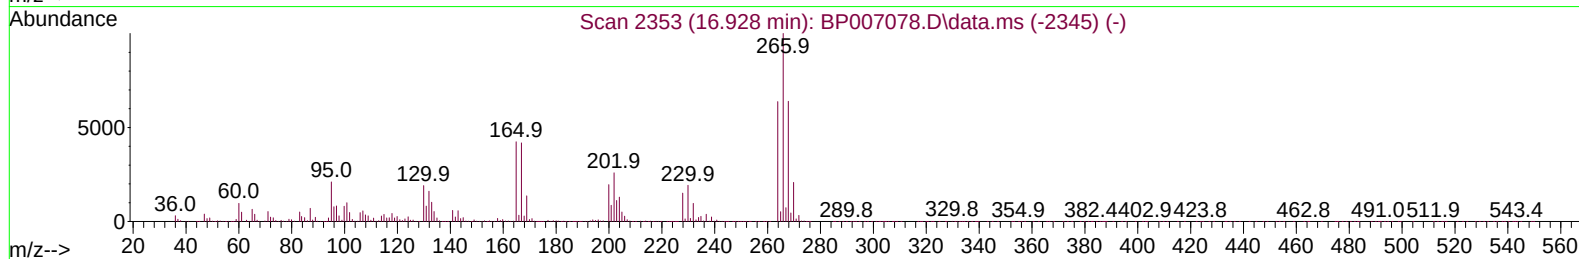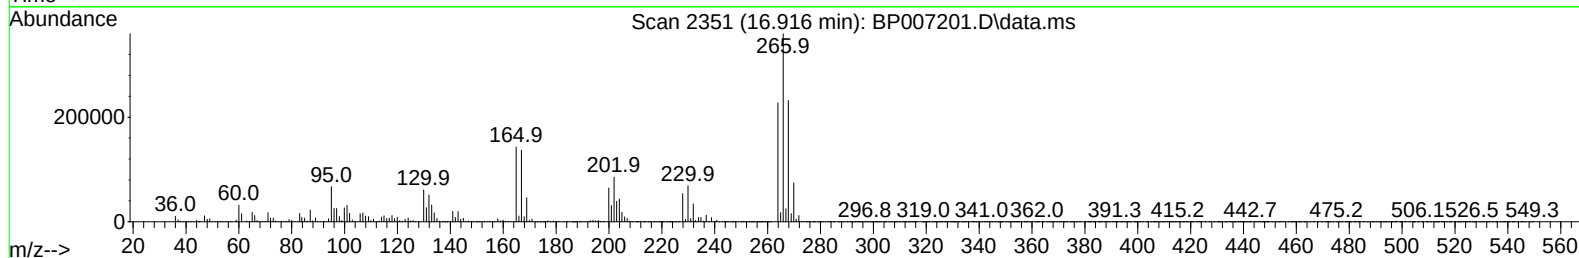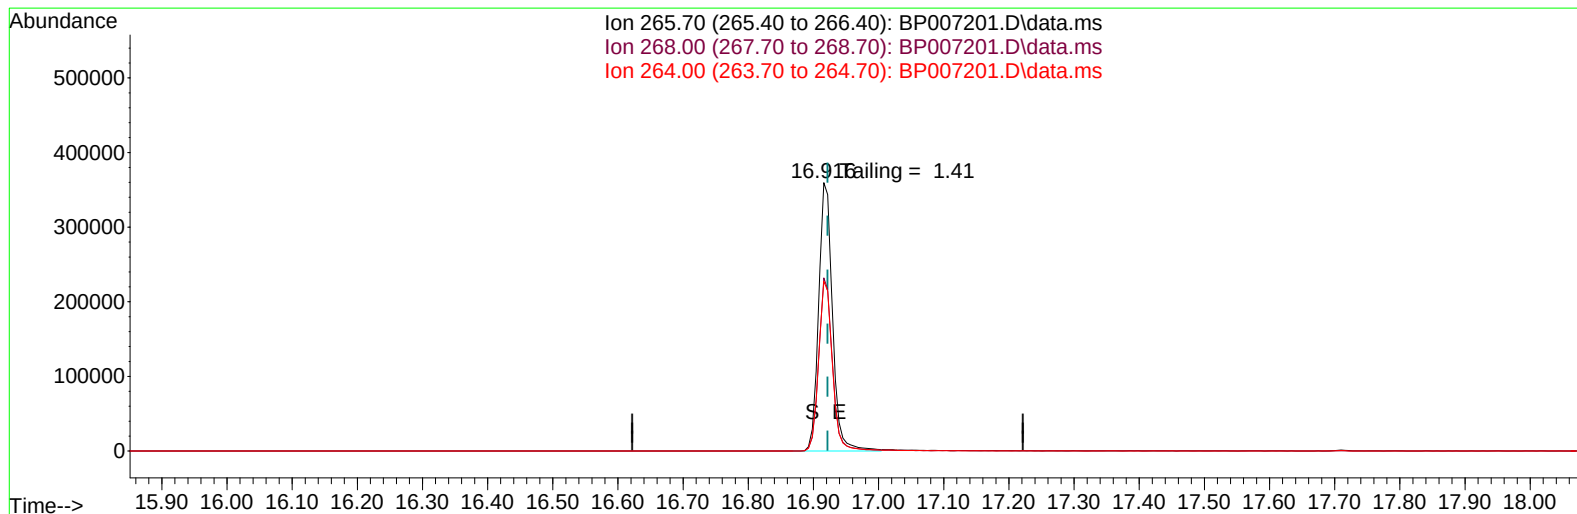

TIC: BP007201.D\data.ms

(70) Pentachlorophenol (C)

16.916min (-0.006) 1428218.80 ng




response 537177

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.50	64.54
264.00	62.90	63.26
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP092721\
 Data File : BP007201.D
 Acq On : 27 Sep 2021 12:26
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Quant Time: Sep 27 13:29:44 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP092121.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Sep 23 11:17:25 2021
 Response via : Initial Calibration

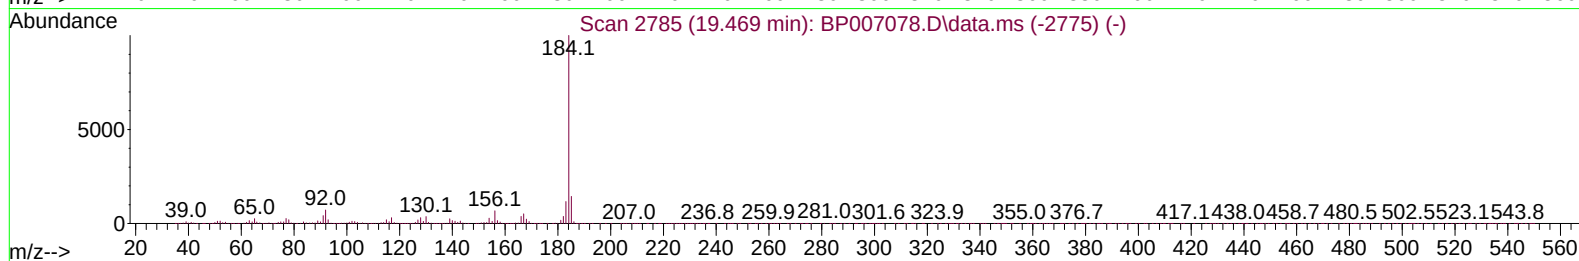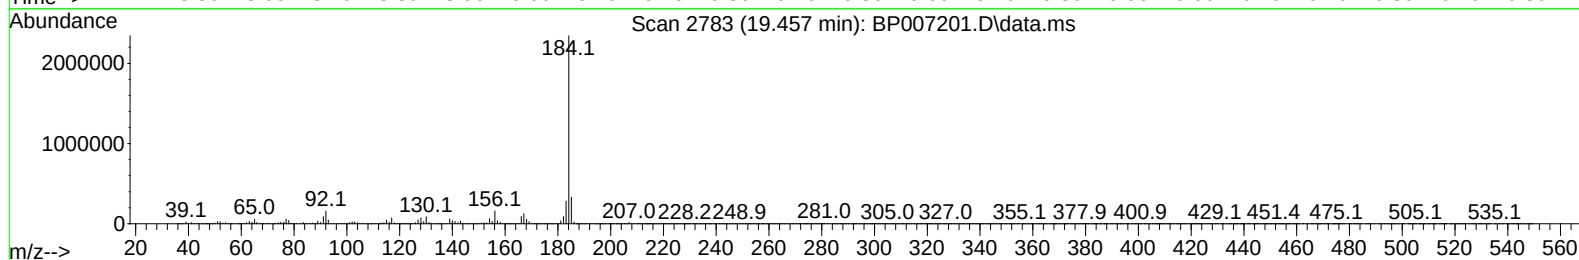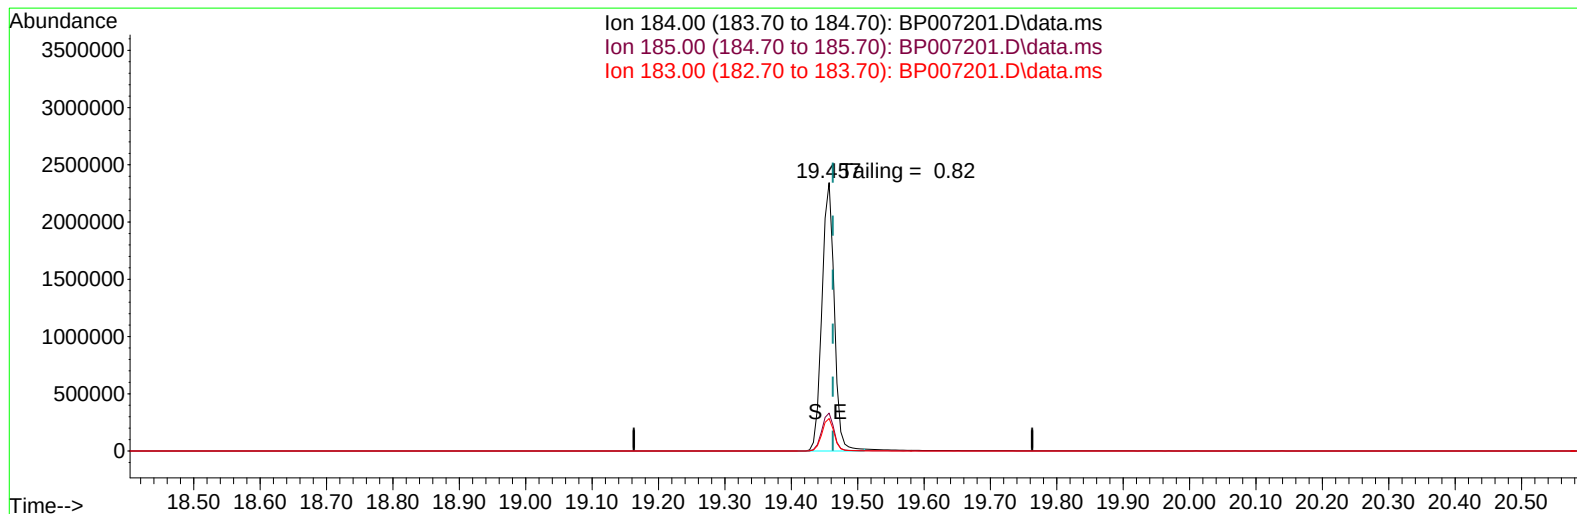

TIC: BP007201.D\data.ms

(77) Benzidine

19.457min (-0.006) 743834.38 ng

response 3063132

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.70	14.16
183.00	11.90	12.09
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
9/27/2021	BNA_P	<u>BP007201.D</u>
Compound Name	Response	Retention Time
DDT	1525447	20.63
DDD	5051	20.23
DDE	706	19.73
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
5757	1531204	0.38