

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP092723\
 Data File : BP017400.D
 Acq On : 27 Sep 2023 16:35
 Operator : MA/JU
 Sample : 04359-02 10X
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 JYCA3

Quant Time: Sep 27 22:31:09 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP092023.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Sep 26 04:52:29 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.922	152	113772	20.000	ng/ul	0.00
20) Naphthalene-d8	10.740	136	478364	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.581	164	280844	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.351	188	600988	20.000	ng/ul	0.00
79) Chrysene-d12	21.457	240	557195	20.000	ng/ul	0.00
88) Perylene-d12	23.968	264	605552	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.293	96	9073	3.276	ng/uL	0.00
4) Pyridine-d5	3.728	84	106782	13.790	ng/ul	0.00
7) Phenol-d5	7.081	99	45031	4.819	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.263	67	285898	50.699	ng/ul	0.00
11) 2-Chlorophenol-d4	7.440	132	134714	18.177	ng/ul	0.00
15) 4-Methylphenol-d8	8.634	113	104398	14.371	ng/ul	0.00
21) Nitrobenzene-d5	9.116	128	172159	49.782	ng/ul	-0.01
24) 2-Nitrophenol-d4	9.834	143	81024	21.577	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.357	165	150683	21.240	ng/ul	0.00
31) 4-Chloroaniline-d4	10.910	131	335739	32.670	ng/ul	0.00
46) Dimethylphthalate-d6	13.998	166	1125866	55.961	ng/ul	0.00
49) Acenaphthylene-d8	14.281	160	1192441	51.534	ng/ul	0.00
54) 4-Nitrophenol-d4	14.839	143	6647	1.896	ng/ul	0.02
60) Fluorene-d10	15.581	176	967699	55.870	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.716	200	36460	10.764	ng/ul	0.00
73) Anthracene-d10	17.451	188	1584728	59.455	ng/ul	0.00
81) Pyrene-d10	19.698	212	1875249	62.235	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.804	264	1817975	62.354	ng/ul	0.00
Target Compounds						
					Qvalue	
6) Benzaldehyde	7.087	77	7207	1.511	ng/ul	97
47) Dimethylphthalate	14.045	163	67877	3.349	ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP092723\
Data File : BP017400.D
Acq On : 27 Sep 2023 16:35
Operator : MA/JU
Sample : 04359-02 10X
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
JYCA3

Quant Time: Sep 27 22:31:09 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP092023.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Sep 26 04:52:29 2023
Response via : Initial Calibration




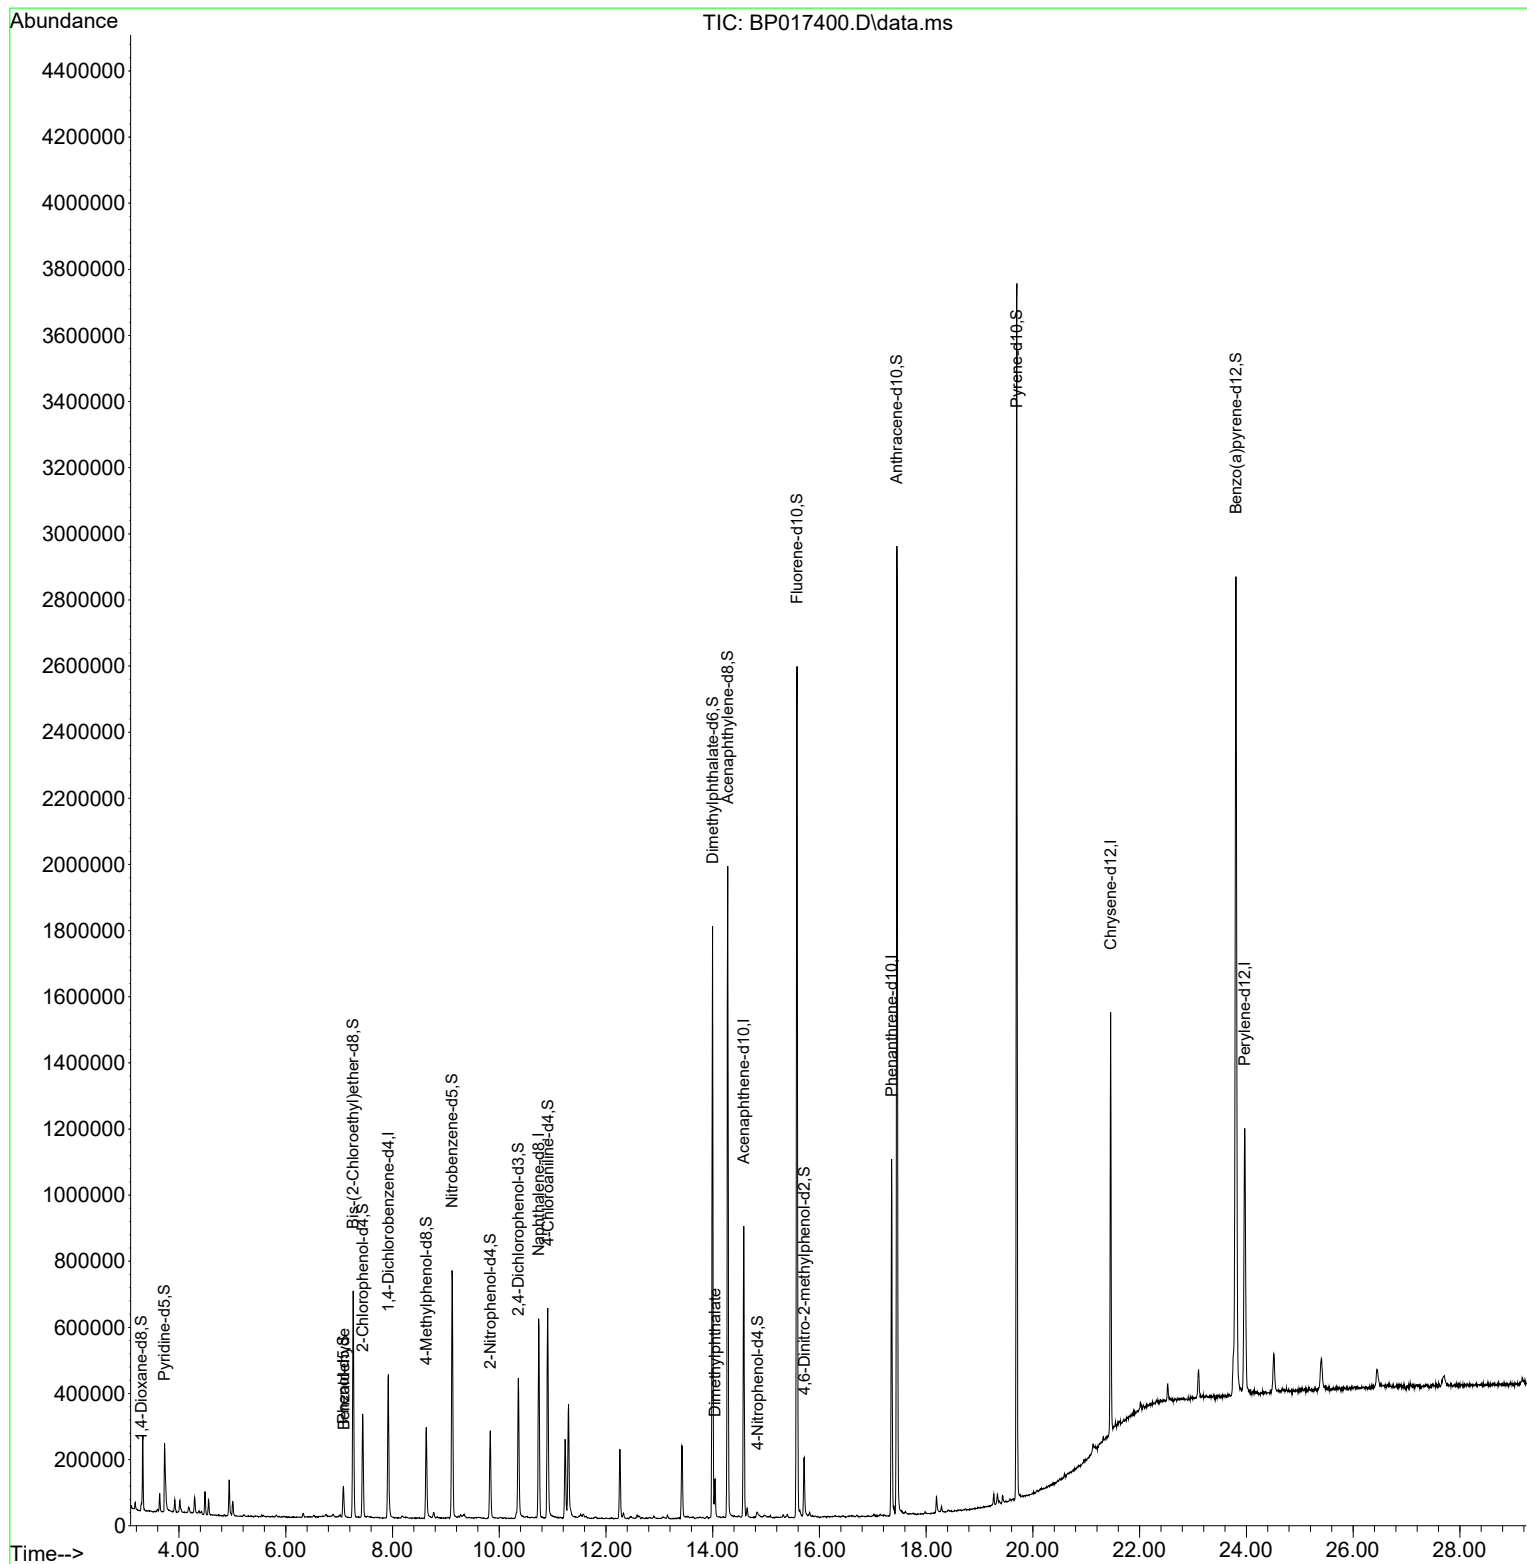


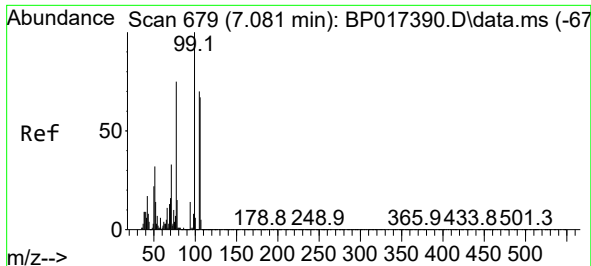

#6
Benzaldehyde
Concen: 1.511 ng/ul
RT: 7.087 min Scan# 61
Delta R.T. -0.000 min
Lab File: BP017400.D
Acq: 27 Sep 2023 16:35

Instrument :
BNA_P
ClientSampleId :
JYCA3

Tgt Ion: 77 Resp: 7207
Ion Ratio Lower Upper
77 100
105 94.5 78.0 117.0
106 93.8 73.2 109.8

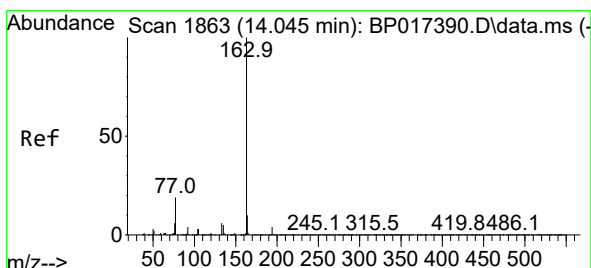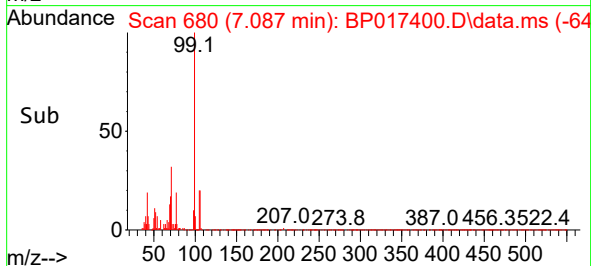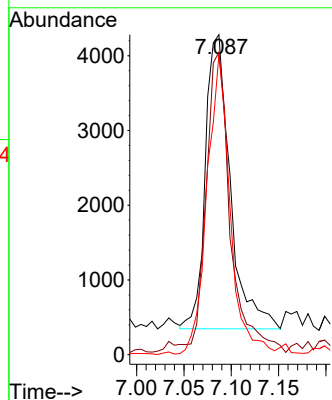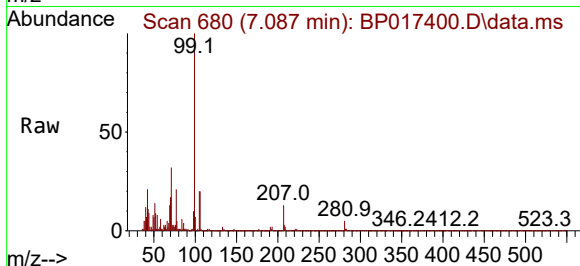

#47
Dimethylphthalate
Concen: 3.349 ng/ul
RT: 14.045 min Scan# 1863
Delta R.T. -0.006 min
Lab File: BP017400.D
Acq: 27 Sep 2023 16:35

Tgt Ion: 163 Resp: 67877
Ion Ratio Lower Upper
163 100
194 4.2 3.2 4.8
164 9.8 7.5 11.3

