

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP092723\
 Data File : BP017391.D
 Acq On : 27 Sep 2023 11:29
 Operator : MA/JU
 Sample : PB155856BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK856

Integration Parameters: LSCINT.P

Integrator: RTE

Smoother: OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0.1 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP092023.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP017391.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.293	31	35	40	rVB	51181	60414	1.47%	0.150%
2	3.722	105	108	127	rBV	623336	911560	22.21%	2.271%
3	5.781	455	458	462	rBV6	3294	5832	0.14%	0.015%
4	7.075	671	678	690	rBV	689596	1093452	26.64%	2.724%
5	7.263	703	710	719	rVB	577388	886286	21.59%	2.208%
6	7.440	732	740	756	rBV	723251	1127668	27.48%	2.809%
7	7.916	814	821	829	rBV	459348	713980	17.40%	1.779%
8	8.628	935	942	956	rBV	824383	1367284	33.31%	3.406%
9	9.116	1018	1025	1035	rBV	678568	1074809	26.19%	2.677%
10	9.828	1138	1146	1157	rBV	532111	883156	21.52%	2.200%
11	10.357	1228	1236	1253	rBV	820225	1430934	34.86%	3.564%
12	10.640	1280	1284	1288	rVB7	2472	4222	0.10%	0.011%
13	10.740	1294	1301	1310	rBV	678655	1103828	26.89%	2.750%
14	10.904	1321	1329	1347	rBV	830211	1490935	36.33%	3.714%
15	11.769	1472	1476	1479	rBV6	2838	4746	0.12%	0.012%
16	11.793	1479	1480	1489	rVB8	4394	8069	0.20%	0.020%
17	12.004	1511	1516	1520	rVB8	2396	4377	0.11%	0.011%
18	12.328	1564	1571	1577	rBV2	12853	24824	0.60%	0.062%
19	13.422	1753	1757	1765	rBV4	12874	22016	0.54%	0.055%
20	13.998	1847	1855	1865	rBV	1523466	2117483	51.59%	5.275%
21	14.281	1895	1903	1915	rBV	1771326	2510748	61.17%	6.254%
22	14.581	1946	1954	1963	rBV	1067959	1520906	37.06%	3.789%
23	14.816	1987	1994	2011	rBV	347316	728739	17.76%	1.815%
24	15.581	2116	2124	2138	rBV	2280731	3249087	79.16%	8.094%
25	15.710	2140	2146	2155	rVV	416879	575745	14.03%	1.434%
26	15.810	2160	2163	2170	rVB4	11008	20873	0.51%	0.052%
27	16.363	2254	2257	2260	rVB5	4102	4489	0.11%	0.011%
28	17.351	2418	2425	2435	rBV	1334301	1851786	45.12%	4.613%
29	17.451	2435	2442	2458	rVV	2553735	3545580	86.39%	8.832%
30	19.269	2747	2751	2755	rBV	28732	36784	0.90%	0.092%
31	19.339	2759	2763	2767	rVV2	24322	33871	0.83%	0.084%
32	19.698	2818	2824	2834	rBV	3238175	4104256	100.00%	10.224%
33	21.457	3118	3123	3131	rBV	1478281	1932496	47.09%	4.814%
34	23.804	3515	3522	3536	rVB2	1880840	3850791	93.82%	9.592%
35	23.968	3544	3550	3560	rVB	914457	1842015	44.88%	4.589%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP092723\
Data File : BP017391.D
Acq On : 27 Sep 2023 11:29
Operator : MA/JU
Sample : PB155856BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK856

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP092023.MA.M
Title : SVOA CALIBRATION




Sum of corrected areas: 40144041

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP092723\
Data File : BP017391.D
Acq On : 27 Sep 2023 11:29
Operator : MA/JU
Sample : PB155856BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK856

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP092023.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

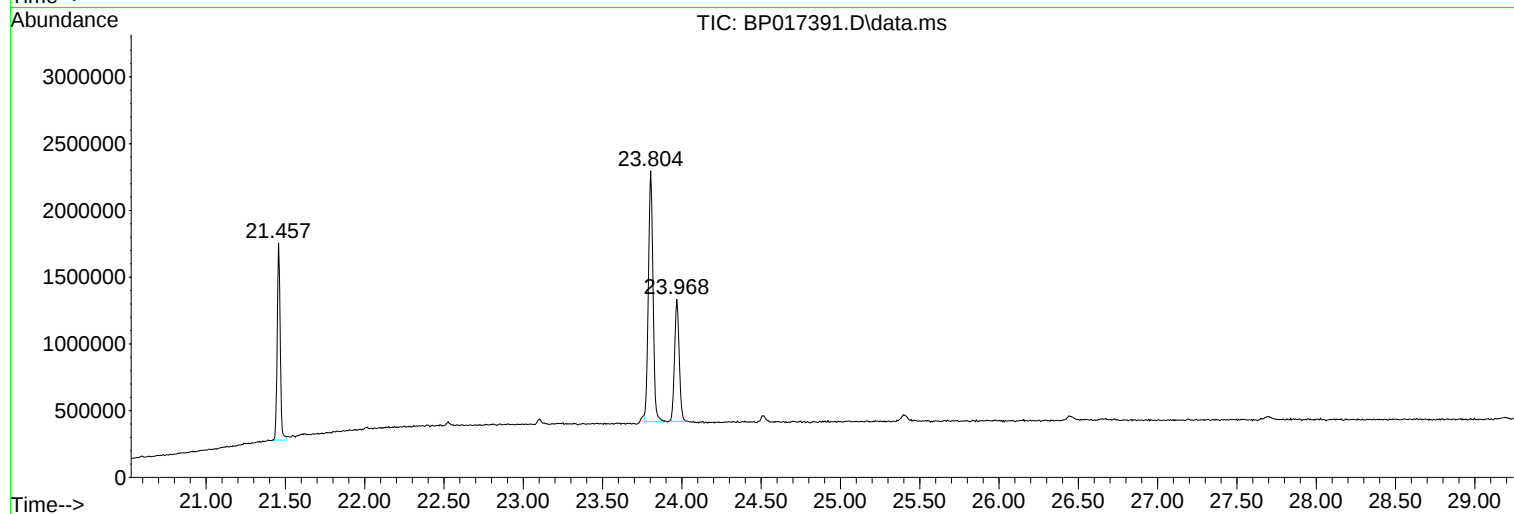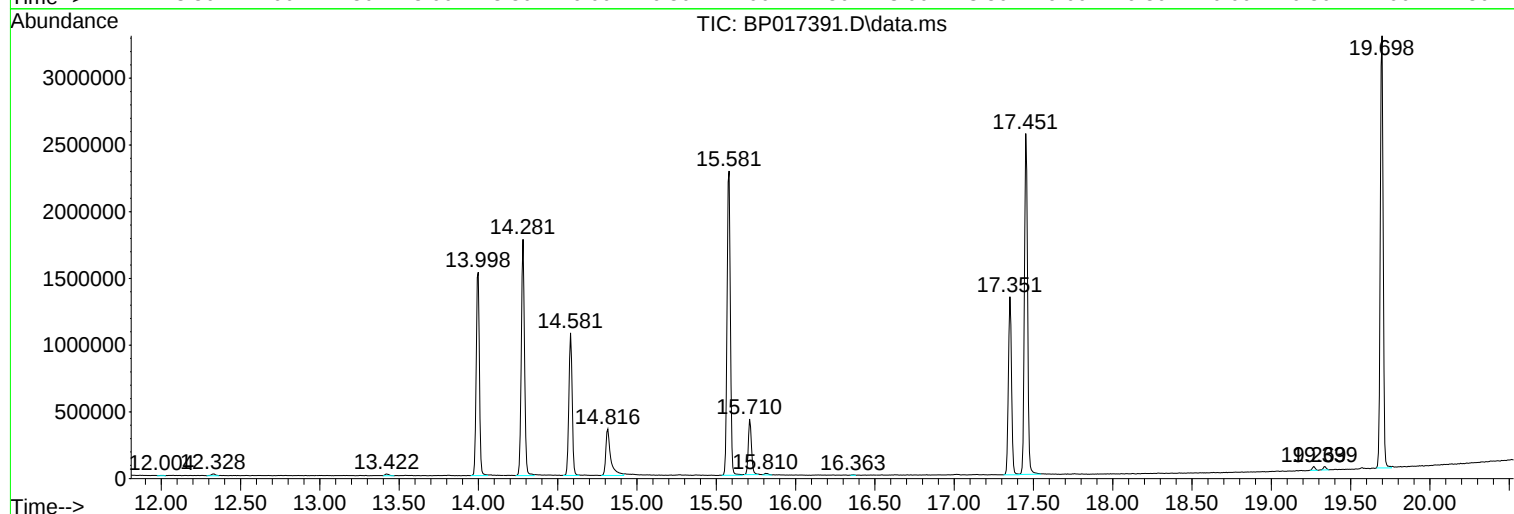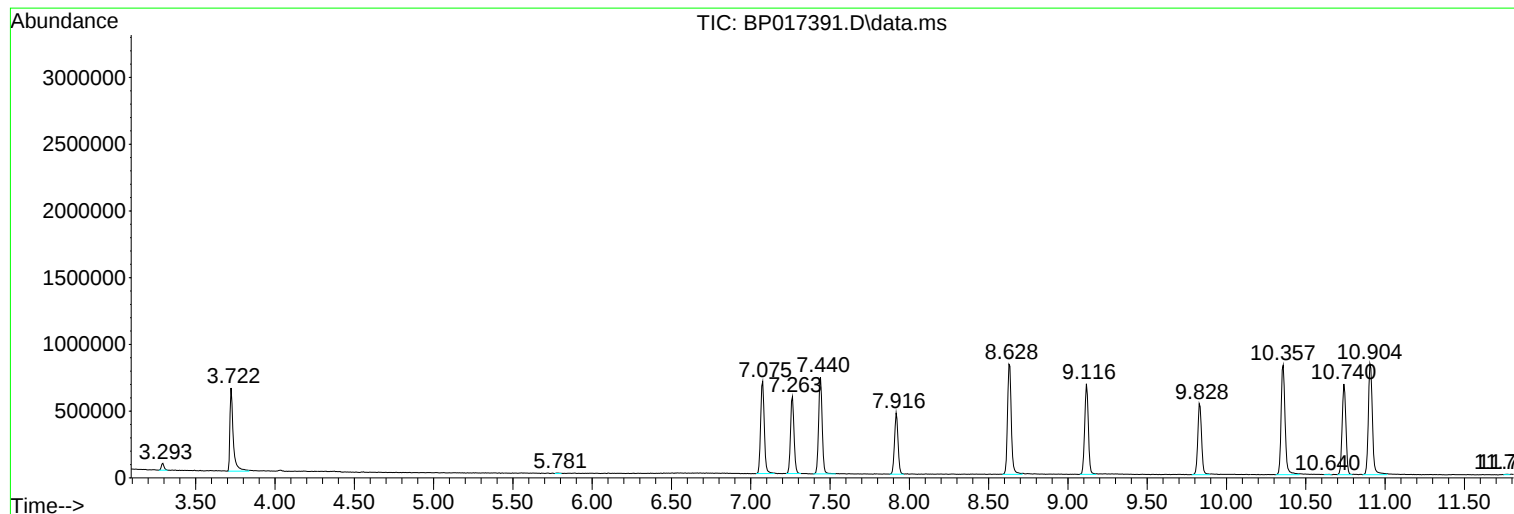

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP092723\
Data File : BP017391.D
Acq On : 27 Sep 2023 11:29
Operator : MA/JU
Sample : PB155856BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK856

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP092023.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP092723\
Data File : BP017391.D
Acq On : 27 Sep 2023 11:29
Operator : MA/JU
Sample : PB155856BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK856

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP092023.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------