

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP092723\
 Data File : BP017393.D
 Acq On : 27 Sep 2023 12:36
 Operator : MA/JU
 Sample : PB155590TB 10X
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SLEB590

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP092023.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP017393.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.293	31	35	45	rVB	56385	74059	1.76%	0.204%
2	3.722	105	108	128	rBV	668095	1013281	24.09%	2.792%
3	7.075	672	678	689	rBV	810079	1249095	29.69%	3.441%
4	7.263	704	710	721	rVB	664404	1015670	24.14%	2.798%
5	7.440	733	740	754	rBV	829856	1286435	30.58%	3.544%
6	7.922	816	822	829	rVB	137555	217550	5.17%	0.599%
7	8.634	936	943	963	rBV	981035	1580192	37.56%	4.354%
8	9.116	1018	1025	1038	rBV	743062	1235156	29.36%	3.403%
9	9.834	1138	1147	1158	rBV	629611	1020800	24.27%	2.812%
10	10.357	1229	1236	1252	rBV	957623	1616320	38.42%	4.453%
11	10.740	1294	1301	1310	rVB	205395	348255	8.28%	0.959%
12	10.910	1321	1330	1348	rBV	963767	1686113	40.08%	4.645%
13	11.793	1470	1480	1481	rBV9	3764	9718	0.23%	0.027%
14	12.328	1565	1571	1580	rVB2	17405	31156	0.74%	0.086%
15	13.422	1751	1757	1762	rBV	13908	22767	0.54%	0.063%
16	13.810	1820	1823	1830	rBV8	2657	4736	0.11%	0.013%
17	13.998	1848	1855	1868	rBV	1735658	2379349	56.56%	6.555%
18	14.281	1895	1903	1919	rBV	1980539	2806820	66.72%	7.733%
19	14.581	1947	1954	1963	rBV	312499	454115	10.80%	1.251%
20	14.816	1987	1994	2010	rBV	362201	775376	18.43%	2.136%
21	15.039	2030	2032	2036	rVB4	3624	4295	0.10%	0.012%
22	15.263	2067	2070	2073	rBV5	4444	4609	0.11%	0.013%
23	15.581	2117	2124	2135	rBV	2436240	3508140	83.40%	9.665%
24	15.710	2140	2146	2156	rVV	459459	639043	15.19%	1.761%
25	15.810	2160	2163	2170	rVB5	11893	21092	0.50%	0.058%
26	16.363	2253	2257	2262	rBV7	2804	5011	0.12%	0.014%
27	16.475	2275	2276	2282	rVB6	3417	5468	0.13%	0.015%
28	17.010	2361	2367	2368	rBV6	4713	7717	0.18%	0.021%
29	17.351	2417	2425	2435	rBV	374443	529935	12.60%	1.460%
30	17.451	2435	2442	2462	rBV	2690579	3708361	88.16%	10.217%
31	19.269	2747	2751	2755	rBV2	29227	38024	0.90%	0.105%
32	19.333	2759	2762	2767	rVB2	23155	33136	0.79%	0.091%
33	19.698	2818	2824	2832	rBV	3232605	4206602	100.00%	11.590%
34	21.457	3119	3123	3130	rBV	365989	503242	11.96%	1.387%
35	23.804	3515	3522	3533	rVB2	1878397	3800368	90.34%	10.471%
36	23.968	3546	3550	3558	rVB	235842	453813	10.79%	1.250%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP092723\
Data File : BP017393.D
Acq On : 27 Sep 2023 12:36
Operator : MA/JU
Sample : PB155590TB 10X
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SLEB590

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP092023.MA.M
Title : SVOA CALIBRATION




Sum of corrected areas: 36295819

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP092723\
Data File : BP017393.D
Acq On : 27 Sep 2023 12:36
Operator : MA/JU
Sample : PB155590TB 10X
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SLEB590

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP092023.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

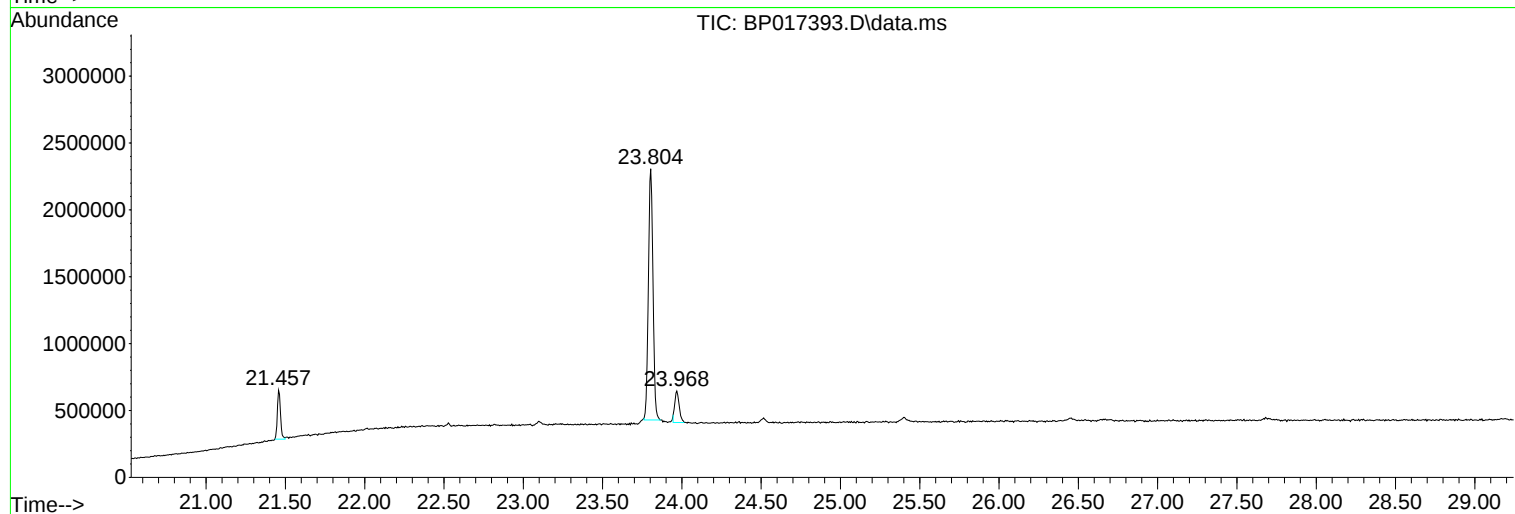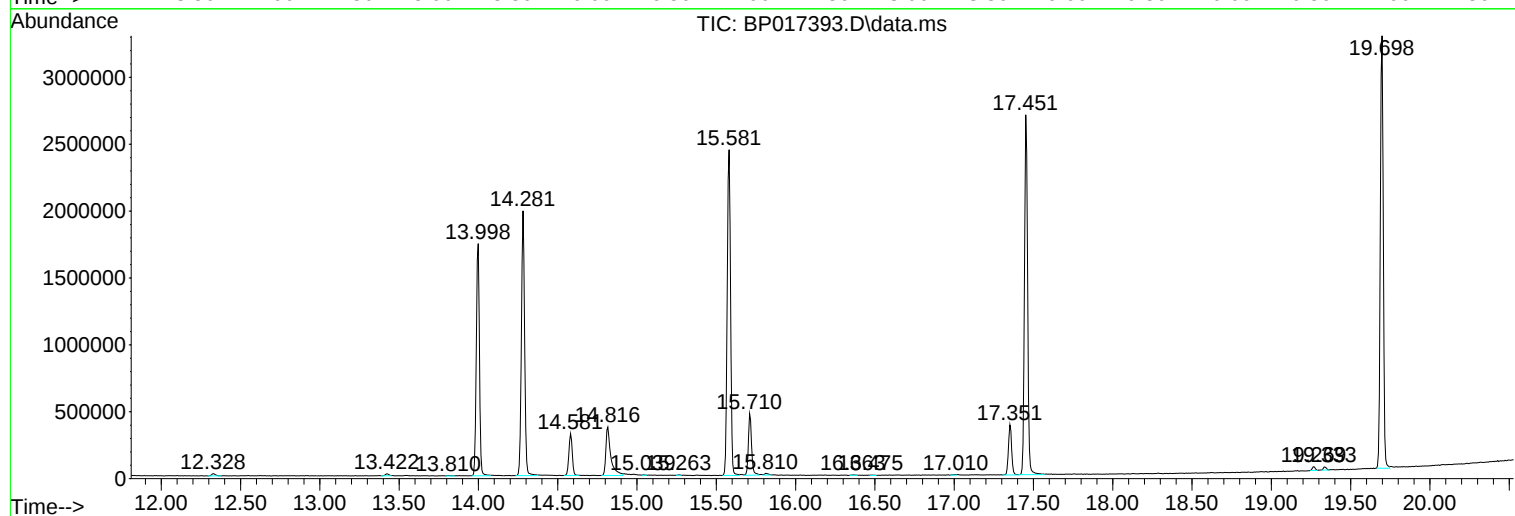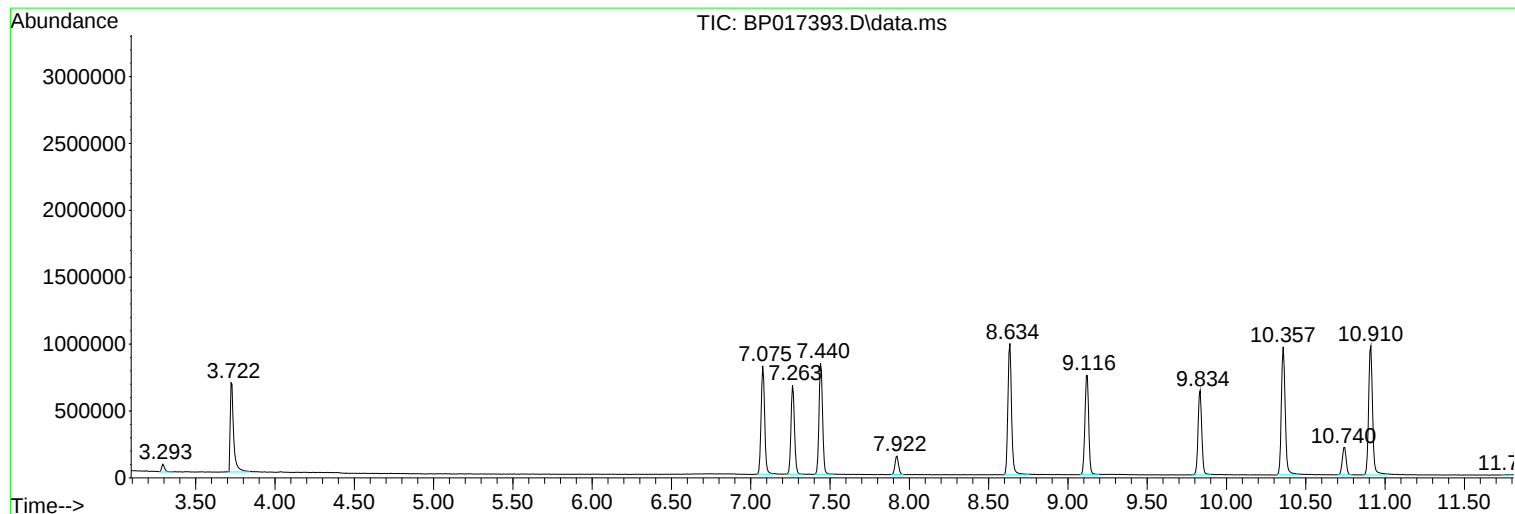

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP092723\
Data File : BP017393.D
Acq On : 27 Sep 2023 12:36
Operator : MA/JU
Sample : PB155590TB 10X
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SLEB590

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP092023.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP092723\
Data File : BP017393.D
Acq On : 27 Sep 2023 12:36
Operator : MA/JU
Sample : PB155590TB 10X
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SLEB590

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP092023.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------