

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP092723\
 Data File : BP017394.D
 Acq On : 27 Sep 2023 13:10
 Operator : MA/JU
 Sample : 04578-05
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SVOC-GPC-BLANK

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP092023.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP017394.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	4.040	158	162	165	rBV6	6482	8703	0.47%	0.098%
2	4.893	303	307	312	rBV8	2383	3529	0.19%	0.040%
3	6.404	561	564	566	rBV4	2149	2362	0.13%	0.027%
4	6.422	566	567	571	rBV4	1267	1911	0.10%	0.022%
5	7.487	746	748	751	rVB4	3753	3452	0.18%	0.039%
6	7.516	751	753	755	rBV3	2801	2625	0.14%	0.030%
7	7.593	764	766	771	rVB6	1741	2497	0.13%	0.028%
8	7.722	786	788	790	rBV3	2190	2075	0.11%	0.023%
9	7.781	796	798	801	rVB4	2423	2334	0.12%	0.026%
10	7.922	815	822	834	rBV	462298	727620	38.96%	8.206%
11	8.216	869	872	874	rBV4	1656	2216	0.12%	0.025%
12	8.663	945	948	950	rBV4	2321	3142	0.17%	0.035%
13	9.246	1045	1047	1050	rBV4	2369	2644	0.14%	0.030%
14	9.316	1056	1059	1061	rVB4	2667	2228	0.12%	0.025%
15	9.610	1106	1109	1112	rVB5	1876	2518	0.13%	0.028%
16	10.745	1292	1302	1313	rBV	640510	1094605	58.62%	12.344%
17	11.081	1357	1359	1363	rVB5	1757	2062	0.11%	0.023%
18	11.145	1367	1370	1373	rVB5	1571	2109	0.11%	0.024%
19	11.322	1395	1400	1402	rBV5	1666	2034	0.11%	0.023%
20	12.334	1570	1572	1578	rVB7	1479	2136	0.11%	0.024%
21	12.592	1613	1616	1618	rBV4	1675	2143	0.11%	0.024%
22	12.634	1620	1623	1626	rVB5	1825	2849	0.15%	0.032%
23	13.051	1692	1694	1697	rVB4	2520	2518	0.13%	0.028%
24	13.092	1697	1701	1704	rBV6	2366	3002	0.16%	0.034%
25	13.139	1706	1709	1712	rVB5	1835	2259	0.12%	0.025%
26	13.345	1742	1744	1750	rVB7	1844	2960	0.16%	0.033%
27	13.398	1750	1753	1754	rBV3	2357	2322	0.12%	0.026%
28	13.422	1754	1757	1758	rBV3	3956	4211	0.23%	0.047%
29	13.510	1769	1772	1775	rBV4	1808	2649	0.14%	0.030%
30	13.828	1824	1826	1828	rVB3	2213	1908	0.10%	0.022%
31	14.292	1901	1905	1907	rBV5	2416	4670	0.25%	0.053%
32	14.581	1947	1954	1967	rBV	1014548	1474699	78.97%	16.631%
33	14.998	2022	2025	2027	rVB4	2841	2501	0.13%	0.028%
34	15.028	2027	2030	2034	rBV6	1660	2365	0.13%	0.027%
35	15.181	2054	2056	2061	rVB5	1785	2425	0.13%	0.027%
36	15.292	2072	2075	2078	rBV5	1352	1944	0.10%	0.022%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP092723\
 Data File : BP017394.D
 Acq On : 27 Sep 2023 13:10
 Operator : MA/JU
 Sample : 04578-05
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SVOC-GPC-BLANK

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP092023.MA.M
 Title : SVOA CALIBRATION

37	15.380	2086	2090	2093	rBV6	2382	3879	0.21%	0.044%
38	15.492	2104	2109	2110	rBV5	1536	2246	0.12%	0.025%
39	15.657	2136	2137	2141	rVB4	1638	1871	0.10%	0.021%
40	15.892	2174	2177	2181	rBV6	2098	3068	0.16%	0.035%
41	15.933	2182	2184	2188	rVB4	1853	2287	0.12%	0.026%
42	16.427	2267	2268	2271	rBV2	2635	2160	0.12%	0.024%
43	16.622	2299	2301	2303	rBV2	2402	2547	0.14%	0.029%
44	17.010	2366	2367	2369	rVV2	2932	2601	0.14%	0.029%
45	17.057	2373	2375	2378	rVB4	2201	2094	0.11%	0.024%
46	17.145	2385	2390	2394	rBV8	4083	6911	0.37%	0.078%
47	17.298	2414	2416	2419	rVB4	2493	2153	0.12%	0.024%
48	17.357	2419	2426	2439	rBV	1208743	1807110	96.77%	20.379%
49	17.616	2468	2470	2474	rVB5	2571	2732	0.15%	0.031%
50	18.004	2534	2536	2539	rBV4	2316	2475	0.13%	0.028%
51	18.163	2560	2563	2566	rBV5	2825	4608	0.25%	0.052%
52	21.457	3118	3123	3131	rBV	1376673	1867380	100.00%	21.059%
53	23.968	3544	3550	3561	rVB	838259	1762975	94.41%	19.882%




Sum of corrected areas: 8867324

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP092723\
Data File : BP017394.D
Acq On : 27 Sep 2023 13:10
Operator : MA/JU
Sample : 04578-05
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SVOC-GPC-BLANK

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP092023.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

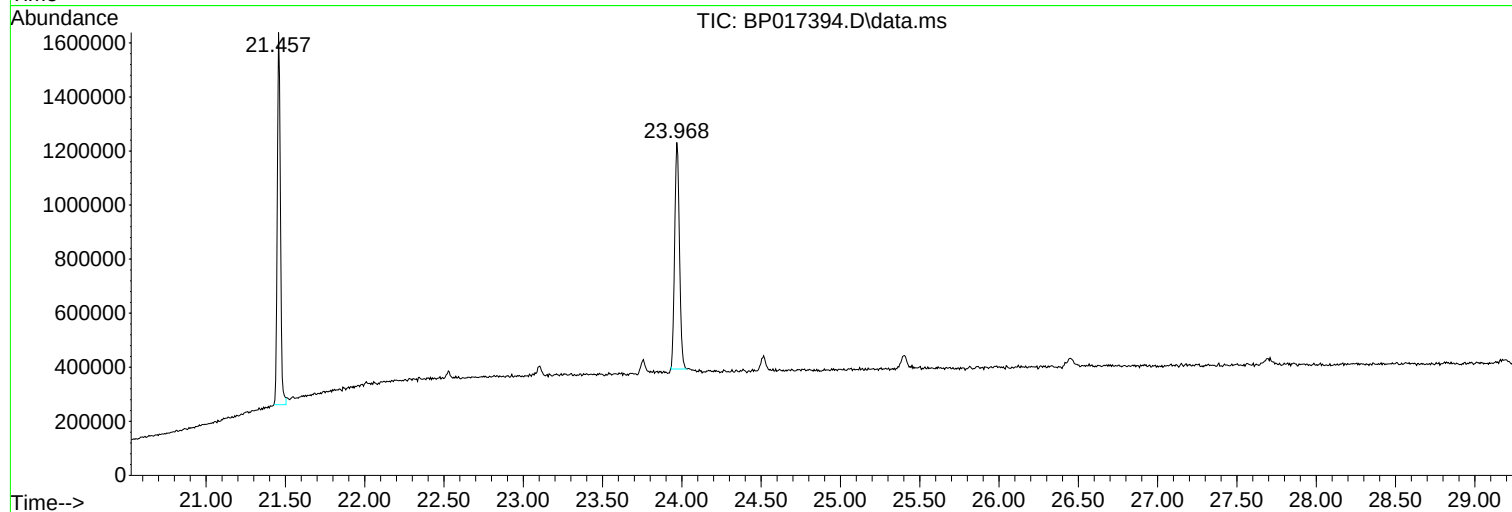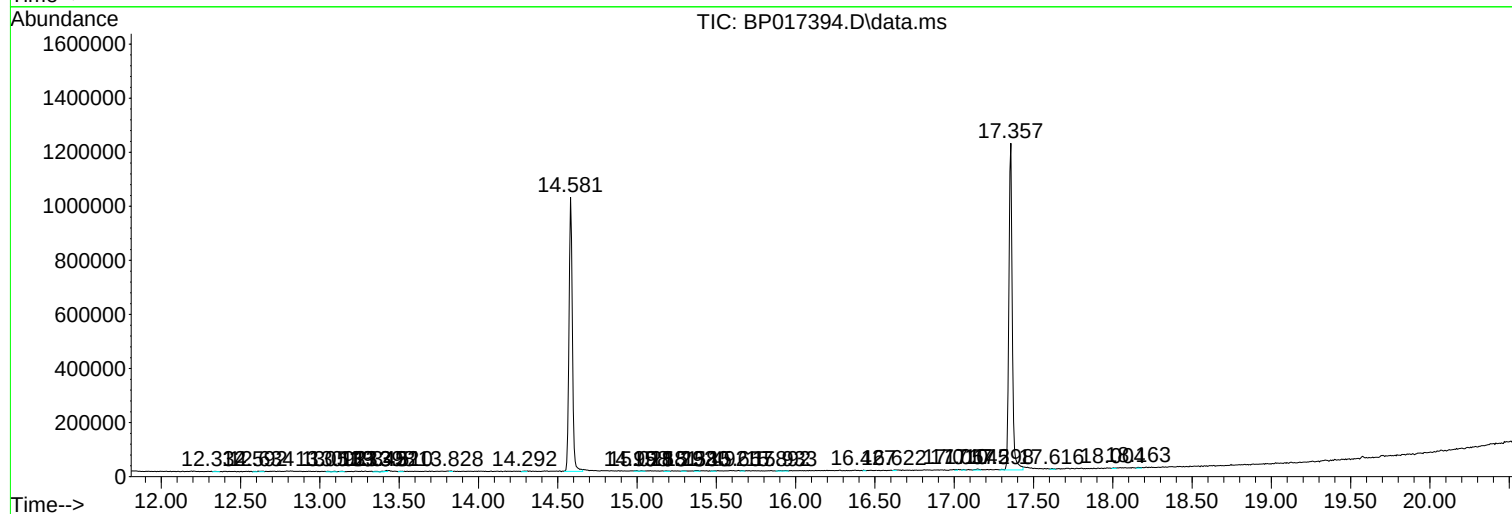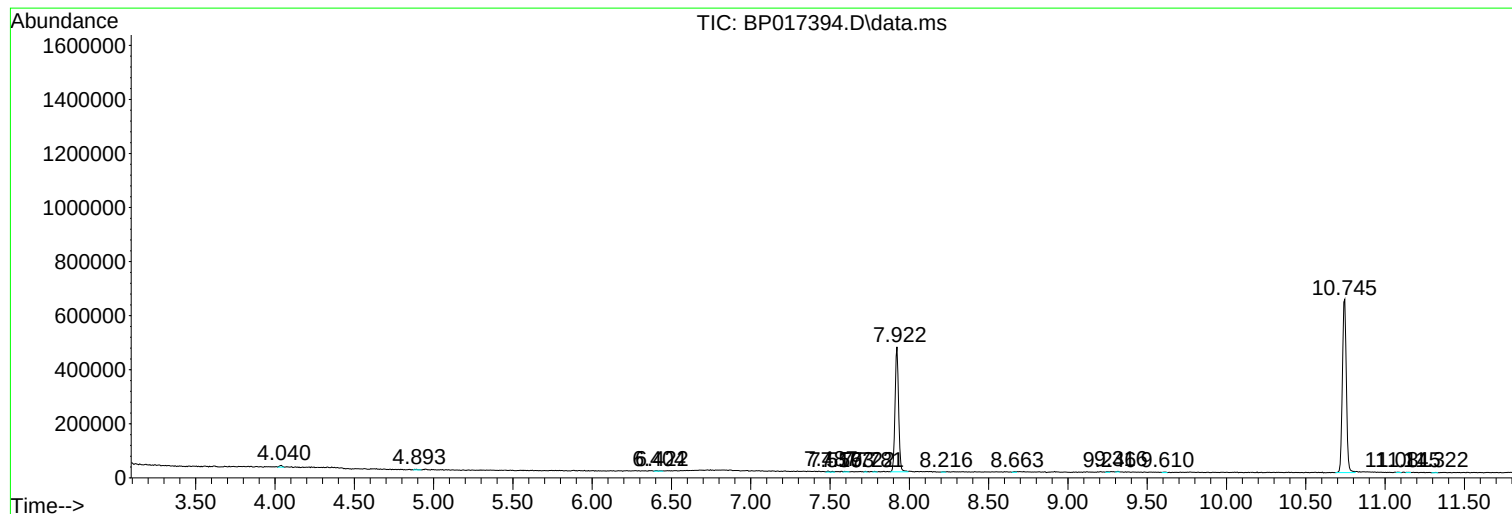

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP092723\
Data File : BP017394.D
Acq On : 27 Sep 2023 13:10
Operator : MA/JU
Sample : 04578-05
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SVOC-GPC-BLANK

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP092023.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP092723\
Data File : BP017394.D
Acq On : 27 Sep 2023 13:10
Operator : MA/JU
Sample : 04578-05
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SVOC-GPC-BLANK

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP092023.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------