

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP092724\
 Data File : BP022074.D
 Acq On : 27 Sep 2024 10:52
 Operator : RC/JU
 Sample : PB163390BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK390

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP092424.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP022074.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.046	7	10	15	rVB2	9515	10907	0.29%	0.032%
2	3.211	34	38	42	rVB	31895	40902	1.10%	0.120%
3	3.617	103	107	128	rVB	394012	572683	15.33%	1.677%
4	3.940	159	162	168	rVB2	9241	11539	0.31%	0.034%
5	4.158	196	199	202	rBV3	6865	8857	0.24%	0.026%
6	4.558	265	267	272	rVB6	3950	5919	0.16%	0.017%
7	5.046	344	350	354	rBV7	2785	5123	0.14%	0.015%
8	6.864	651	659	671	rBV	493978	774491	20.74%	2.268%
9	7.016	678	685	694	rBV	328919	566246	15.16%	1.658%
10	7.222	711	720	732	rBV	482579	765840	20.51%	2.242%
11	7.681	791	798	807	rBV	436534	709818	19.01%	2.078%
12	8.122	869	873	879	rVB8	3421	6061	0.16%	0.018%
13	8.381	909	917	926	rBV	622438	934666	25.03%	2.737%
14	8.493	934	936	943	rVB5	6022	7688	0.21%	0.023%
15	8.816	984	991	1004	rBV	468980	758249	20.30%	2.220%
16	9.387	1084	1088	1093	rVB4	3201	5150	0.14%	0.015%
17	9.534	1105	1113	1125	rBV	395797	649124	17.38%	1.900%
18	9.628	1125	1129	1133	rVB7	4003	7395	0.20%	0.022%
19	10.069	1196	1204	1223	rBV	625537	1054569	28.24%	3.088%
20	10.440	1260	1267	1275	rBV	589688	949793	25.43%	2.781%
21	10.581	1282	1291	1302	rBV	462020	882464	23.63%	2.584%
22	10.781	1319	1325	1332	rVB	5103	9448	0.25%	0.028%
23	11.746	1486	1489	1494	rVB7	2633	3977	0.11%	0.012%
24	12.040	1534	1539	1546	rVV3	8141	14660	0.39%	0.043%
25	12.104	1546	1550	1556	rVB6	4121	7475	0.20%	0.022%
26	12.322	1585	1587	1598	rVB3	5293	10172	0.27%	0.030%
27	12.475	1606	1613	1621	rBV9	4779	11686	0.31%	0.034%
28	12.728	1651	1656	1662	rVB10	3408	6387	0.17%	0.019%
29	12.816	1666	1671	1676	rBV8	2941	5109	0.14%	0.015%
30	13.093	1711	1718	1720	rBV5	6923	9828	0.26%	0.029%
31	13.122	1721	1723	1728	rVV2	4993	8376	0.22%	0.025%
32	13.175	1728	1732	1738	rVB4	4759	8209	0.22%	0.024%
33	13.710	1816	1823	1829	rBV	1366319	1590128	42.58%	4.656%
34	13.875	1846	1851	1855	rBV7	2549	4103	0.11%	0.012%
35	13.998	1864	1872	1882	rBV	1097639	1741635	46.63%	5.099%
36	14.304	1917	1924	1931	rBV	953805	1373739	36.78%	4.022%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP092724\
 Data File : BP022074.D
 Acq On : 27 Sep 2024 10:52
 Operator : RC/JU
 Sample : PB163390BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK390

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP092424.MA.M
 Title : SVOA CALIBRATION

37	14.375	1931	1936	1941	rVB6	8085	13551	0.36%	0.040%
38	14.510	1952	1959	1975	rBV	397872	763893	20.45%	2.237%
39	14.716	1991	1994	2002	rVB2	10241	19452	0.52%	0.057%
40	14.945	2028	2033	2038	rBV9	5371	8712	0.23%	0.026%
41	15.134	2060	2065	2070	rVB2	6930	9687	0.26%	0.028%
42	15.316	2088	2096	2103	rBV	1470027	2312693	61.93%	6.771%
43	15.375	2103	2106	2110	rVV4	15098	23316	0.62%	0.068%
44	15.440	2111	2117	2131	rVB	479045	628106	16.82%	1.839%
45	15.551	2133	2136	2139	rBV4	5911	9533	0.26%	0.028%
46	15.975	2203	2208	2213	rBV9	3659	6268	0.17%	0.018%
47	16.045	2216	2220	2228	rVB10	3902	7384	0.20%	0.022%
48	16.110	2228	2231	2242	rBV10	5243	11580	0.31%	0.034%
49	16.281	2256	2260	2265	rBV5	6958	11428	0.31%	0.033%
50	16.398	2274	2280	2285	rBV6	8614	15329	0.41%	0.045%
51	16.451	2285	2289	2293	rVV4	5306	8078	0.22%	0.024%
52	16.498	2293	2297	2300	rVV5	3694	5385	0.14%	0.016%
53	16.563	2303	2308	2313	rBV9	5241	9933	0.27%	0.029%
54	16.757	2337	2341	2342	rBV4	3959	5191	0.14%	0.015%
55	16.892	2358	2364	2370	rBV7	4387	7795	0.21%	0.023%
56	16.981	2374	2379	2381	rBV5	3790	5065	0.14%	0.015%
57	17.116	2395	2402	2412	rBV	1238535	1891184	50.64%	5.537%
58	17.210	2412	2418	2431	rVB	1788516	2634562	70.54%	7.713%
59	17.539	2470	2474	2477	rBV3	6604	9790	0.26%	0.029%
60	17.581	2477	2481	2485	rVB7	7615	10751	0.29%	0.031%
61	18.057	2559	2562	2569	rBV7	7547	14360	0.38%	0.042%
62	18.128	2571	2574	2579	rVB	7949	12257	0.33%	0.036%
63	18.386	2613	2618	2624	rVB8	7125	14472	0.39%	0.042%
64	19.139	2742	2746	2751	rVB3	22198	33022	0.88%	0.097%
65	19.216	2756	2759	2762	rBV2	16059	23366	0.63%	0.068%
66	19.598	2817	2824	2835	rBV	2277387	3513921	94.09%	10.288%
67	21.545	3149	3155	3167	rVB	1512728	2440472	65.35%	7.145%
68	24.616	3667	3677	3695	rVB	1499427	3734619	100.00%	10.934%
69	24.833	3706	3714	3733	rVB2	822211	2407899	64.48%	7.050%




Sum of corrected areas: 34155470

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP092724\
Data File : BP022074.D
Acq On : 27 Sep 2024 10:52
Operator : RC/JU
Sample : PB163390BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK390

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP092424.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

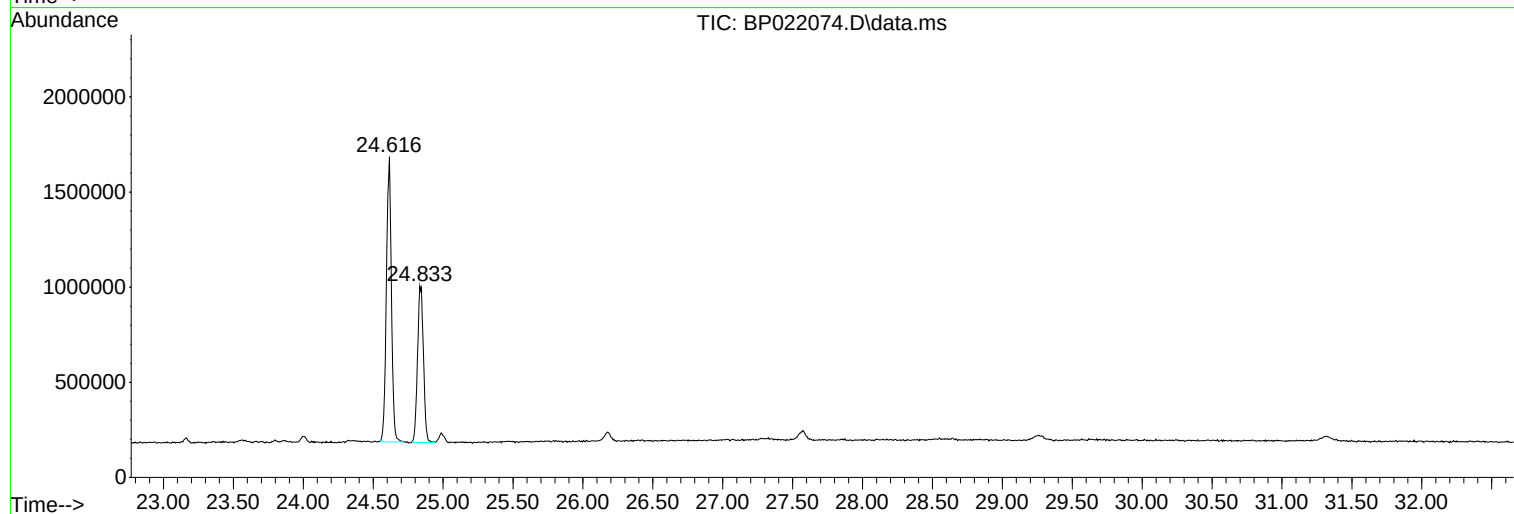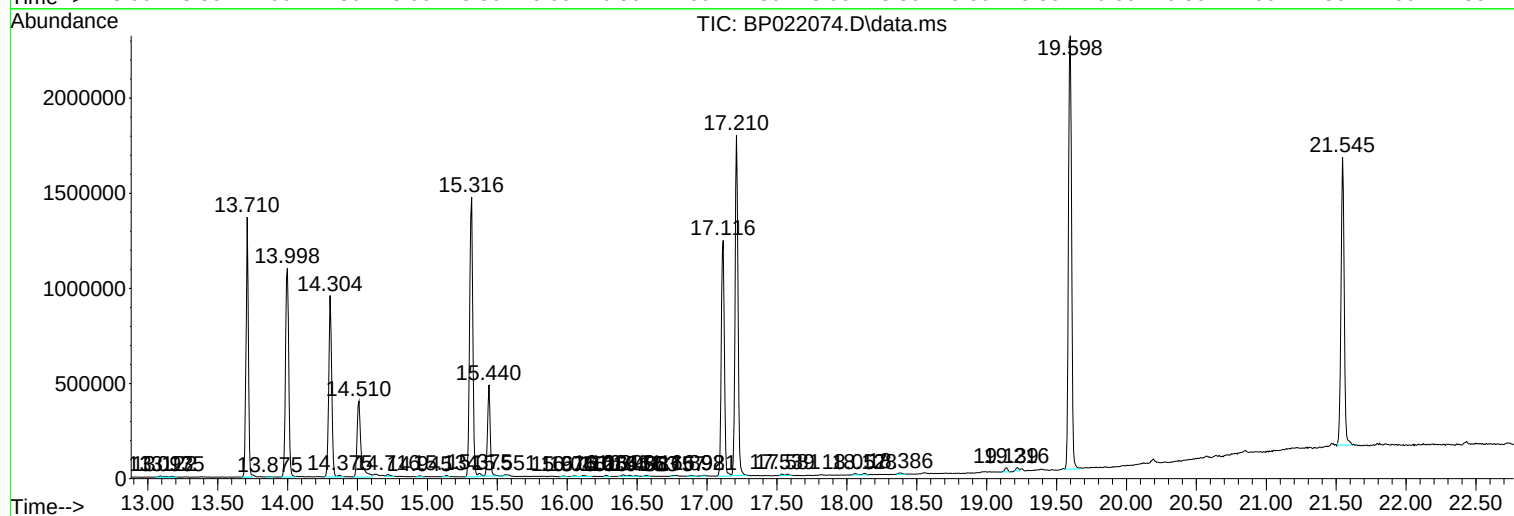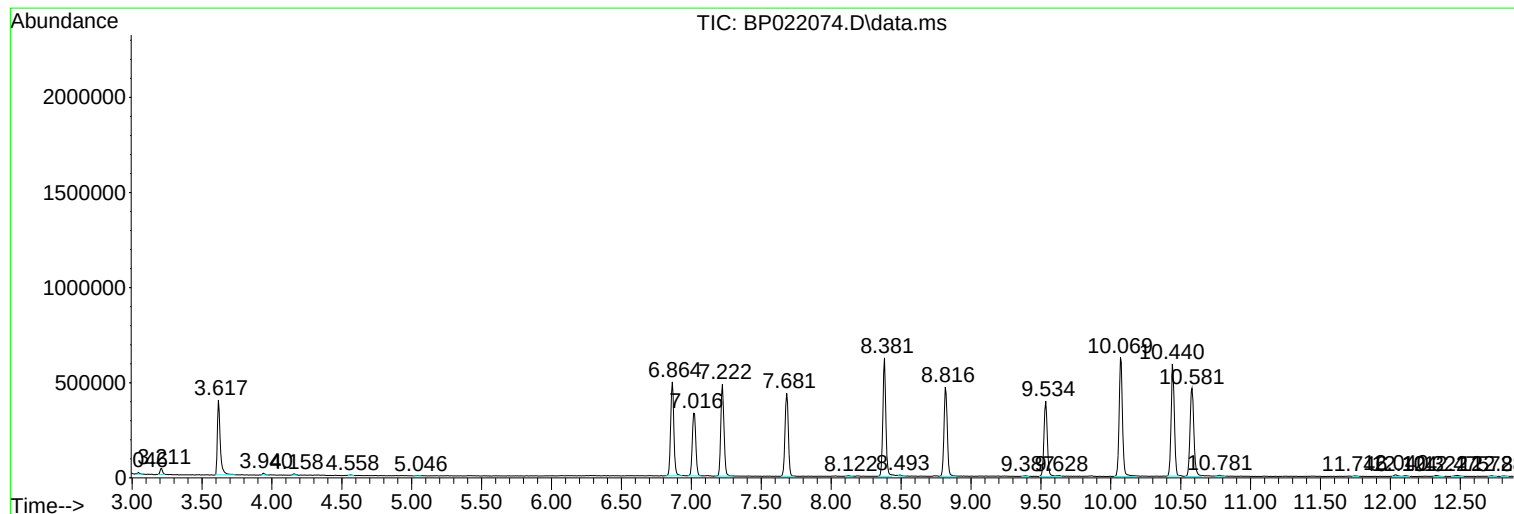

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP092724\
Data File : BP022074.D
Acq On : 27 Sep 2024 10:52
Operator : RC/JU
Sample : PB163390BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK390

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP092424.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP092724\
Data File : BP022074.D
Acq On : 27 Sep 2024 10:52
Operator : RC/JU
Sample : PB163390BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK390

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP092424.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc