

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP092823\
 Data File : BP017416.D
 Acq On : 28 Sep 2023 16:22
 Operator : MA/JU
 Sample : 04417-25
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 EZYF1

Quant Time: Sep 28 22:31:02 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP092023.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Sep 28 15:31:53 2023
 Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.975	152	155586	20.000	ng/u1	0.02
20) Naphthalene-d8	10.816	136	606133	20.000	ng/u1	0.02
38) Acenaphthene-d10	14.669	164	332997	20.000	ng/u1	0.02
64) Phenanthrene-d10	17.463	188	643550	20.000	ng/u1	0.02
79) Chrysene-d12	21.592	240	590403	20.000	ng/u1	# 0.02
88) Perylene-d12	24.192	264	744363	20.000	ng/u1	# 0.04
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.305	96	9378	2.476	ng/uL	0.00
4) Pyridine-d5	3.752	84	19388	1.831	ng/u1	0.02
7) Phenol-d5	7.134	99	112510	8.805	ng/u1	0.02
9) Bis-(2-Chloroethyl)eth...	7.310	67	106860	13.857	ng/u1	0.01
11) 2-Chlorophenol-d4	7.493	132	49367	4.871	ng/u1	0.02
15) 4-Methylphenol-d8	8.699	113	47382	4.769	ng/u1	0.02
21) Nitrobenzene-d5	9.181	128	67423	15.386	ng/u1	0.02
24) 2-Nitrophenol-d4	9.904	143	5205	1.094	ng/u1	0.02
28) 2,4-Dichlorophenol-d3	10.440	165	10863	1.208	ng/u1	0.03
31) 4-Chloroaniline-d4	10.987	131	112012	8.602	ng/u1	0.02
46) Dimethylphthalate-d6	14.081	166	374697	15.707	ng/u1	0.02
49) Acenaphthylene-d8	14.369	160	429905	15.669	ng/u1	0.02
54) 4-Nitrophenol-d4	14.875	143	253	0.061	ng/u1	0.00
60) Fluorene-d10	15.675	176	325660	15.857	ng/u1	0.02
65) 4,6-Dinitro-2-methylph...	15.810	200	254	0.070	ng/u1	0.02
73) Anthracene-d10	17.563	188	469962	16.466	ng/u1	0.02
81) Pyrene-d10	19.816	212	544479	17.054	ng/u1	0.02
92) Benzo(a)pyrene-d12	24.021	264	581780	16.233	ng/u1	0.04
Target Compounds						
16) Acetophenone	8.828	105	64378	4.194	ng/u1	Qvalue 97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP092823\
Data File : BP017416.D
Acq On : 28 Sep 2023 16:22
Operator : MA/JU
Sample : 04417-25
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
EZYF1

Quant Time: Sep 28 22:31:02 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP092023.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Sep 28 15:31:53 2023
Response via : Initial Calibration

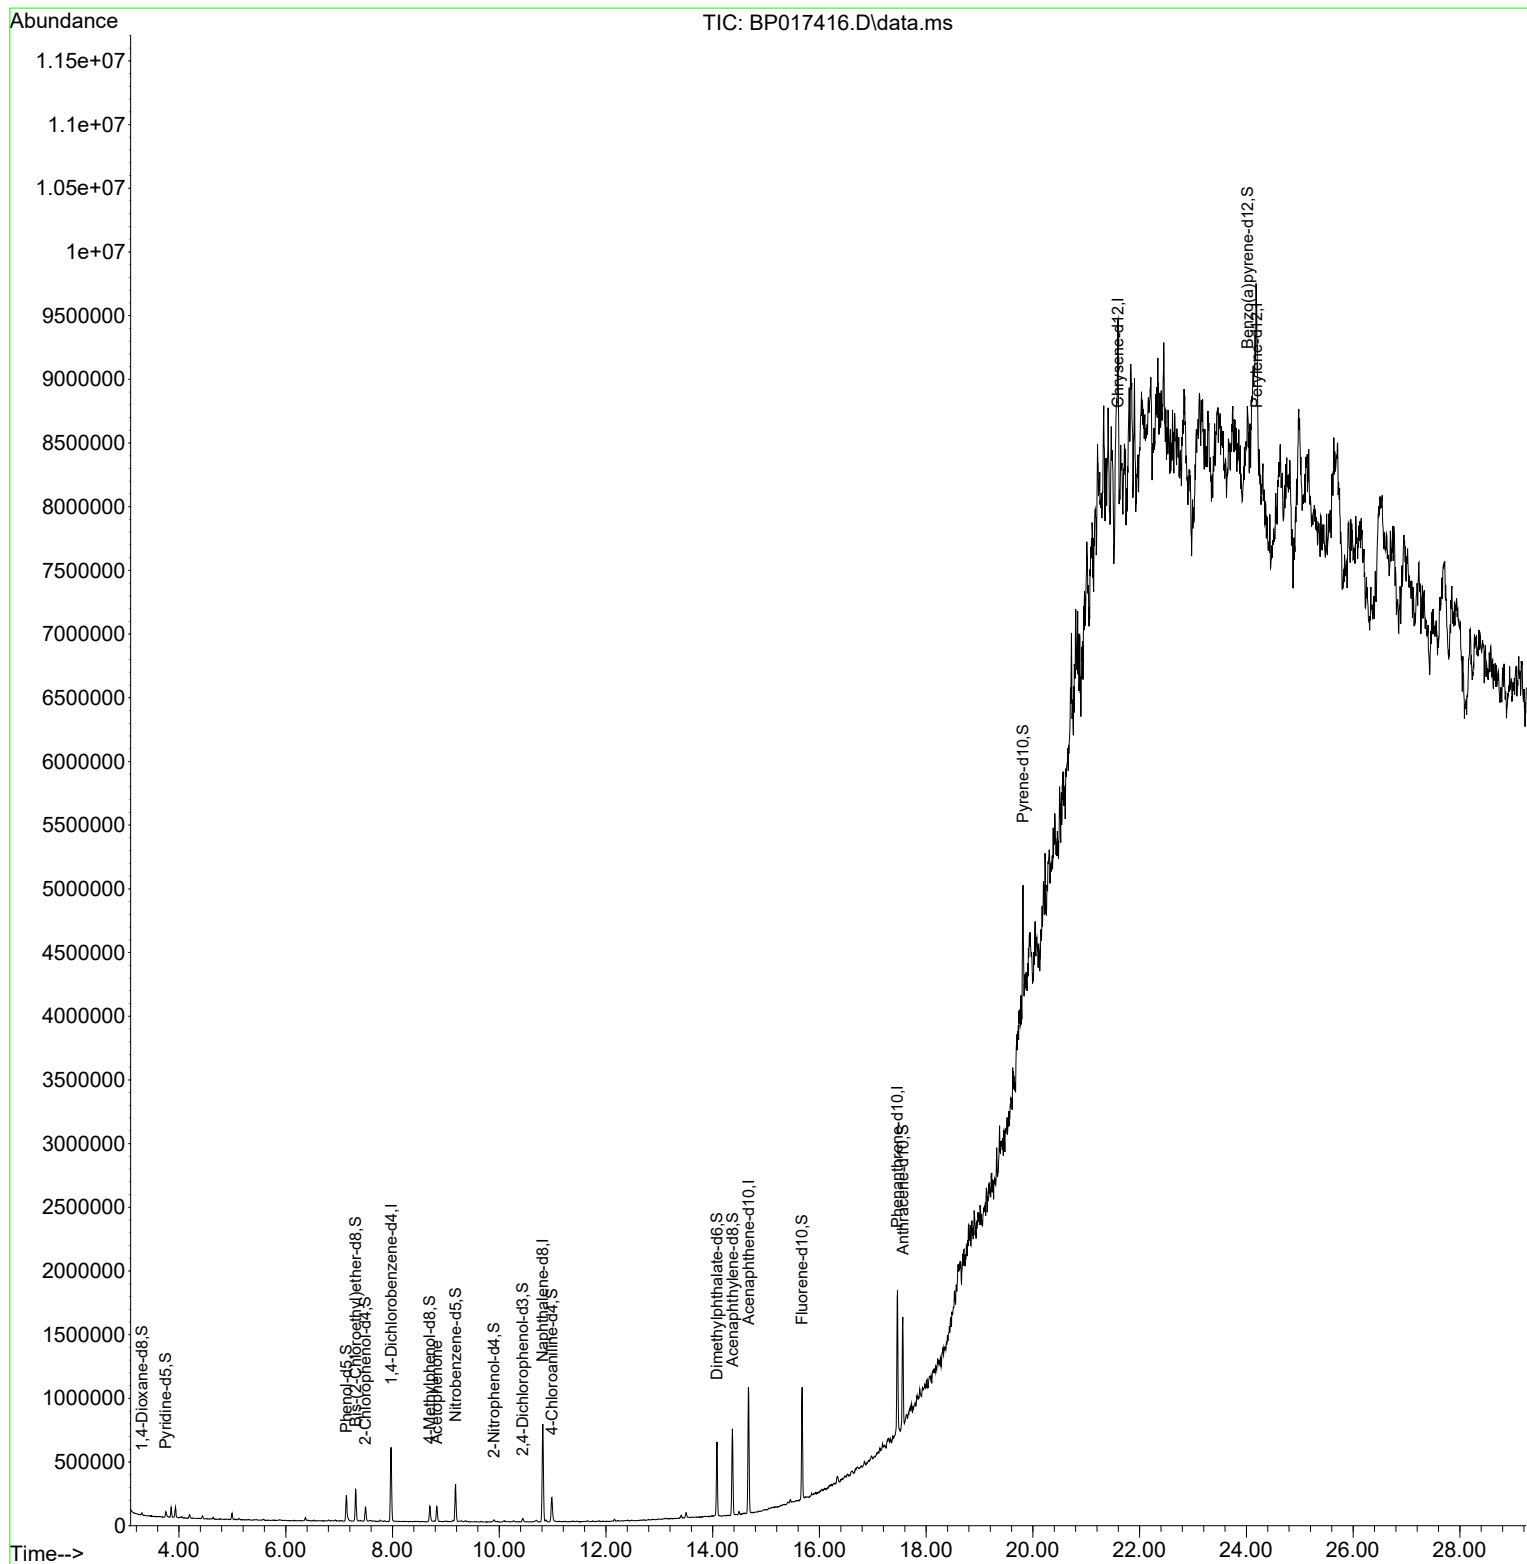

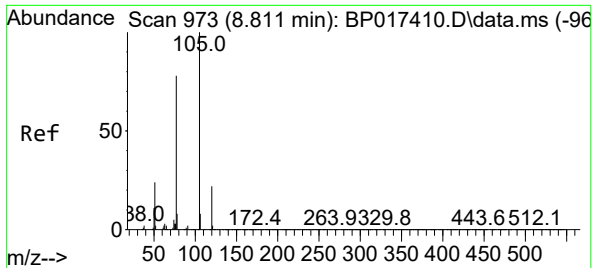

#16
 Acetophenone
 Concen: 4.194 ng/ul
 RT: 8.828 min Scan# 91
 Delta R.T. 0.017 min
 Lab File: BP017416.D
 Acq: 28 Sep 2023 16:22

Instrument :
 BNA_P
 ClientSampleId :
 EZYF1

Tgt Ion:	105	Resp:	64378
Ion	Ratio	Lower	Upper
105	100		
77	81.1	63.6	95.4
51	27.4	19.2	28.8

