

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP092823\
 Data File : BP017417.D
 Acq On : 28 Sep 2023 16:57
 Operator : MA/JU
 Sample : 04417-26
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 EZYF2

Quant Time: Sep 28 22:31:14 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP092023.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Sep 28 15:31:53 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.975	152	128046	20.000	ng/ul	0.02
20) Naphthalene-d8	10.816	136	509805	20.000	ng/ul	0.02
38) Acenaphthene-d10	14.669	164	302122	20.000	ng/ul	0.02
64) Phenanthrene-d10	17.457	188	633082	20.000	ng/ul	0.02
79) Chrysene-d12	21.592	240	592188	20.000	ng/ul	0.02
88) Perylene-d12	24.186	264	721936	20.000	ng/ul	0.04
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.299	96	5307	1.702	ng/uL	0.00
4) Pyridine-d5	3.775	84	3294	0.378	ng/ul	0.04
7) Phenol-d5	7.128	99	86178	8.195	ng/ul	0.02
9) Bis-(2-Chloroethyl)eth...	7.311	67	60394	9.516	ng/ul	0.01
11) 2-Chlorophenol-d4	7.493	132	71254	8.543	ng/ul	0.02
15) 4-Methylphenol-d8	8.693	113	23872	2.920	ng/ul	0.02
21) Nitrobenzene-d5	9.181	128	38486	10.442	ng/ul	0.02
24) 2-Nitrophenol-d4	9.899	143	25654	6.411	ng/ul	0.02
28) 2,4-Dichlorophenol-d3	10.434	165	46829	6.194	ng/ul	0.02
31) 4-Chloroaniline-d4	10.981	131	62770	5.731	ng/ul	0.02
46) Dimethylphthalate-d6	14.081	166	230543	10.652	ng/ul	0.02
49) Acenaphthylene-d8	14.369	160	265653	10.672	ng/ul	0.02
54) 4-Nitrophenol-d4	14.887	143	144	0.038	ng/ul	0.00
60) Fluorene-d10	15.675	176	205239	11.015	ng/ul	0.02
65) 4,6-Dinitro-2-methylph...	15.798	200	101	0.028	ng/ul	0.00
73) Anthracene-d10	17.557	188	295010	10.507	ng/ul	0.02
81) Pyrene-d10	19.810	212	360252	11.249	ng/ul	0.02
92) Benzo(a)pyrene-d12	24.015	264	376211	10.823	ng/ul	0.04
Target Compounds						
					Qvalue	
16) Acetophenone	8.828	105	53231	4.213	ng/ul	97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP092823\
Data File : BP017417.D
Acq On : 28 Sep 2023 16:57
Operator : MA/JU
Sample : 04417-26
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
EZYF2

Quant Time: Sep 28 22:31:14 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP092023.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Sep 28 15:31:53 2023
Response via : Initial Calibration

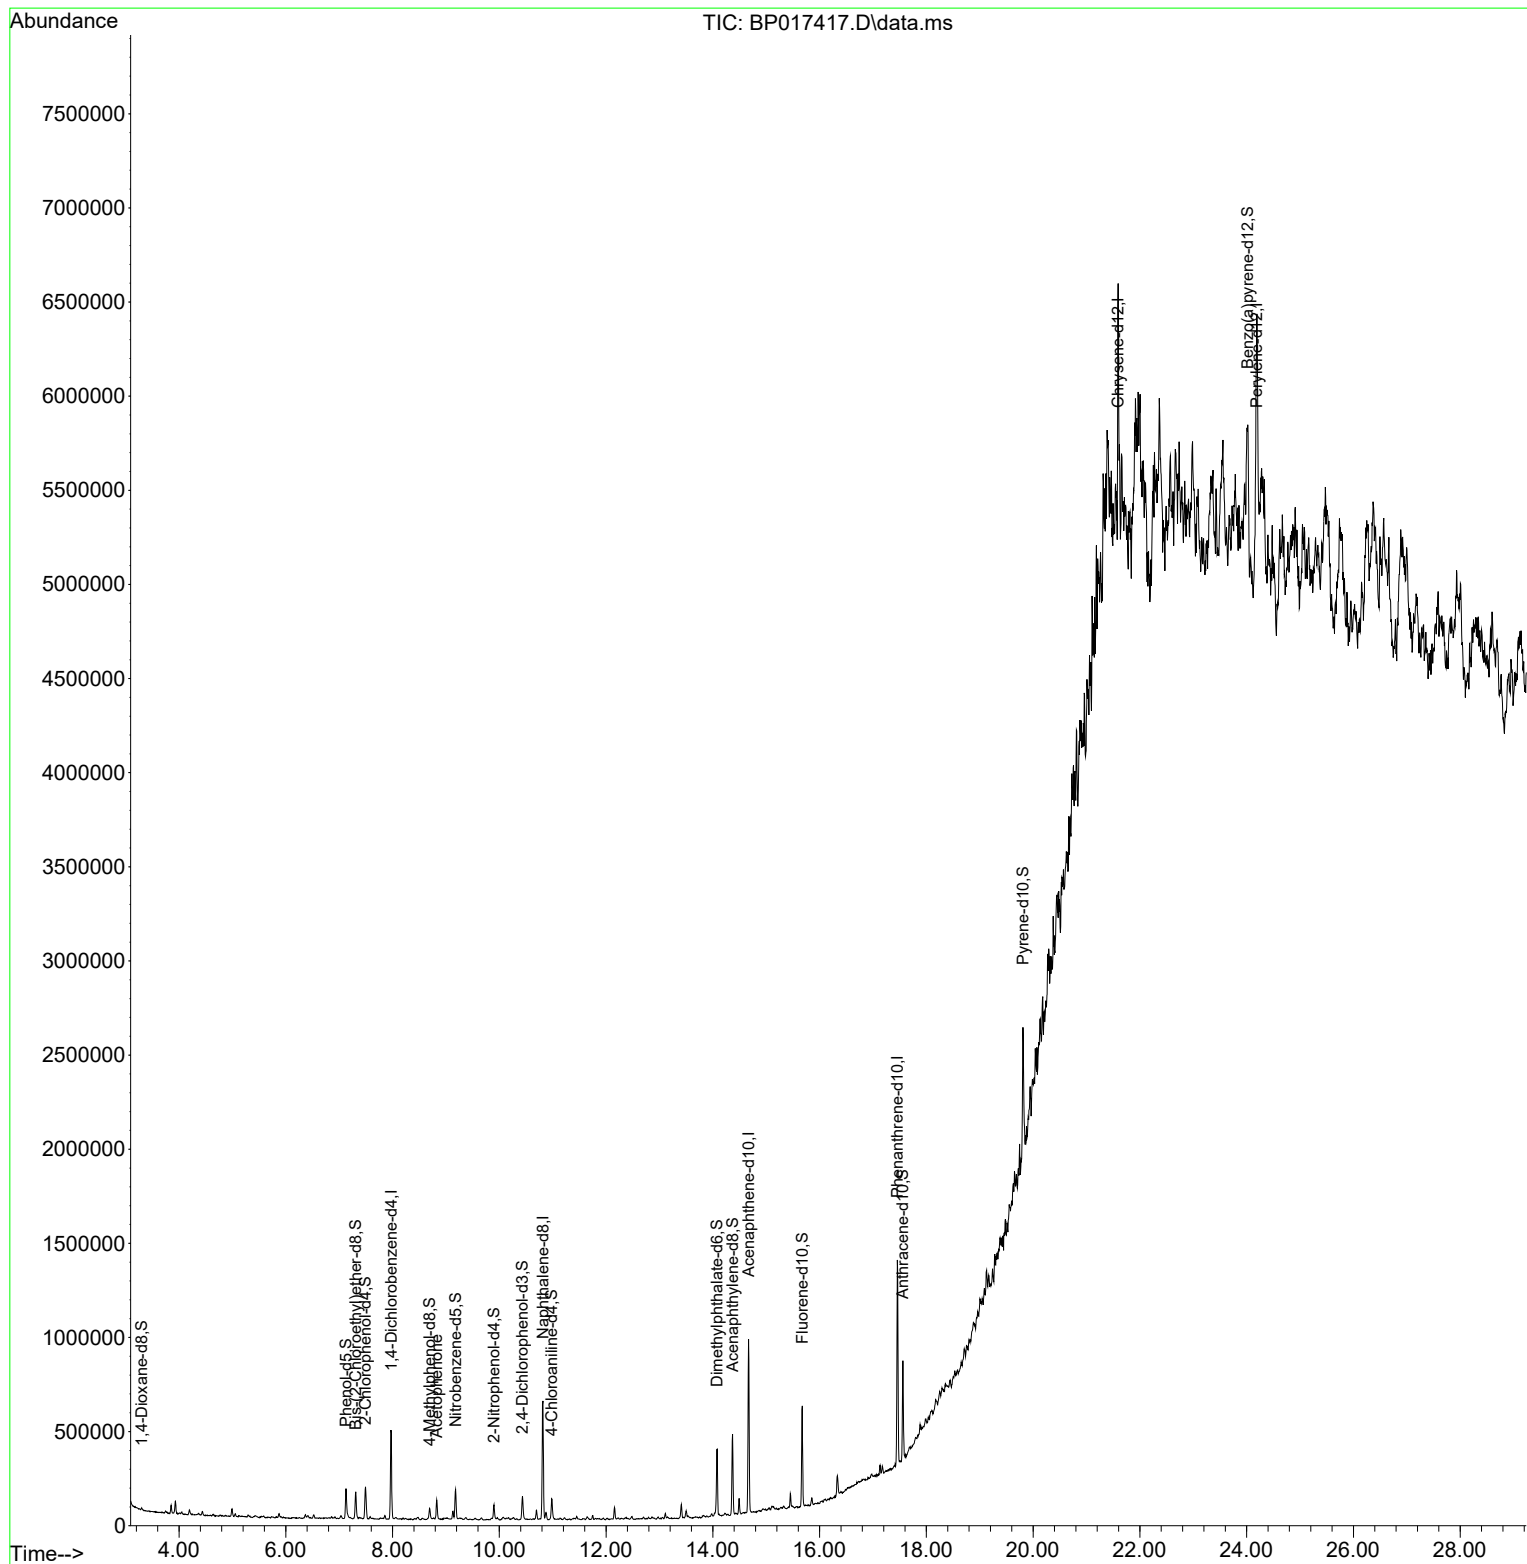

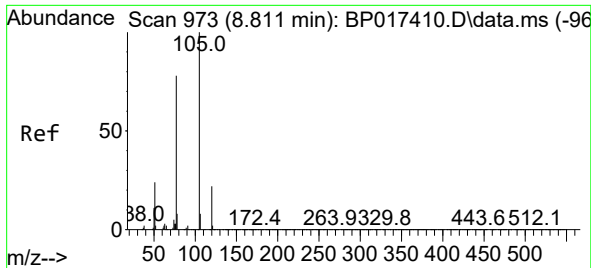

#16
 Acetophenone
 Concen: 4.213 ng/ul
 RT: 8.828 min Scan# 91
 Delta R.T. 0.018 min
 Lab File: BP017417.D
 Acq: 28 Sep 2023 16:57

Instrument :
 BNA_P
 ClientSampleId :
 EZYF2

Tgt Ion:105 Resp: 53231
 Ion Ratio Lower Upper
 105 100
 77 81.2 63.6 95.4
 51 26.6 19.2 28.8

