




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP092823\
Data File : BP017415.D
Acq On : 28 Sep 2023 15:49
Operator : MA/JU
Sample : 04417-24
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
EZYF0

Manual IntegrationsAPPROVED

Quant Time: Sep 28 22:30:50 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP092023.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Sep 28 15:31:53 2023
Response via : Initial Calibration

Reviewed By :Yogesh Patel 09/29/2023
Supervised By :mohammad ahmed 10/02/2023

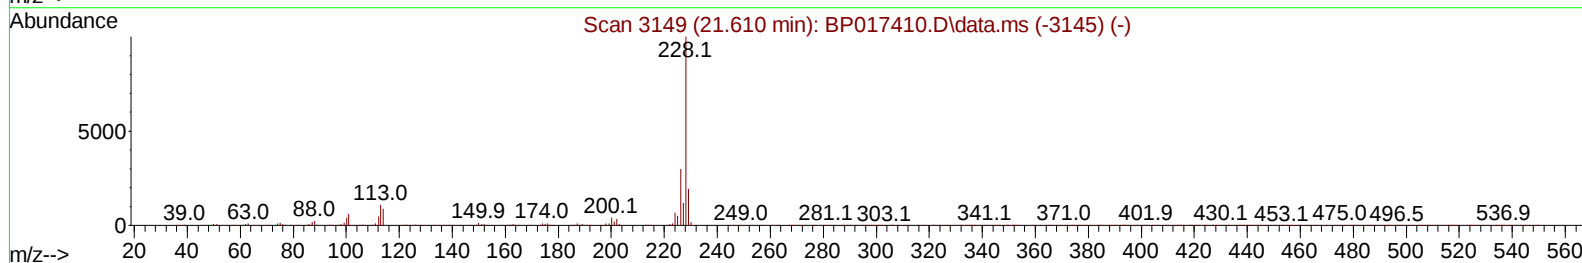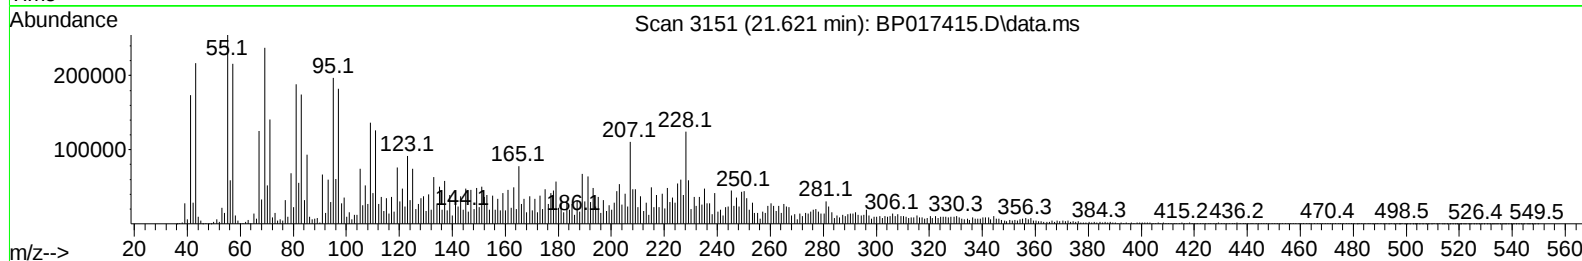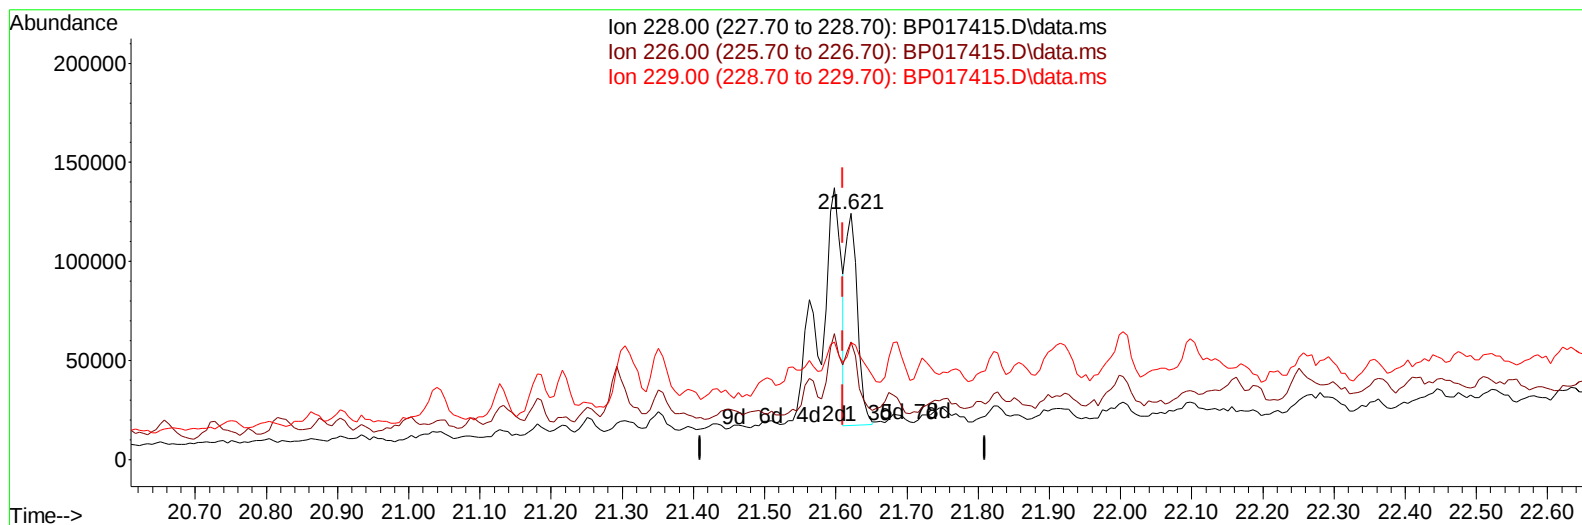

TIC: BP017415.D\data.ms

(87) Chrysene

21.621min (+ 0.012) 1.99 ng/u1

response 120720

Ion	Exp%	Act%
228.00	100.00	100.00
226.00	30.10	47.70#
229.00	18.80	47.59#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP092823\
 Data File : BP017415.D
 Acq On : 28 Sep 2023 15:49
 Operator : MA/JU
 Sample : 04417-24
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 EZYF0

Manual IntegrationsAPPROVED

Quant Time: Sep 28 22:30:50 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP092023.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Sep 28 15:31:53 2023
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 09/29/2023
 Supervised By :mohammad ahmed 10/02/2023

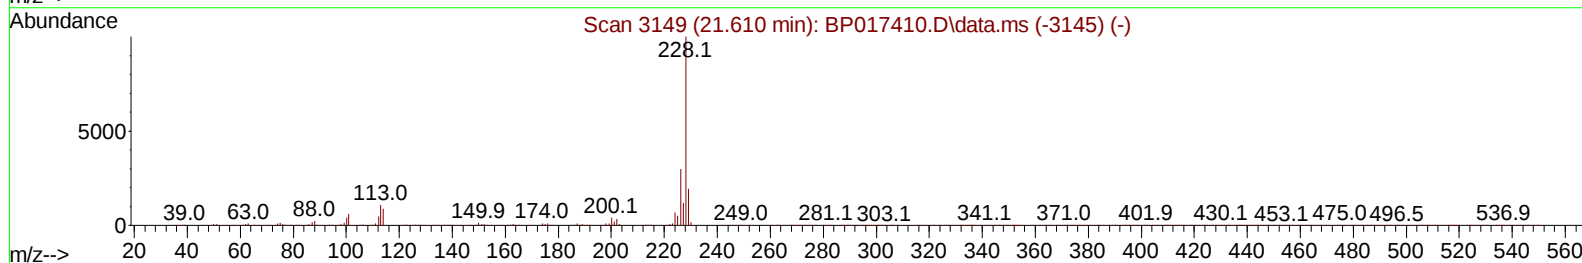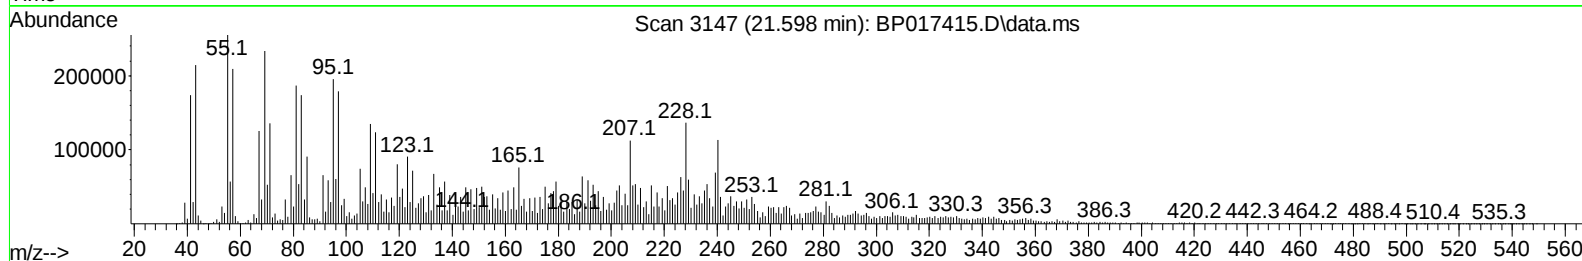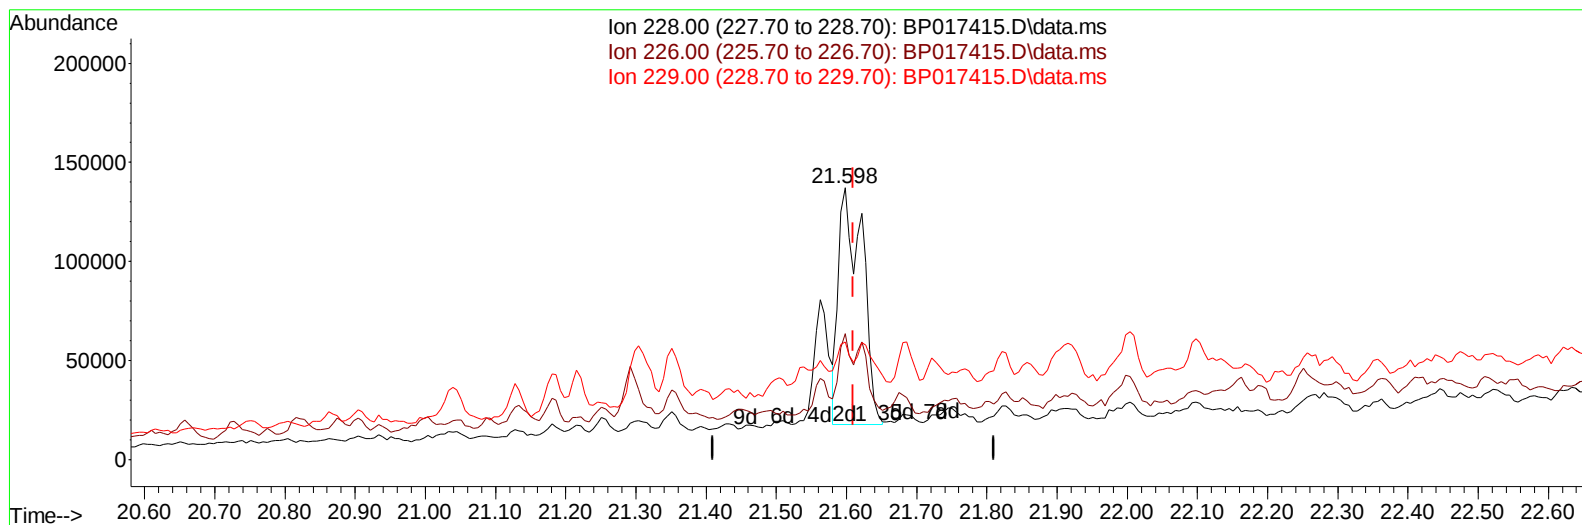

TIC: BP017415.D\data.ms

(87) Chrysene

21.598min (-0.012) 4.62 ng/u1 m

response 279780

Ion	Exp%	Act%
228.00	100.00	100.00
226.00	30.10	46.32#
229.00	18.80	43.28#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP092823\
 Data File : BP017415.D
 Acq On : 28 Sep 2023 15:49
 Operator : MA/JU
 Sample : 04417-24
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 EZYF0

Manual IntegrationsAPPROVED

Quant Time: Sep 28 23:08:37 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP092023.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Sep 28 15:31:53 2023
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 09/29/2023
 Supervised By :mohammad ahmed 10/02/2023

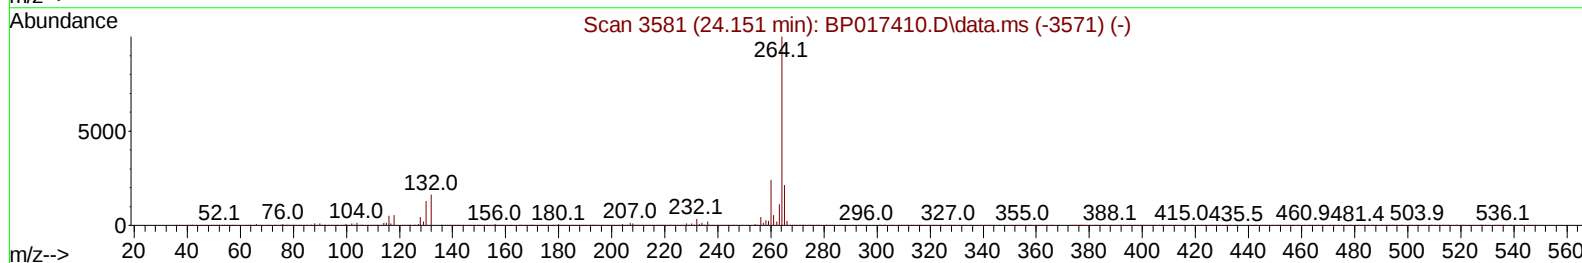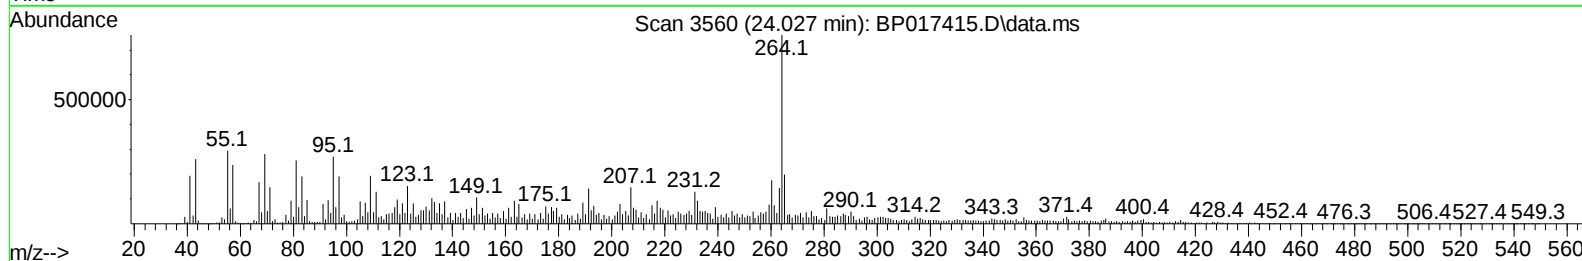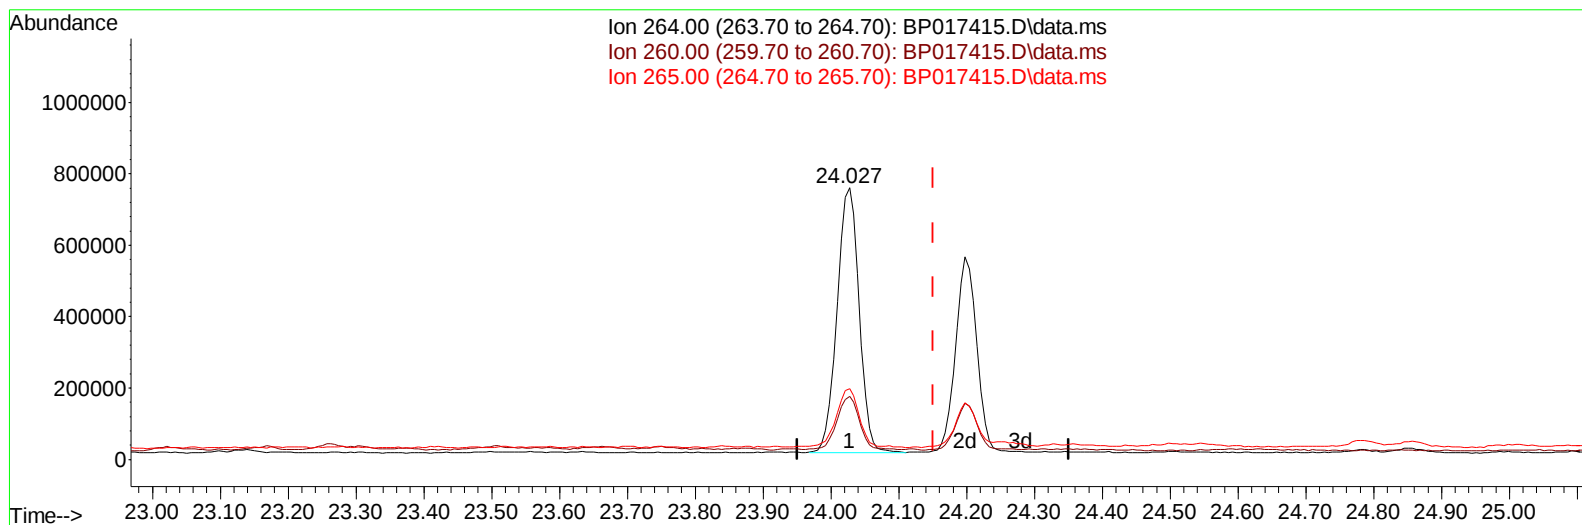

TIC: BP017415.D\data.ms

(88) Perylene-d12 (I)

24.027min (-0.124) 20.00 ng/u1

response 1664976

Ion	Exp%	Act%
264.00	100.00	100.00
260.00	24.00	23.23
265.00	22.30	26.14
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP092823\
 Data File : BP017415.D
 Acq On : 28 Sep 2023 15:49
 Operator : MA/JU
 Sample : 04417-24
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 EZYF0

Manual IntegrationsAPPROVED

Quant Time: Sep 28 23:08:37 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP092023.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Sep 28 15:31:53 2023
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 09/29/2023
 Supervised By :mohammad ahmed 10/02/2023

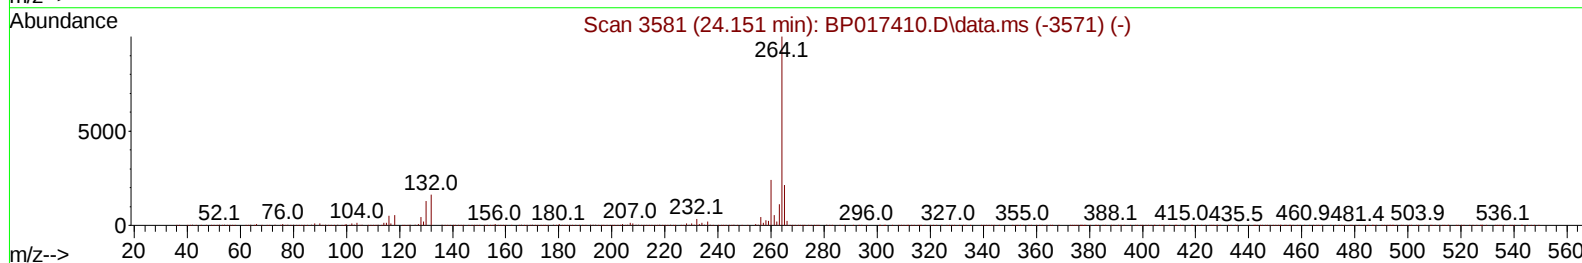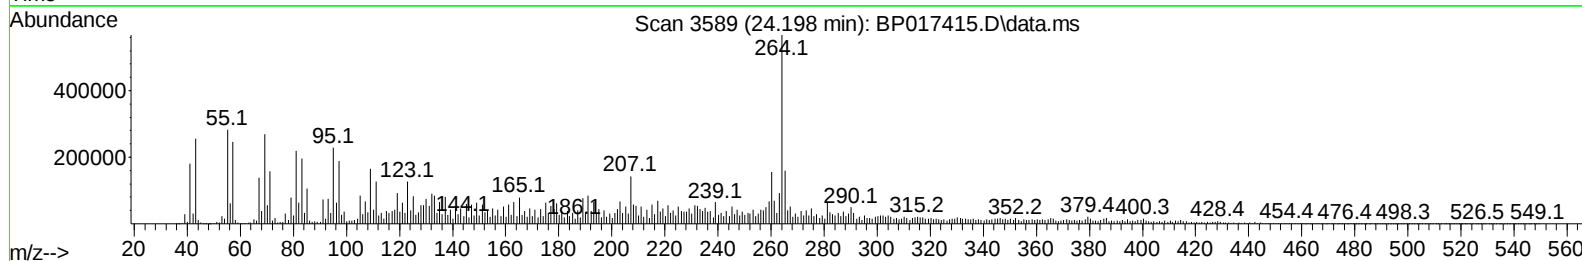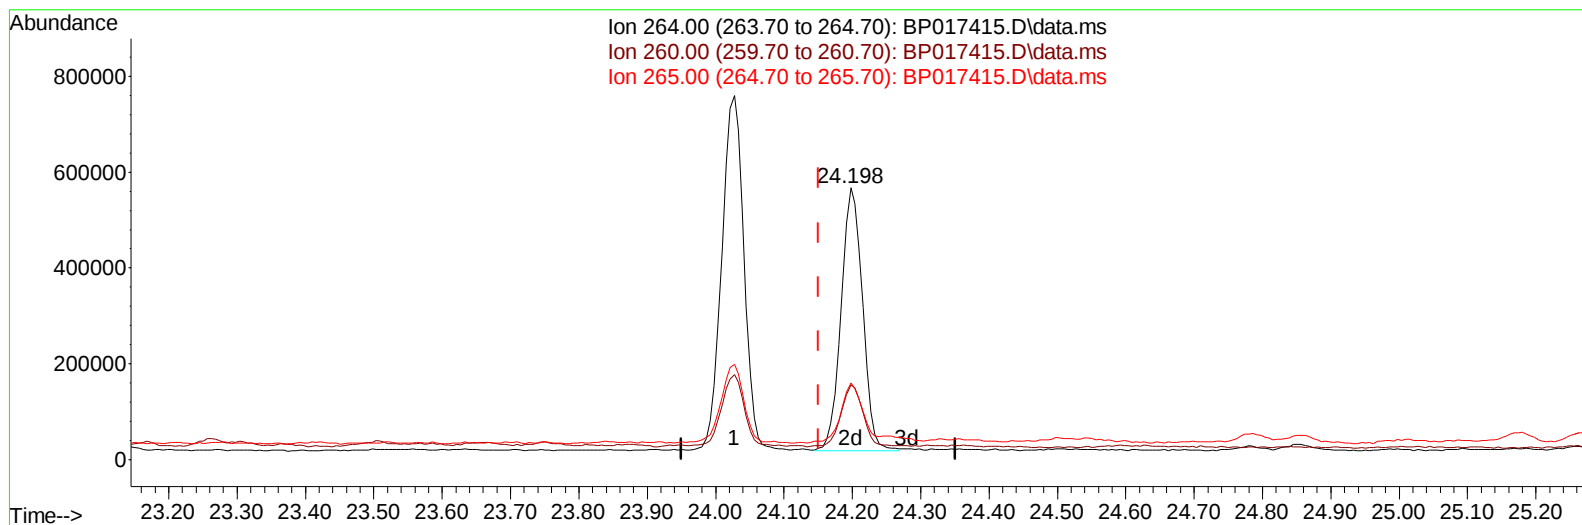

TIC: BP017415.D\data.ms

(88) Perylene-d12 (I)

24.198min (+ 0.047) 20.00 ng/ul m

response 1191021

Ion	Exp%	Act%
264.00	100.00	100.00
260.00	24.00	27.60
265.00	22.30	28.16#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP092823\
 Data File : BP017415.D
 Acq On : 28 Sep 2023 15:49
 Operator : MA/JU
 Sample : 04417-24
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 EZYF0

Manual IntegrationsAPPROVED

Quant Time: Sep 28 23:09:18 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP092023.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Sep 28 15:31:53 2023
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 09/29/2023
 Supervised By :mohammad ahmed 10/02/2023

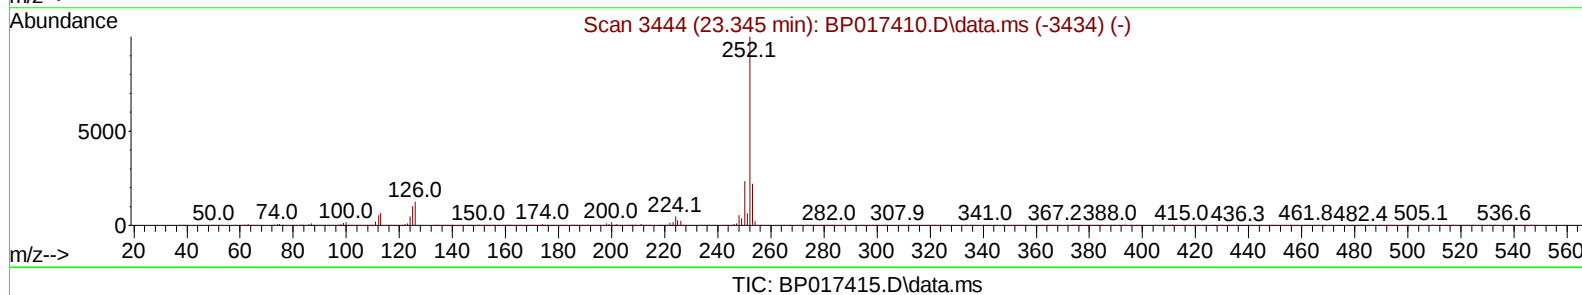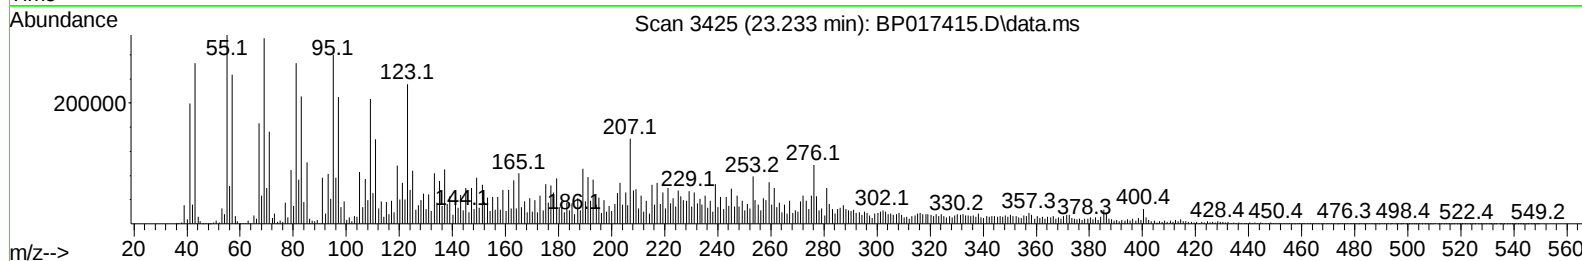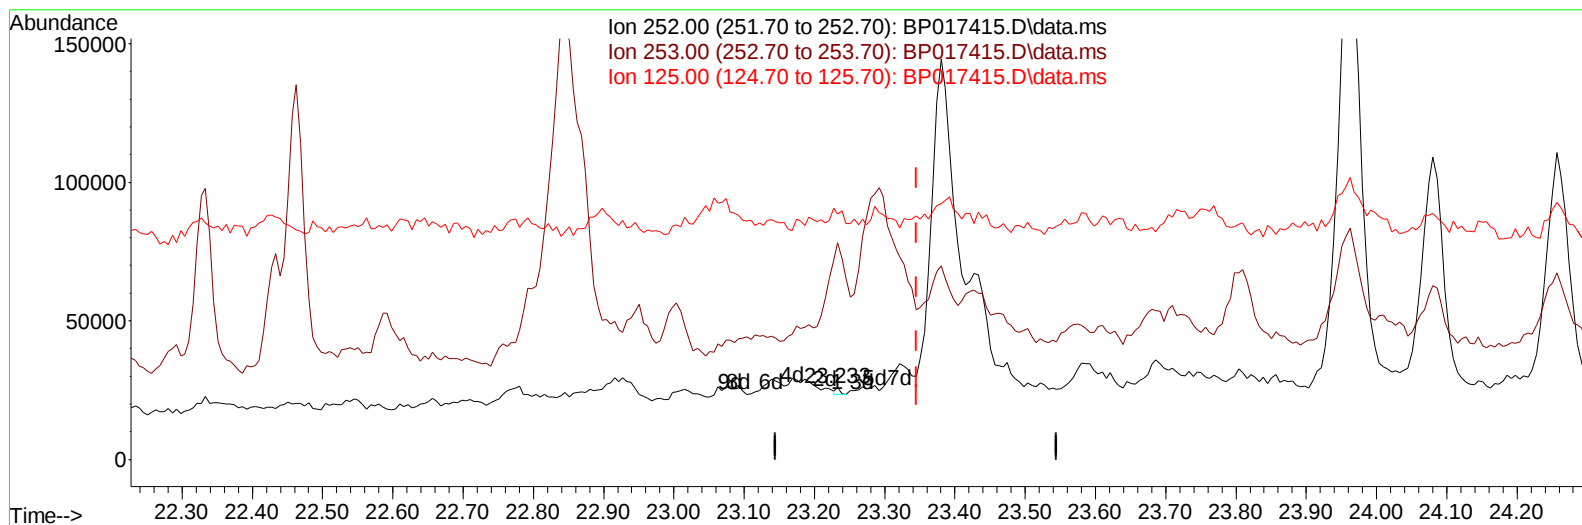

(90) Benzo(b)fluoranthene

23.233min (-0.112) 0.01 ng/u1

response 870

Ion	Exp%	Act%
252.00	100.00	100.00
253.00	21.70	301.42#
125.00	9.80	341.39#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP092823\
Data File : BP017415.D
Acq On : 28 Sep 2023 15:49
Operator : MA/JU
Sample : 04417-24
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
EZYF0

Manual IntegrationsAPPROVED

Quant Time: Sep 28 23:09:18 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP092023.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Sep 28 15:31:53 2023
Response via : Initial Calibration

Reviewed By :Yogesh Patel 09/29/2023
Supervised By :mohammad ahmed 10/02/2023

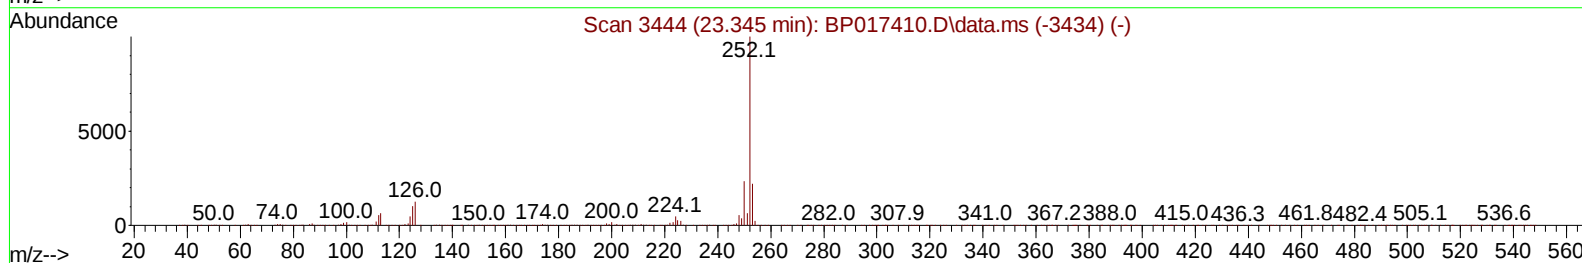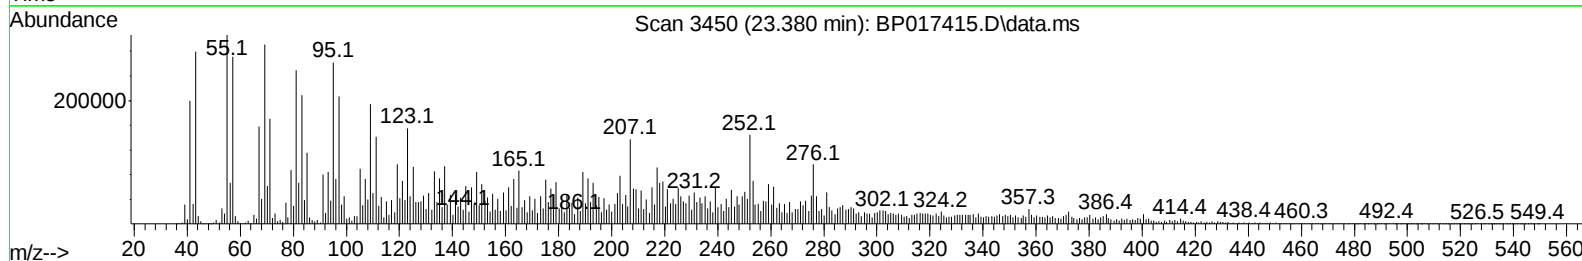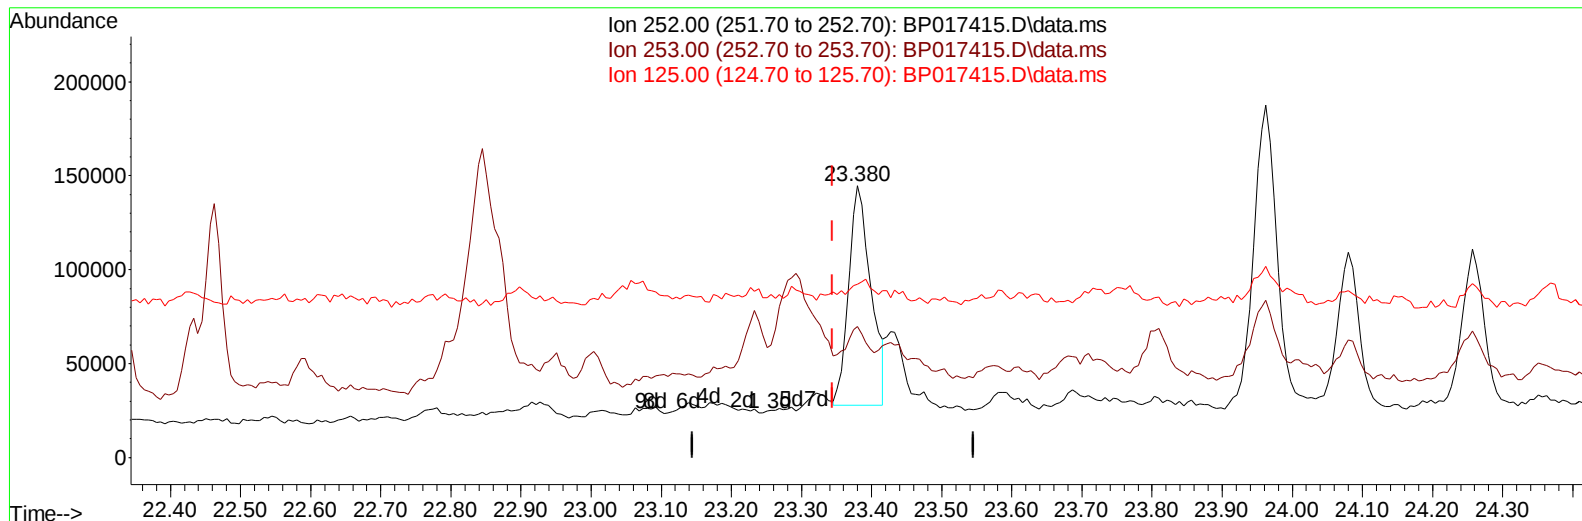

TIC: BP017415.D\data.ms

(90) Benzo(b)fluoranthene

23.380min (+ 0.035) 3.70 ng/u1 m

response 259991

Ion	Exp%	Act%
252.00	100.00	100.00
253.00	21.70	48.33#
125.00	9.80	63.77#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP092823\
 Data File : BP017415.D
 Acq On : 28 Sep 2023 15:49
 Operator : MA/JU
 Sample : 04417-24
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 EZYF0

Manual IntegrationsAPPROVED

Quant Time: Sep 28 23:10:01 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP092023.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Sep 28 15:31:53 2023
 Response via : Initial Calibration

Reviewed By :Yogesh




Patel

09/29/2023

Supervised By :mohammad

ahmed

10/02/2023

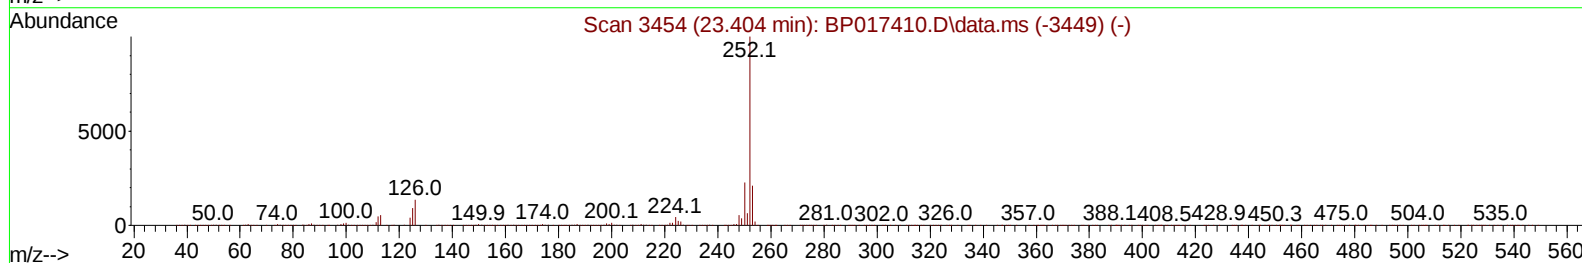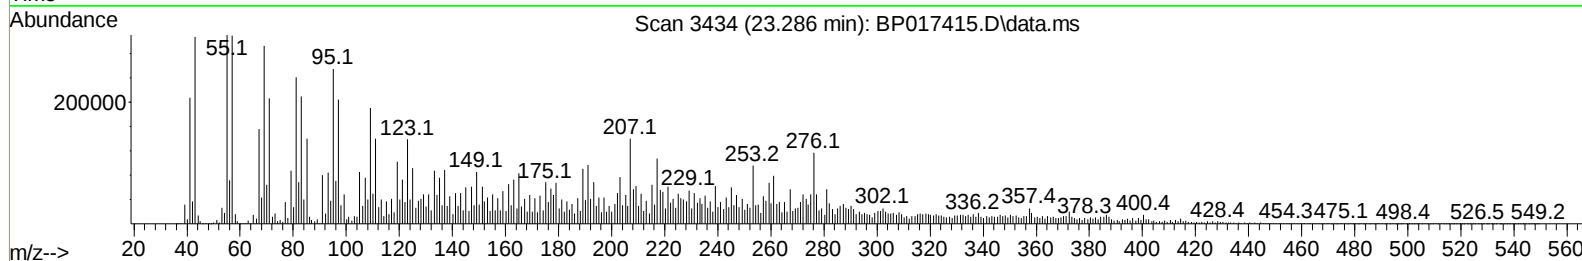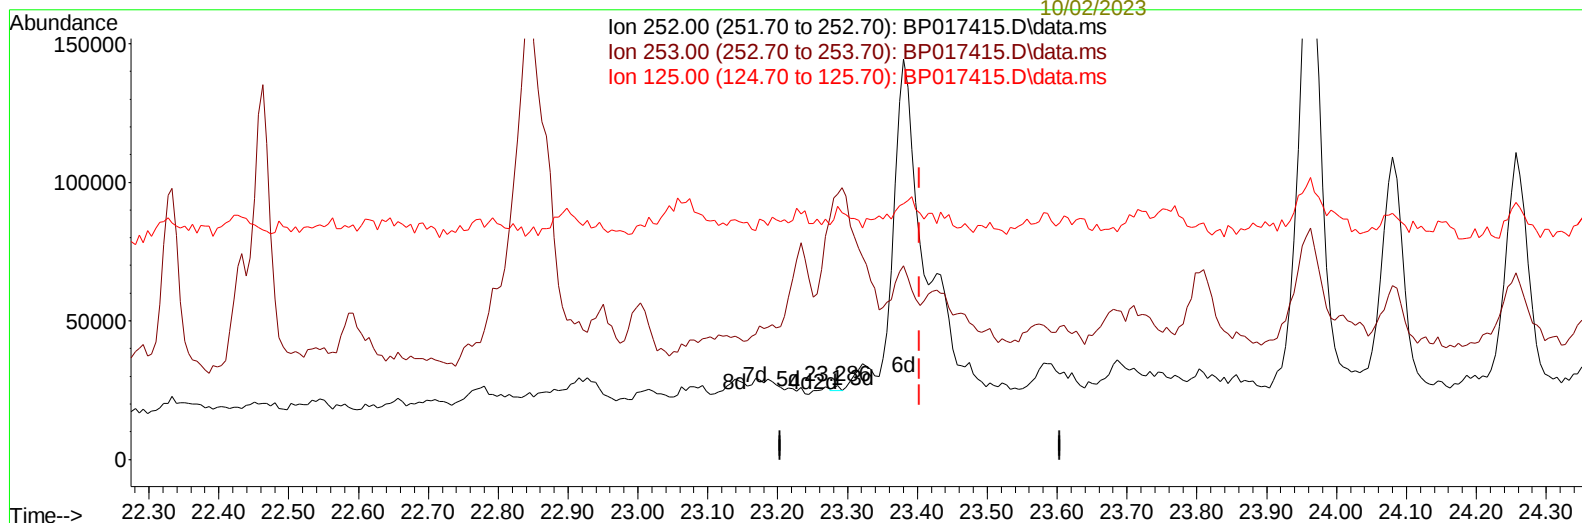

TIC: BP017415.D\data.ms

(91) Benzo(k)fluoranthene

23.286min (-0.118) 0.01 ng/u1

response 957

Ion	Exp%	Act%
252.00	100.00	100.00
253.00	22.40	359.00#
125.00	9.70	342.32#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP092823\
 Data File : BP017415.D
 Acq On : 28 Sep 2023 15:49
 Operator : MA/JU
 Sample : 04417-24
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 EZYF0

Manual IntegrationsAPPROVED

Quant Time: Sep 28 23:10:01 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP092023.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Sep 28 15:31:53 2023
 Response via : Initial Calibration




Reviewed By :Yogesh

Patel

09/29/2023

Supervised By :mohammad
 ahmed

10/02/2023

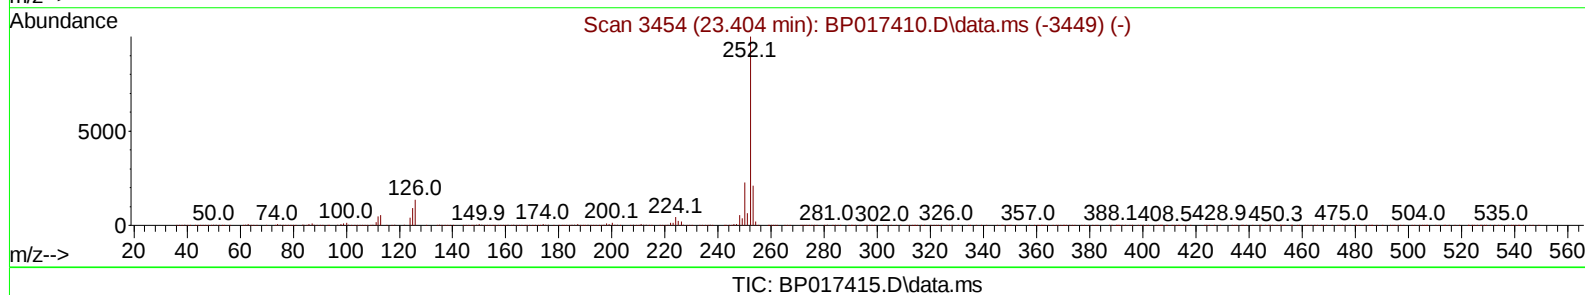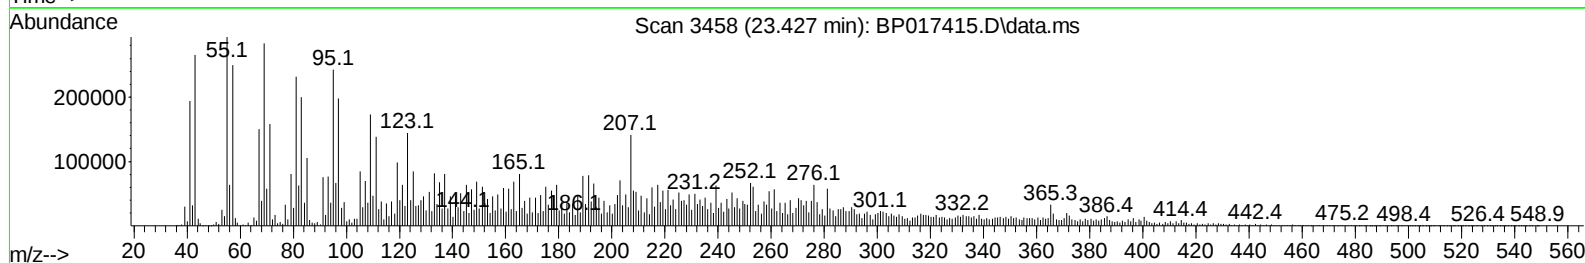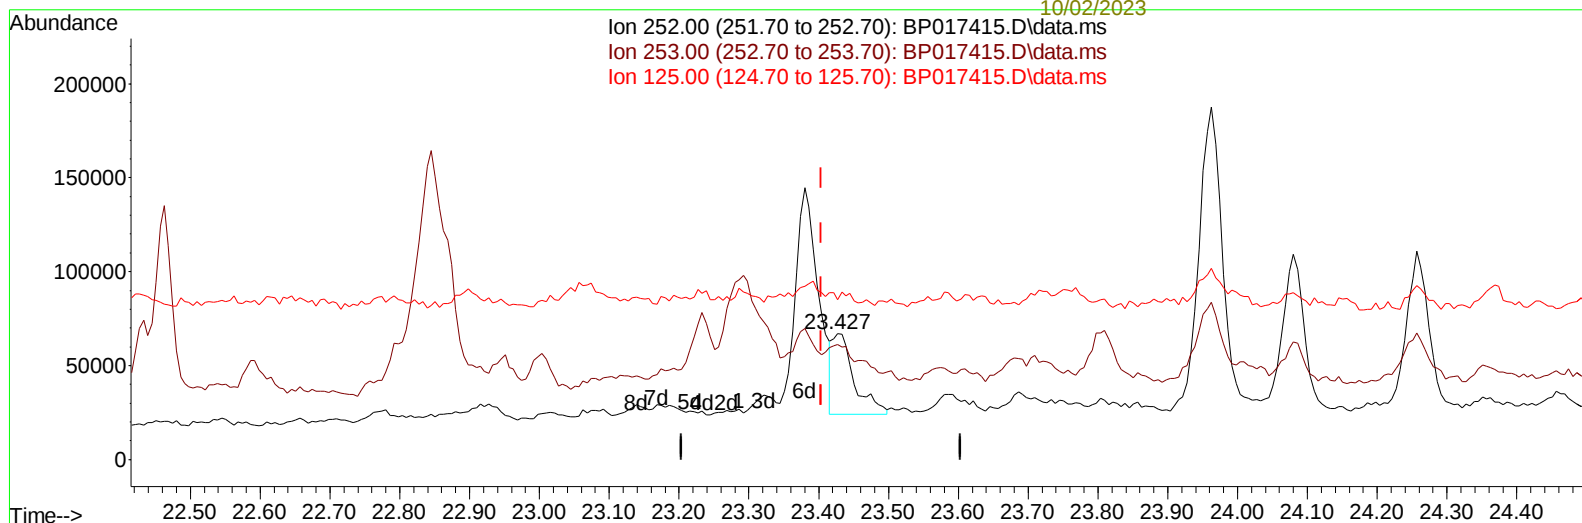

(91) Benzo(k)fluoranthene

23.427min (+ 0.023) 1.30 ng/ul m

response 92063

Ion	Exp%	Act%
252.00	100.00	100.00
253.00	22.40	91.20#
125.00	9.70	126.89#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP092823\
 Data File : BP017415.D
 Acq On : 28 Sep 2023 15:49
 Operator : MA/JU
 Sample : 04417-24
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 EZYF0

Manual IntegrationsAPPROVED

Quant Time: Sep 28 23:10:28 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP092023.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Sep 28 15:31:53 2023
 Response via : Initial Calibration




Reviewed By :Yogesh

Patel

09/29/2023

Supervised By :mohammad
 ahmed

10/02/2023

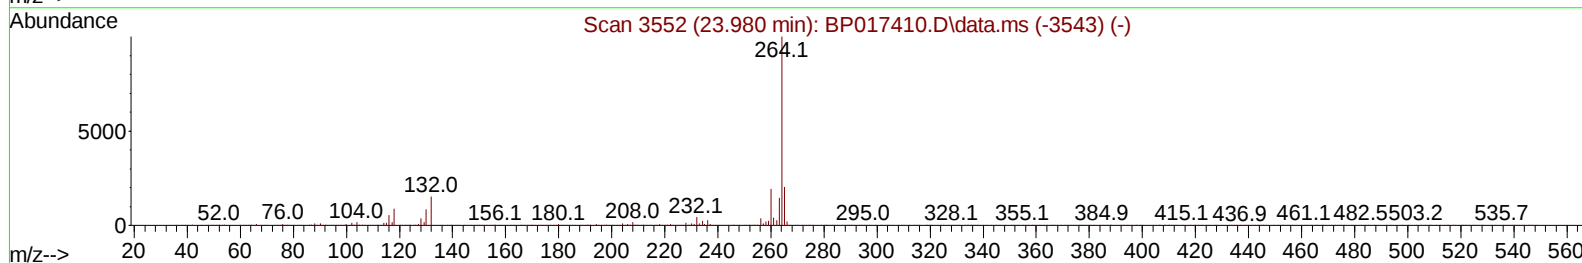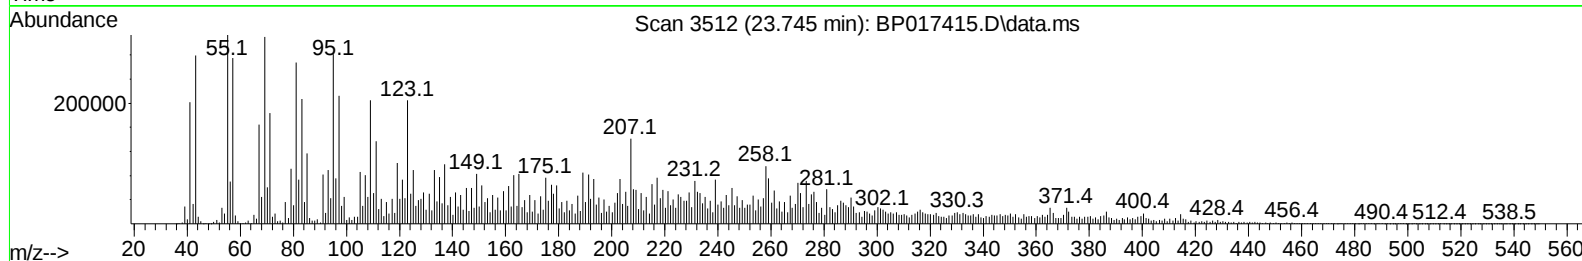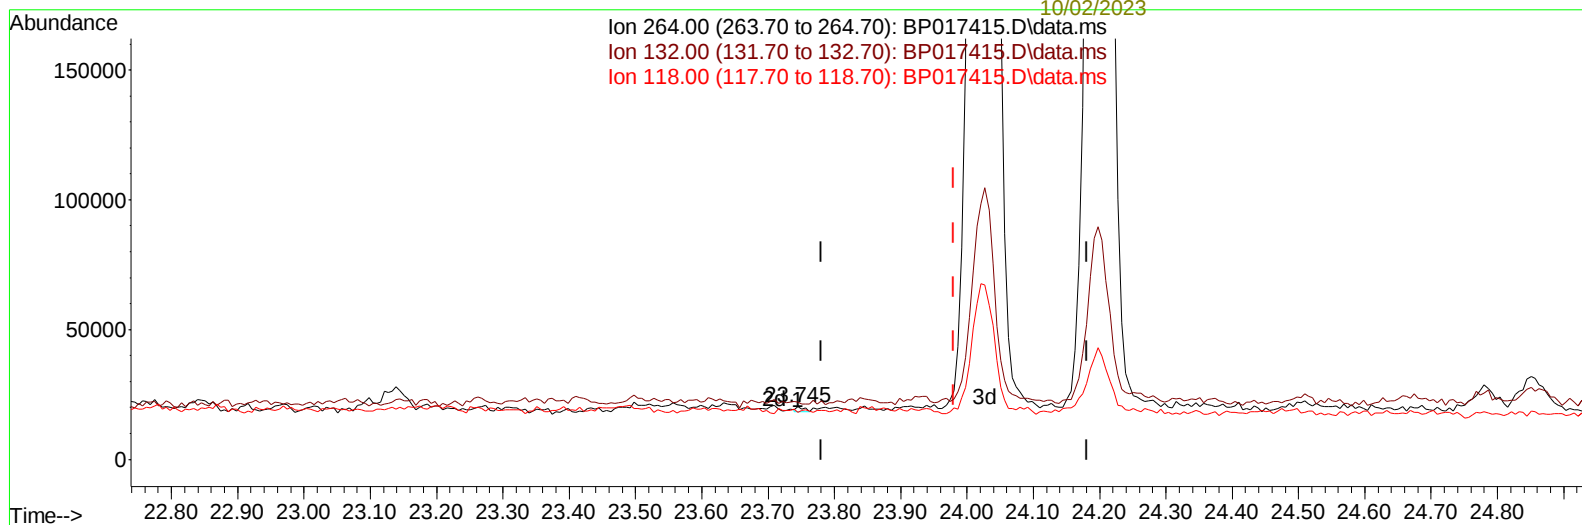

TIC: BP017415.D\data.ms

(92) Benzo(a)pyrene-d12 (S)

23.745min (-0.235) 0.03 ng/u1

response 1518

Ion	Exp%	Act%
264.00	100.00	100.00
132.00	17.40	108.81#
118.00	9.90	89.25#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP092823\
 Data File : BP017415.D
 Acq On : 28 Sep 2023 15:49
 Operator : MA/JU
 Sample : 04417-24
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 EZYF0

Manual IntegrationsAPPROVED

Quant Time: Sep 28 23:10:28 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP092023.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Sep 28 15:31:53 2023
 Response via : Initial Calibration

Reviewed By :Yogesh




Patel

09/29/2023

Supervised By :mohammad

ahmed

10/02/2023

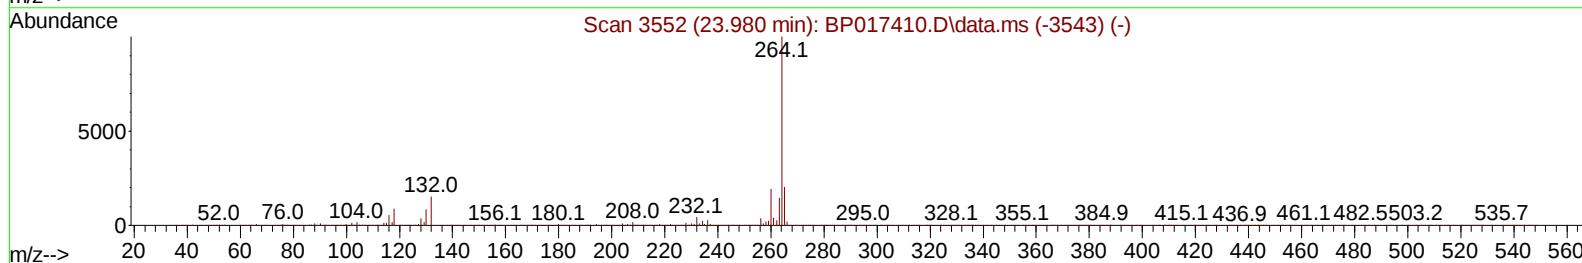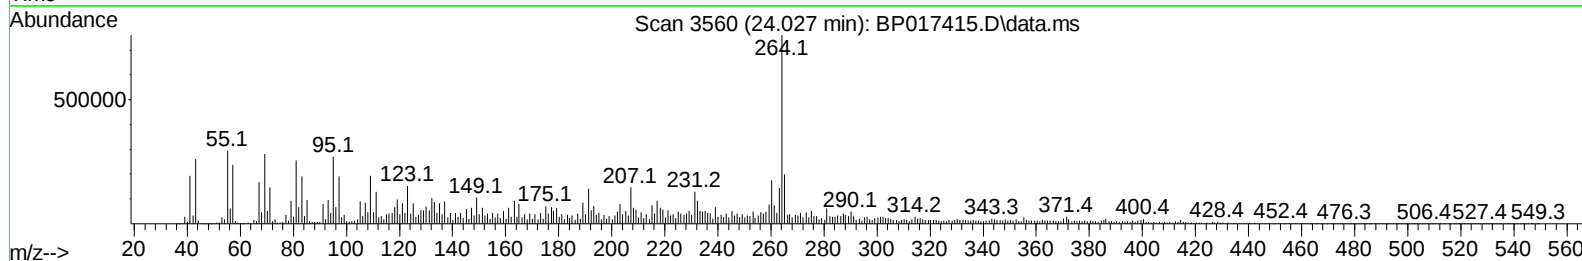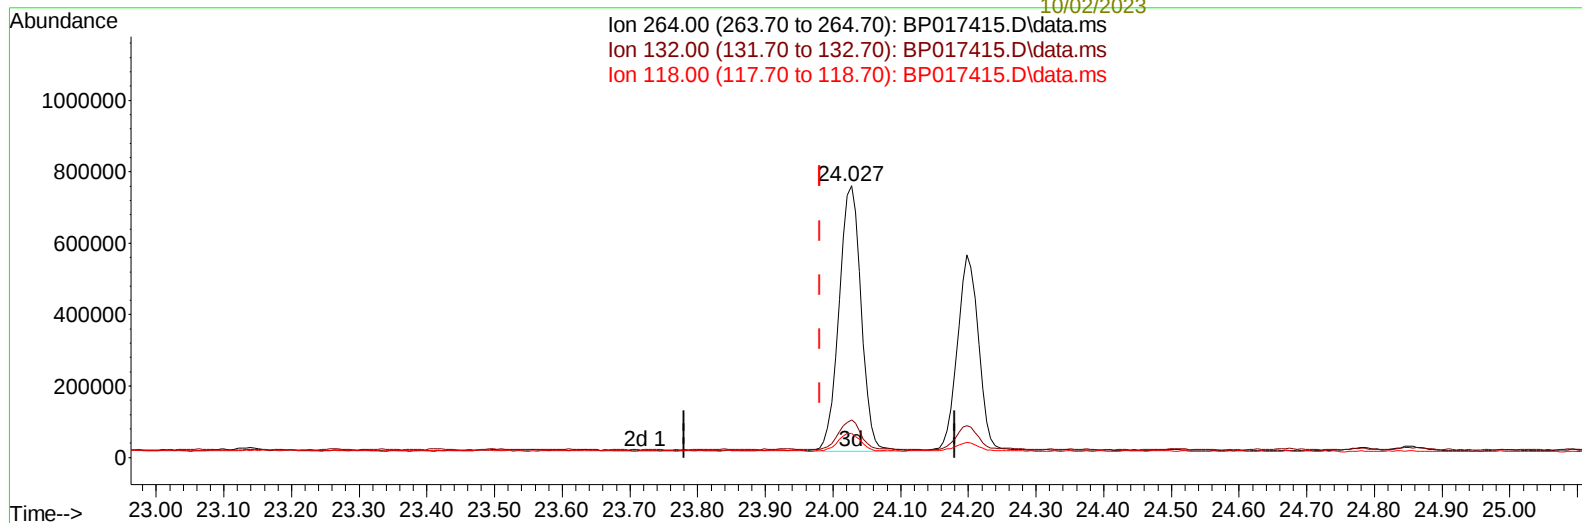

TIC: BP017415.D\data.ms

(92) Benzo(a)pyrene-d12 (S)

24.027min (+ 0.047) 29.37 ng/ul m

response 1684093

Ion	Exp%	Act%
264.00	100.00	100.00
132.00	17.40	13.75#
118.00	9.90	8.83
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP092823\
 Data File : BP017415.D
 Acq On : 28 Sep 2023 15:49
 Operator : MA/JU
 Sample : 04417-24
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 EZYF0

Manual IntegrationsAPPROVED

Quant Time: Sep 28 23:10:55 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP092023.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Sep 28 15:31:53 2023
 Response via : Initial Calibration

Reviewed By :Yogesh




Patel

09/29/2023

Supervised By :mohammad

ahmed

10/02/2023

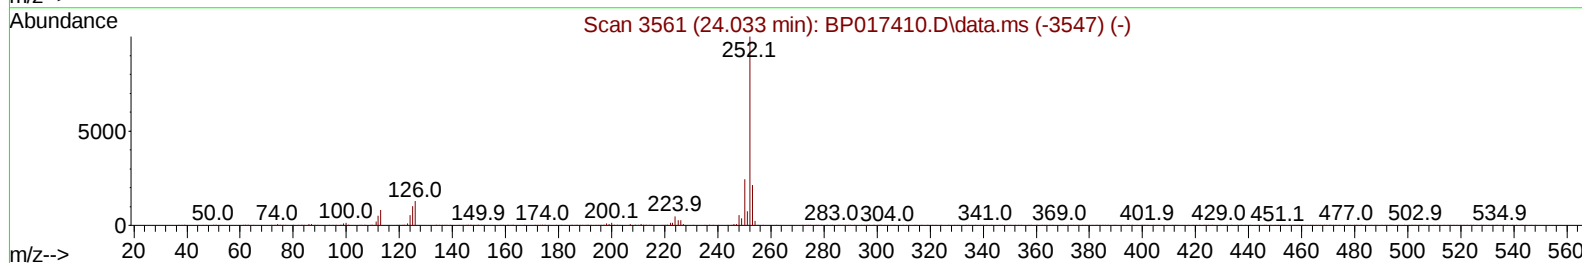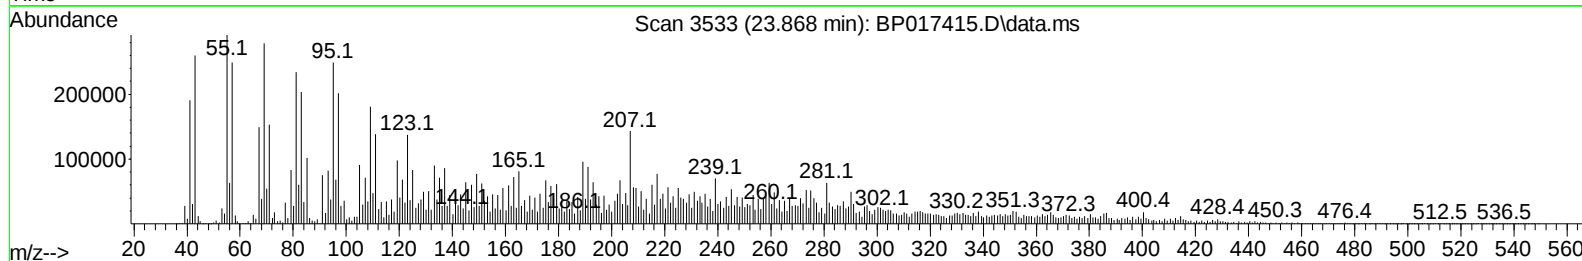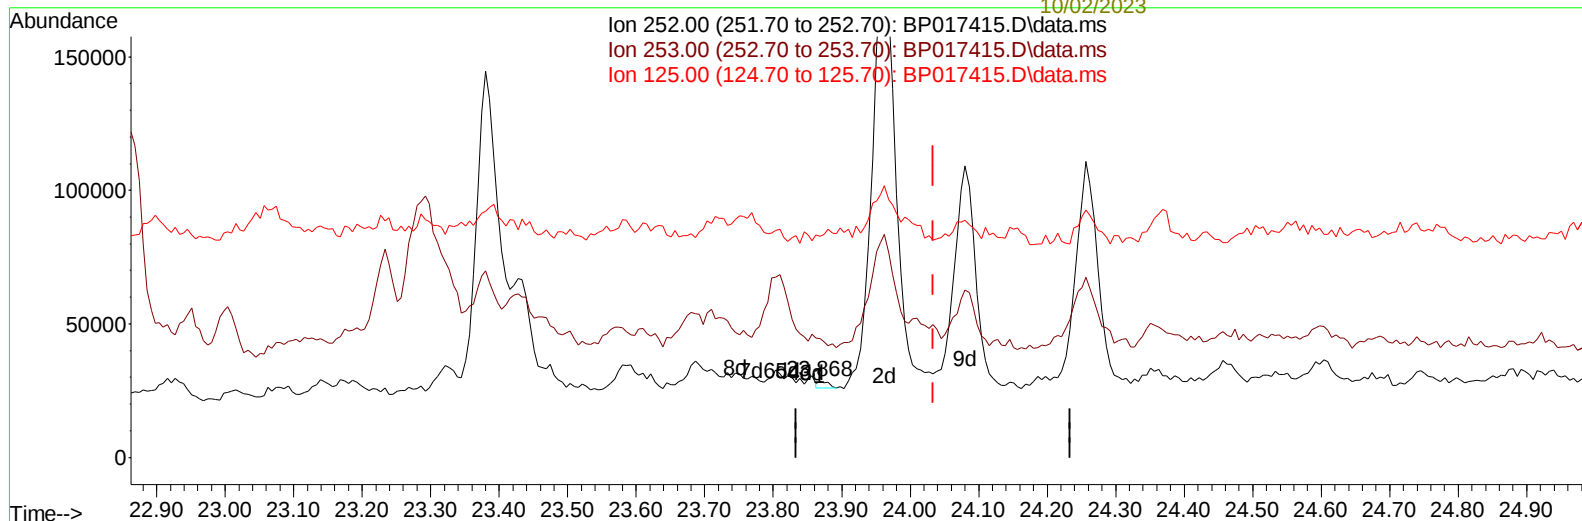

TIC: BP017415.D\data.ms

(93) Benzo(a)pyrene (C)

23.868min (-0.165) 0.04 ng/ul

response 2429

Ion	Exp%	Act%
252.00	100.00	100.00
253.00	21.70	155.85#
125.00	11.10	290.66#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP092823\
Data File : BP017415.D
Acq On : 28 Sep 2023 15:49
Operator : MA/JU
Sample : 04417-24
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
EZYF0

Manual IntegrationsAPPROVED

Quant Time: Sep 28 23:10:55 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP092023.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Sep 28 15:31:53 2023
Response via : Initial Calibration

Reviewed By :Yogesh




Patel

09/29/2023

Supervised By :mohammad

ahmed

10/02/2023

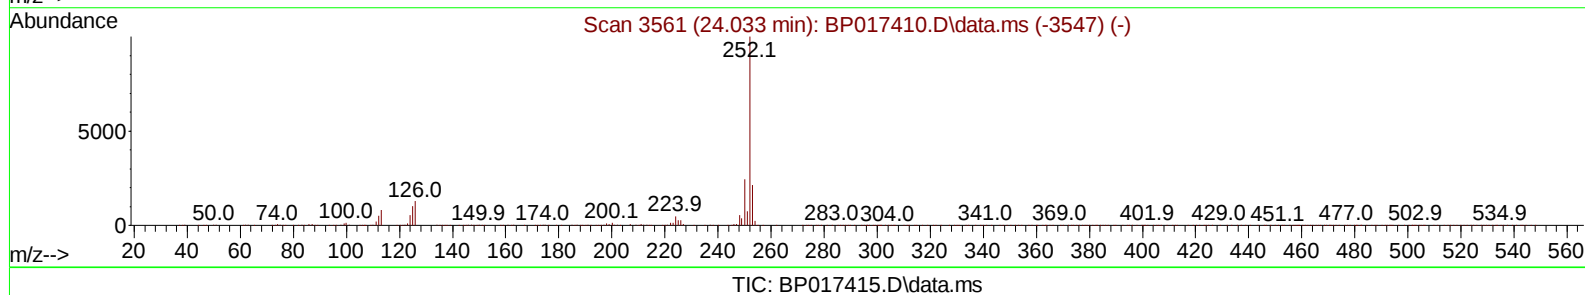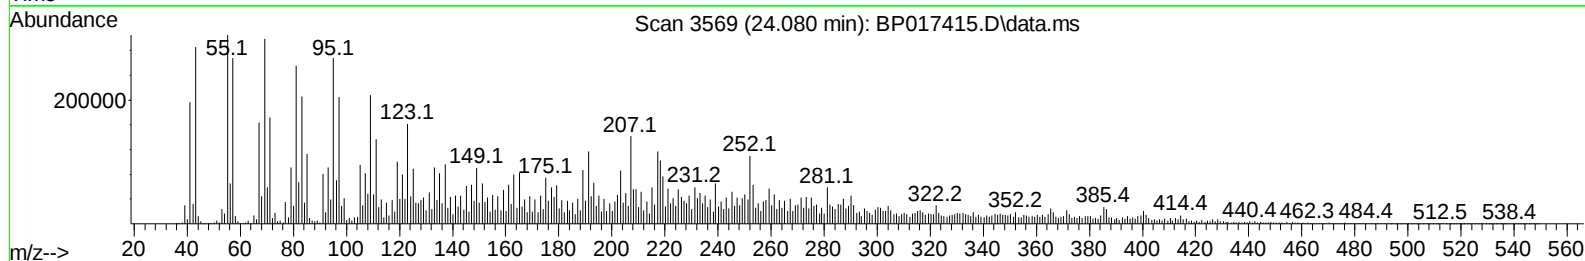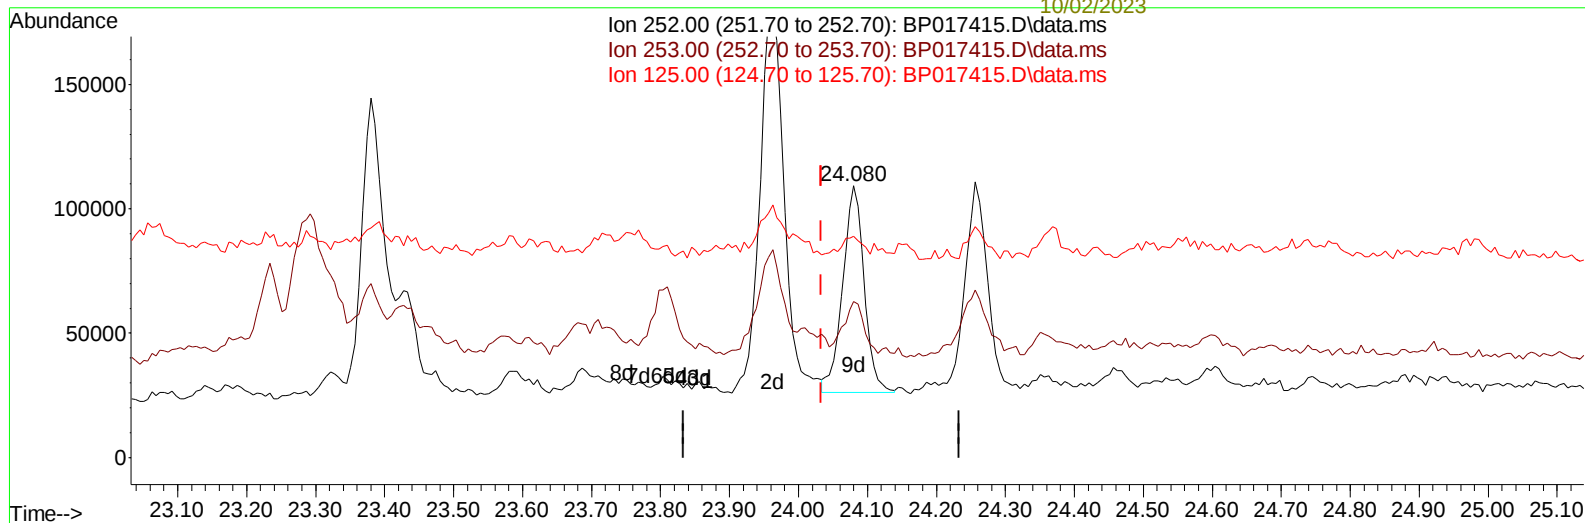

(93) Benzo(a)pyrene (C)

24.080min (+ 0.047) 2.68 ng/ul m

response 180126

Ion	Exp%	Act%
252.00	100.00	100.00
253.00	21.70	57.41#
125.00	11.10	81.36#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP092823\
 Data File : BP017415.D
 Acq On : 28 Sep 2023 15:49
 Operator : MA/JU
 Sample : 04417-24
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 EZYF0

Manual IntegrationsAPPROVED

Quant Time: Sep 28 23:11:28 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP092023.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Sep 28 15:31:53 2023
 Response via : Initial Calibration




Reviewed By :Yogesh

Patel

09/29/2023

Supervised By :mohammad
ahmed

10/02/2023

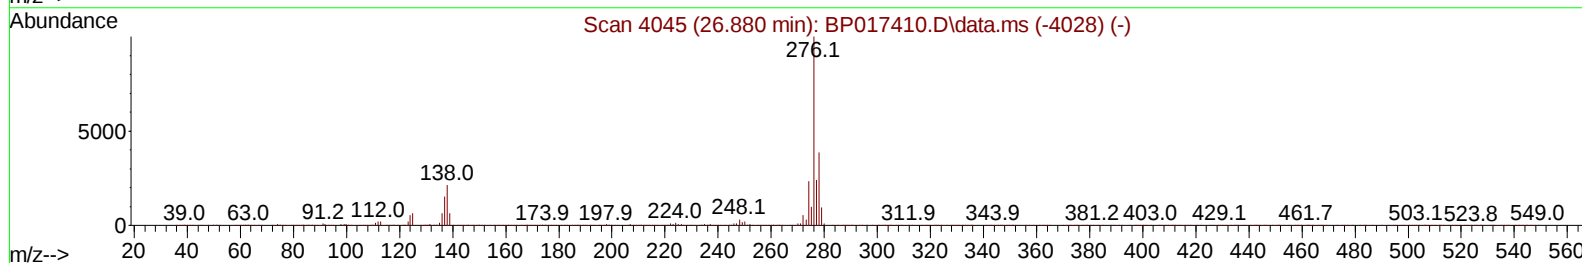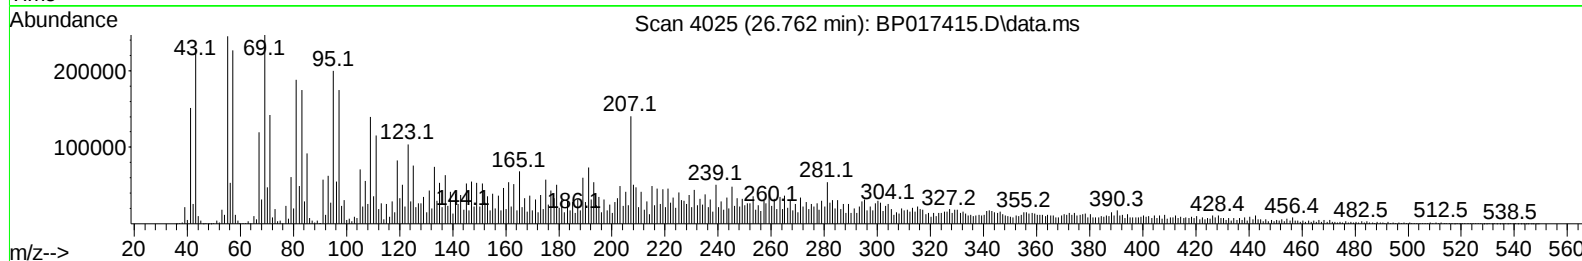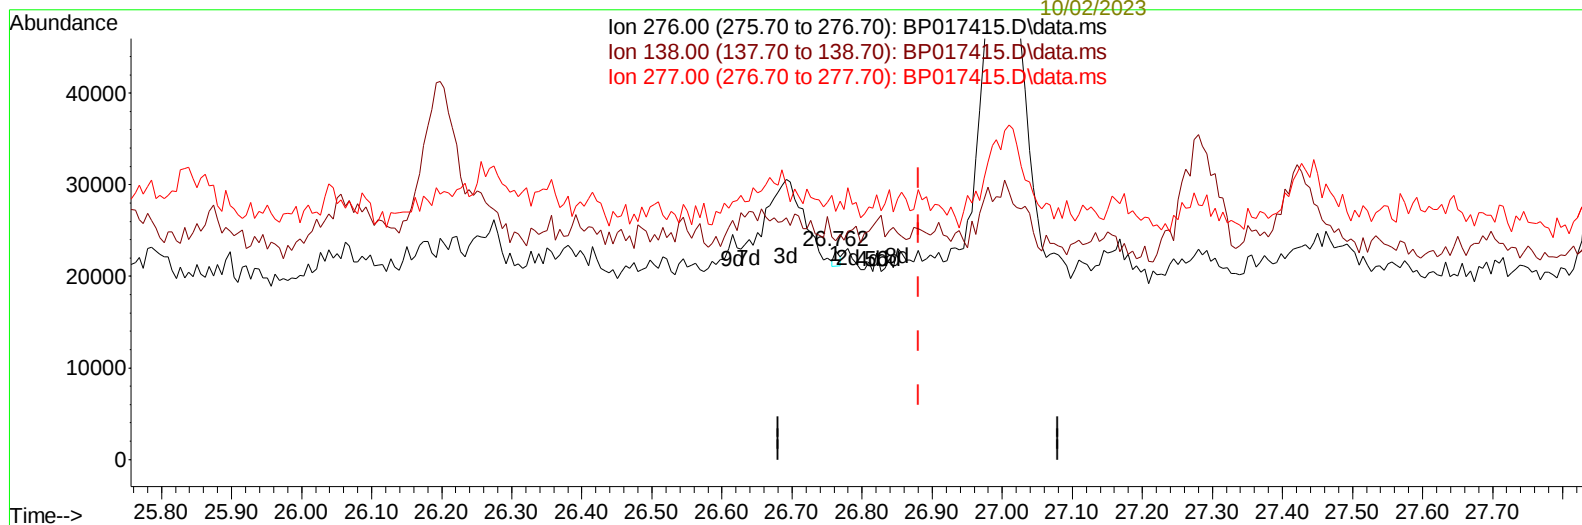

TIC: BP017415.D\data.ms

(94) Indeno(1,2,3-cd)pyrene

26.762min (-0.118) 0.01 ng/ul

response 929

Ion	Exp%	Act%
276.00	100.00	100.00
138.00	22.40	104.85#
277.00	24.40	118.83#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP092823\
Data File : BP017415.D
Acq On : 28 Sep 2023 15:49
Operator : MA/JU
Sample : 04417-24
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
EZYF0

Manual IntegrationsAPPROVED

Quant Time: Sep 28 23:11:28 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP092023.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Sep 28 15:31:53 2023
Response via : Initial Calibration

Reviewed By :Yogesh




Patel

09/29/2023

Supervised By :mohammad

ahmed

10/02/2023

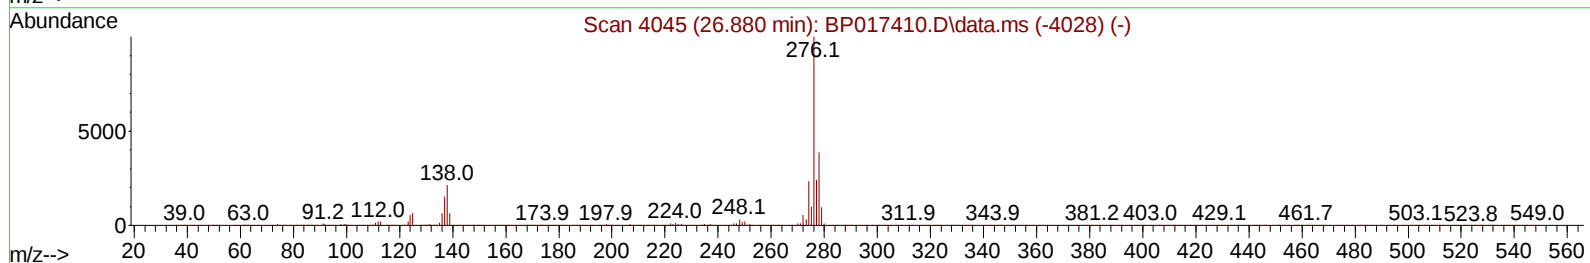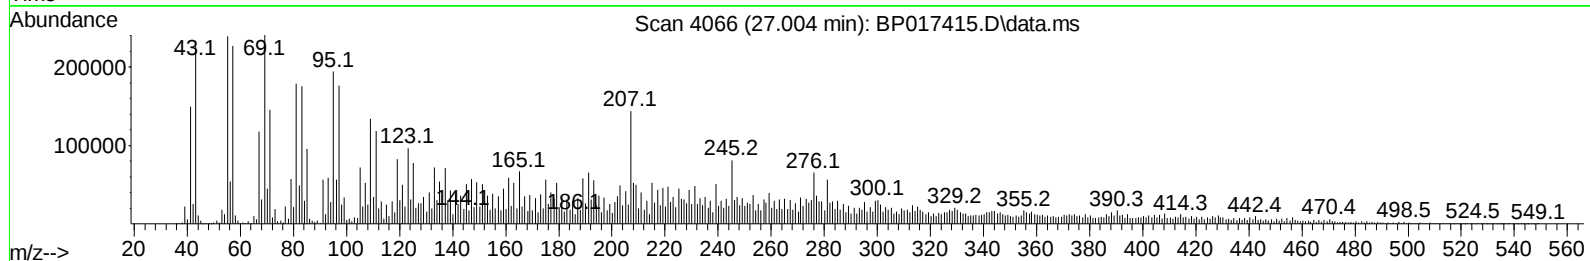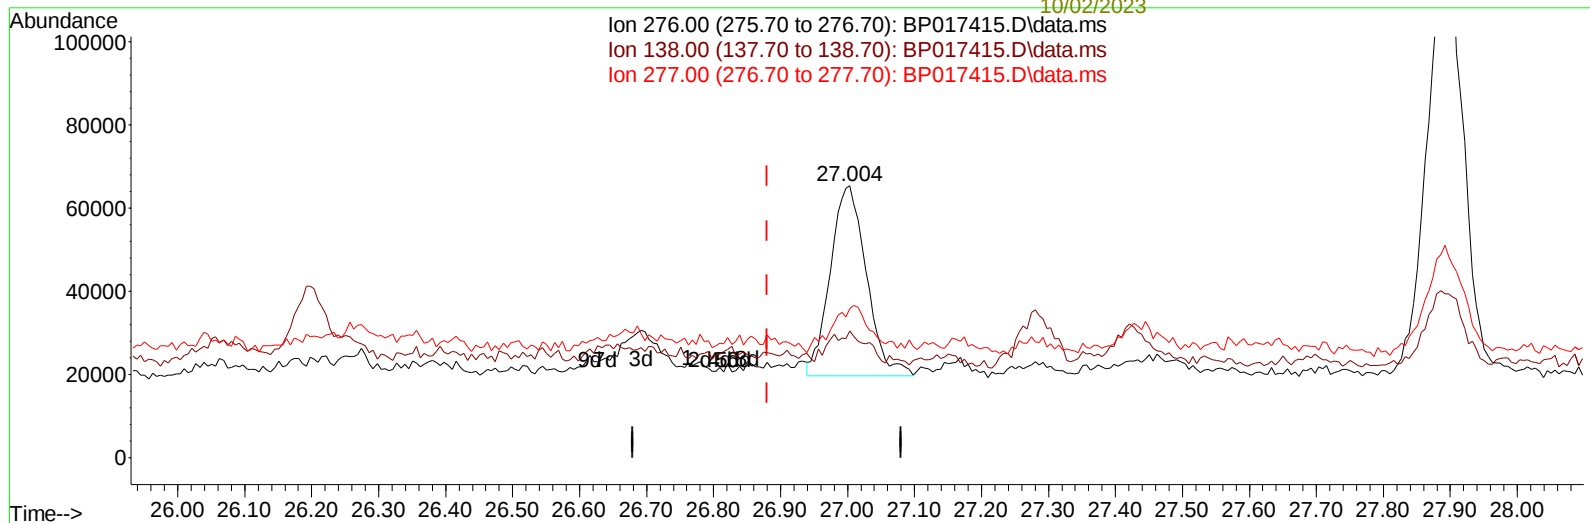

TIC: BP017415.D\data.ms

(94) Indeno(1,2,3-cd)pyrene

27.004min (+ 0.123) 2.03 ng/u1 m

response 171118

Ion	Exp%	Act%
276.00	100.00	100.00
138.00	22.40	46.66#
277.00	24.40	54.93#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP092823\
 Data File : BP017415.D
 Acq On : 28 Sep 2023 15:49
 Operator : MA/JU
 Sample : 04417-24
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 EZYF0

Manual IntegrationsAPPROVED

Quant Time: Sep 28 23:12:09 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP092023.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Sep 28 15:31:53 2023
 Response via : Initial Calibration




Reviewed By :Yogesh

Patel

09/29/2023

Supervised By :mohammad
 ahmed

10/02/2023

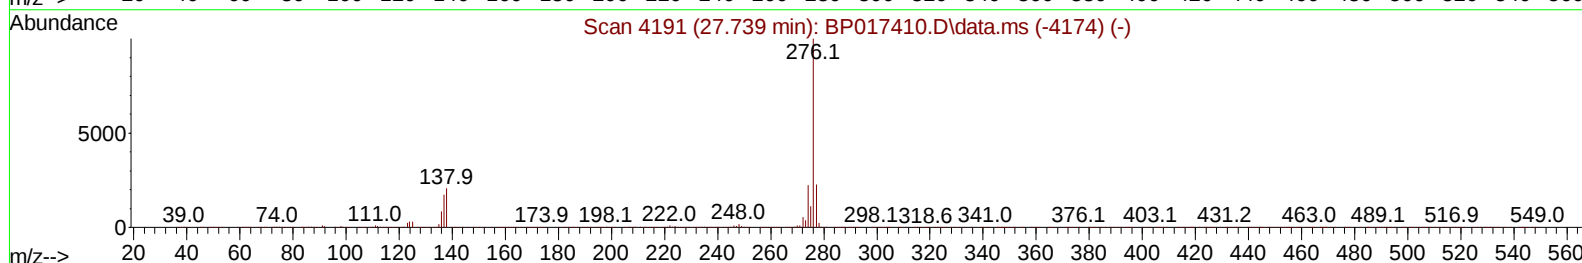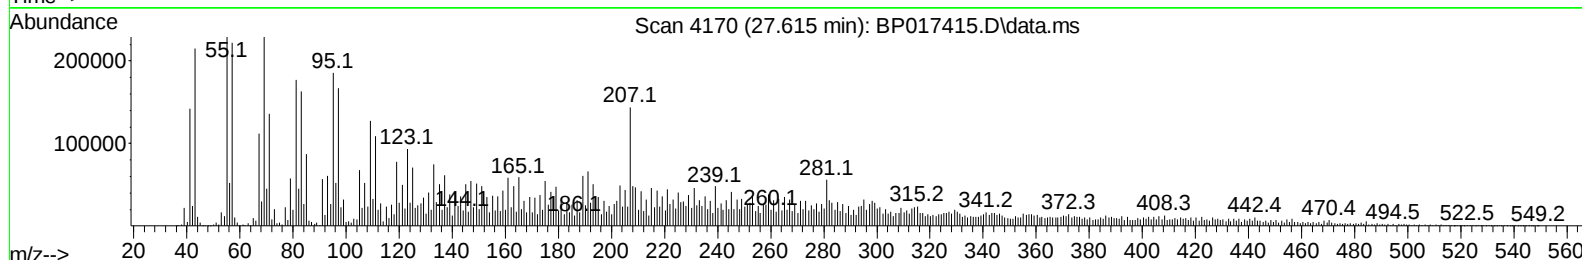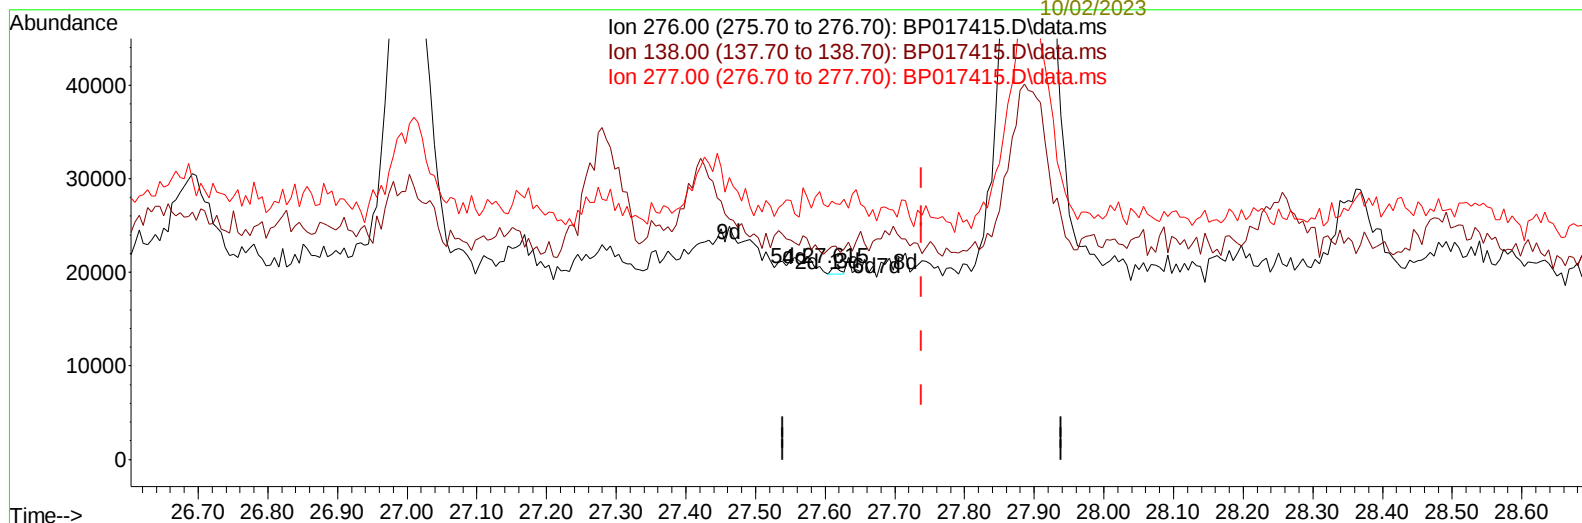

TIC: BP017415.D\data.ms

(96) Benzo(g,h,i)perylene

27.615min (-0.124) 0.01 ng/u1

response 621

Ion	Exp%	Act%
276.00	100.00	100.00
138.00	21.60	111.09#
277.00	23.50	132.85#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP092823\
Data File : BP017415.D
Acq On : 28 Sep 2023 15:49
Operator : MA/JU
Sample : 04417-24
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
EZYF0

Manual IntegrationsAPPROVED

Quant Time: Sep 28 23:12:09 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP092023.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Sep 28 15:31:53 2023
Response via : Initial Calibration

Reviewed By :Yogesh


Patel

09/29/2023


Supervised By :mohammad
ahmed

10/02/2023


Ion 276.00 (275.70 to 276.70): BP017415.D\data.ms
Ion 138.00 (137.70 to 138.70): BP017415.D\data.ms
Ion 277.00 (276.70 to 277.70): BP017415.D\data.ms

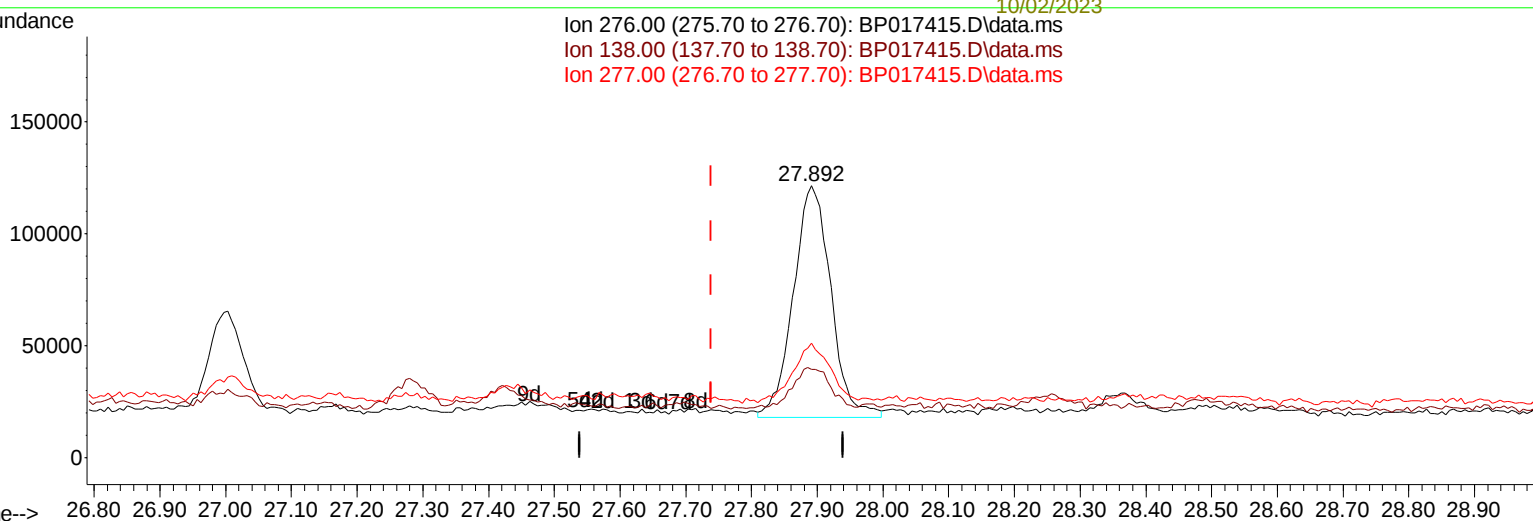

Scan 4217 (27.892 min): BP017415.D\data.ms

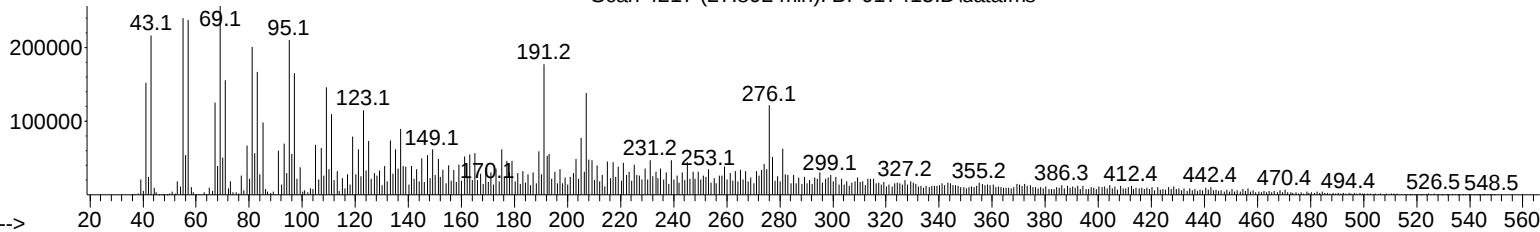

Scan 4191 (27.739 min): BP017410.D\data.ms (-4174) (-)

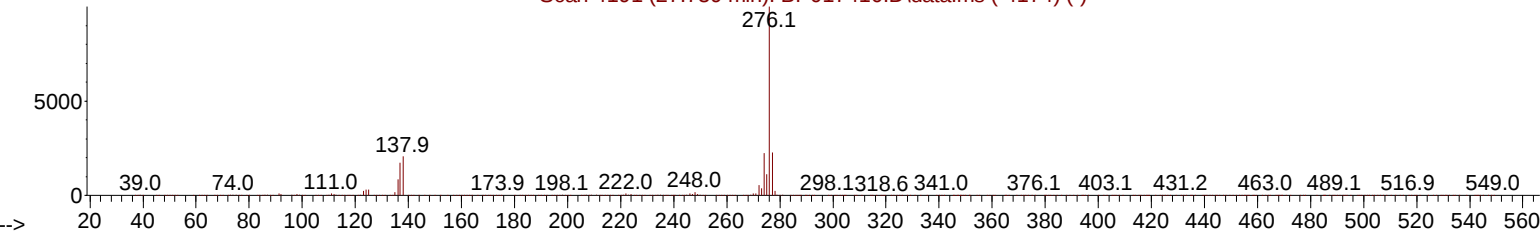

TIC: BP017415.D\data.ms

(96) Benzo(g,h,i)perylene

27.892min (+ 0.153) 5.99 ng/u1 m

response 406756

Ion	Exp%	Act%
276.00	100.00	100.00
138.00	21.60	32.46#
277.00	23.50	42.03#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP092823\
 Data File : BP017415.D
 Acq On : 28 Sep 2023 15:49
 Operator : MA/JU
 Sample : 04417-24
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 EZYF0

Manual IntegrationsAPPROVED

Reviewed By :Yogesh
 Patel
 09/29/2023

Supervised By :mohammad
 ahmed
 10/02/2023

Quant Time: Sep 28 23:12:36 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP092023.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Sep 28 15:31:53 2023
 Response via : Initial Calibration

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Dichlorobenzene-d4	7.963	152		207603	20.000	ng/ul	0.00
20) Naphthalene-d8	10.798	136		897330	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.657	164		542493	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.445	188		1138318	20.000	ng/ul	0.00
79) Chrysene-d12	21.580	240		953884	20.000	ng/ul	# 0.00
88) Perylene-d12	24.198	264		1191021m	20.000	ng/ul	0.05
System Monitoring Compounds							
3) 1,4-Dioxane-d8	3.299	96		24599	4.867	ng/uL	0.00
4) Pyridine-d5	3.740	84		320767	22.701	ng/ul	0.00
7) Phenol-d5	7.116	99		460041	26.981	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.299	67		316284	30.738	ng/ul	0.00
11) 2-Chlorophenol-d4	7.481	132		324154	23.970	ng/ul	0.00
15) 4-Methylphenol-d8	8.681	113		349831	26.391	ng/ul	0.00
21) Nitrobenzene-d5	9.169	128		209345	32.271	ng/ul	0.00
24) 2-Nitrophenol-d4	9.887	143		141773	20.127	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.416	165		196758	14.785	ng/ul	0.00
31) 4-Chloroaniline-d4	10.969	131		241129	12.508	ng/ul	0.00
46) Dimethylphthalate-d6	14.069	166		1170814	30.127	ng/ul	0.00
49) Acenaphthylene-d8	14.351	160		1343096	30.049	ng/ul	0.00
54) 4-Nitrophenol-d4	14.916	143		3644	0.538	ng/ul	0.04
60) Fluorene-d10	15.657	176		1023762	30.599	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.798	200		2024	0.315	ng/ul	0.00
73) Anthracene-d10	17.545	188		1560141	30.903	ng/ul	0.00
81) Pyrene-d10	19.798	212		1668552	32.347	ng/ul	0.00
92) Benzo(a)pyrene-d12	24.027	264		1684093m	29.368	ng/ul	0.05
Target Compounds							
						Qvalue	
80) Fluoranthene	19.463	202		157202	2.613	ng/ul#	94
82) Pyrene	19.827	202		353688	5.531	ng/ul	97
85) Benzo(a)anthracene	21.563	228		93129	1.447	ng/ul#	35
86) Bis(2-ethylhexyl)phtha...	21.439	149		99157	3.028	ng/ul#	70
87) Chrysene	21.598	228		279780m	4.618	ng/ul	
90) Benzo(b)fluoranthene	23.380	252		259991m	3.702	ng/ul	
91) Benzo(k)fluoranthene	23.427	252		92063m	1.299	ng/ul	
93) Benzo(a)pyrene	24.080	252		180126m	2.681	ng/ul	
94) Indeno(1,2,3-cd)pyrene	27.004	276		171118m	2.032	ng/ul	
96) Benzo(g,h,i)perylene	27.892	276		406756m	5.989	ng/ul	

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP092823\
Data File : BP017415.D
Acq On : 28 Sep 2023 15:49
Operator : MA/JU
Sample : 04417-24
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
EZYF0

Manual IntegrationsAPPROVED

Quant Time: Sep 28 23:12:36 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP092023.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Sep 28 15:31:53 2023
Response via : Initial Calibration

Reviewed By :Yogesh

Patel

09/29/2023

Supervised By :mohammad
ahmed

10/02/2023

