

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP092823\
 Data File : BP017434.D
 Acq On : 29 Sep 2023 03:07
 Operator : MA/JU
 Sample : 04472-14
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 EZYM3

Quant Time: Sep 29 04:43:56 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP092023.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Sep 28 23:22:11 2023
 Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.957	152	144030	20.000	ng/u1	0.00
20) Naphthalene-d8	10.798	136	601790	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.651	164	376173	20.000	ng/u1	-0.01
64) Phenanthrene-d10	17.439	188	867711	20.000	ng/u1	-0.01
79) Chrysene-d12	21.568	240	782885	20.000	ng/u1	-0.01
88) Perylene-d12	24.145	264	913221	20.000	ng/u1	-0.03
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.299	96	9126	2.603	ng/uL	0.00
4) Pyridine-d5	3.752	84	13908	1.419	ng/u1	0.01
7) Phenol-d5	7.110	99	228169	19.289	ng/u1	-0.01
9) Bis-(2-Chloroethyl)eth...	7.299	67	145519	20.384	ng/u1	0.00
11) 2-Chlorophenol-d4	7.475	132	160277	17.083	ng/u1	0.00
15) 4-Methylphenol-d8	8.675	113	132552	14.413	ng/u1	-0.01
21) Nitrobenzene-d5	9.163	128	101853	23.411	ng/u1	-0.01
24) 2-Nitrophenol-d4	9.887	143	73628	15.586	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.410	165	146078	16.368	ng/u1	-0.01
31) 4-Chloroaniline-d4	10.969	131	224451	17.361	ng/u1	0.00
46) Dimethylphthalate-d6	14.063	166	621399	23.059	ng/u1	-0.01
49) Acenaphthylene-d8	14.351	160	724050	23.361	ng/u1	-0.01
54) 4-Nitrophenol-d4	14.892	143	20891	4.450	ng/u1	0.00
60) Fluorene-d10	15.657	176	559114	24.100	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.798	200	7762	1.587	ng/u1	-0.02
73) Anthracene-d10	17.539	188	852660	22.156	ng/u1	-0.01
81) Pyrene-d10	19.792	212	1110850	26.239	ng/u1	-0.01
92) Benzo(a)pyrene-d12	23.974	264	1034986	23.539	ng/u1	-0.03
Target Compounds						
16) Acetophenone	8.816	105	48758	3.431	ng/u1	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP092823\
Data File : BP017434.D
Acq On : 29 Sep 2023 03:07
Operator : MA/JU
Sample : 04472-14
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
EZYM3

Quant Time: Sep 29 04:43:56 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP092023.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Sep 28 23:22:11 2023
Response via : Initial Calibration

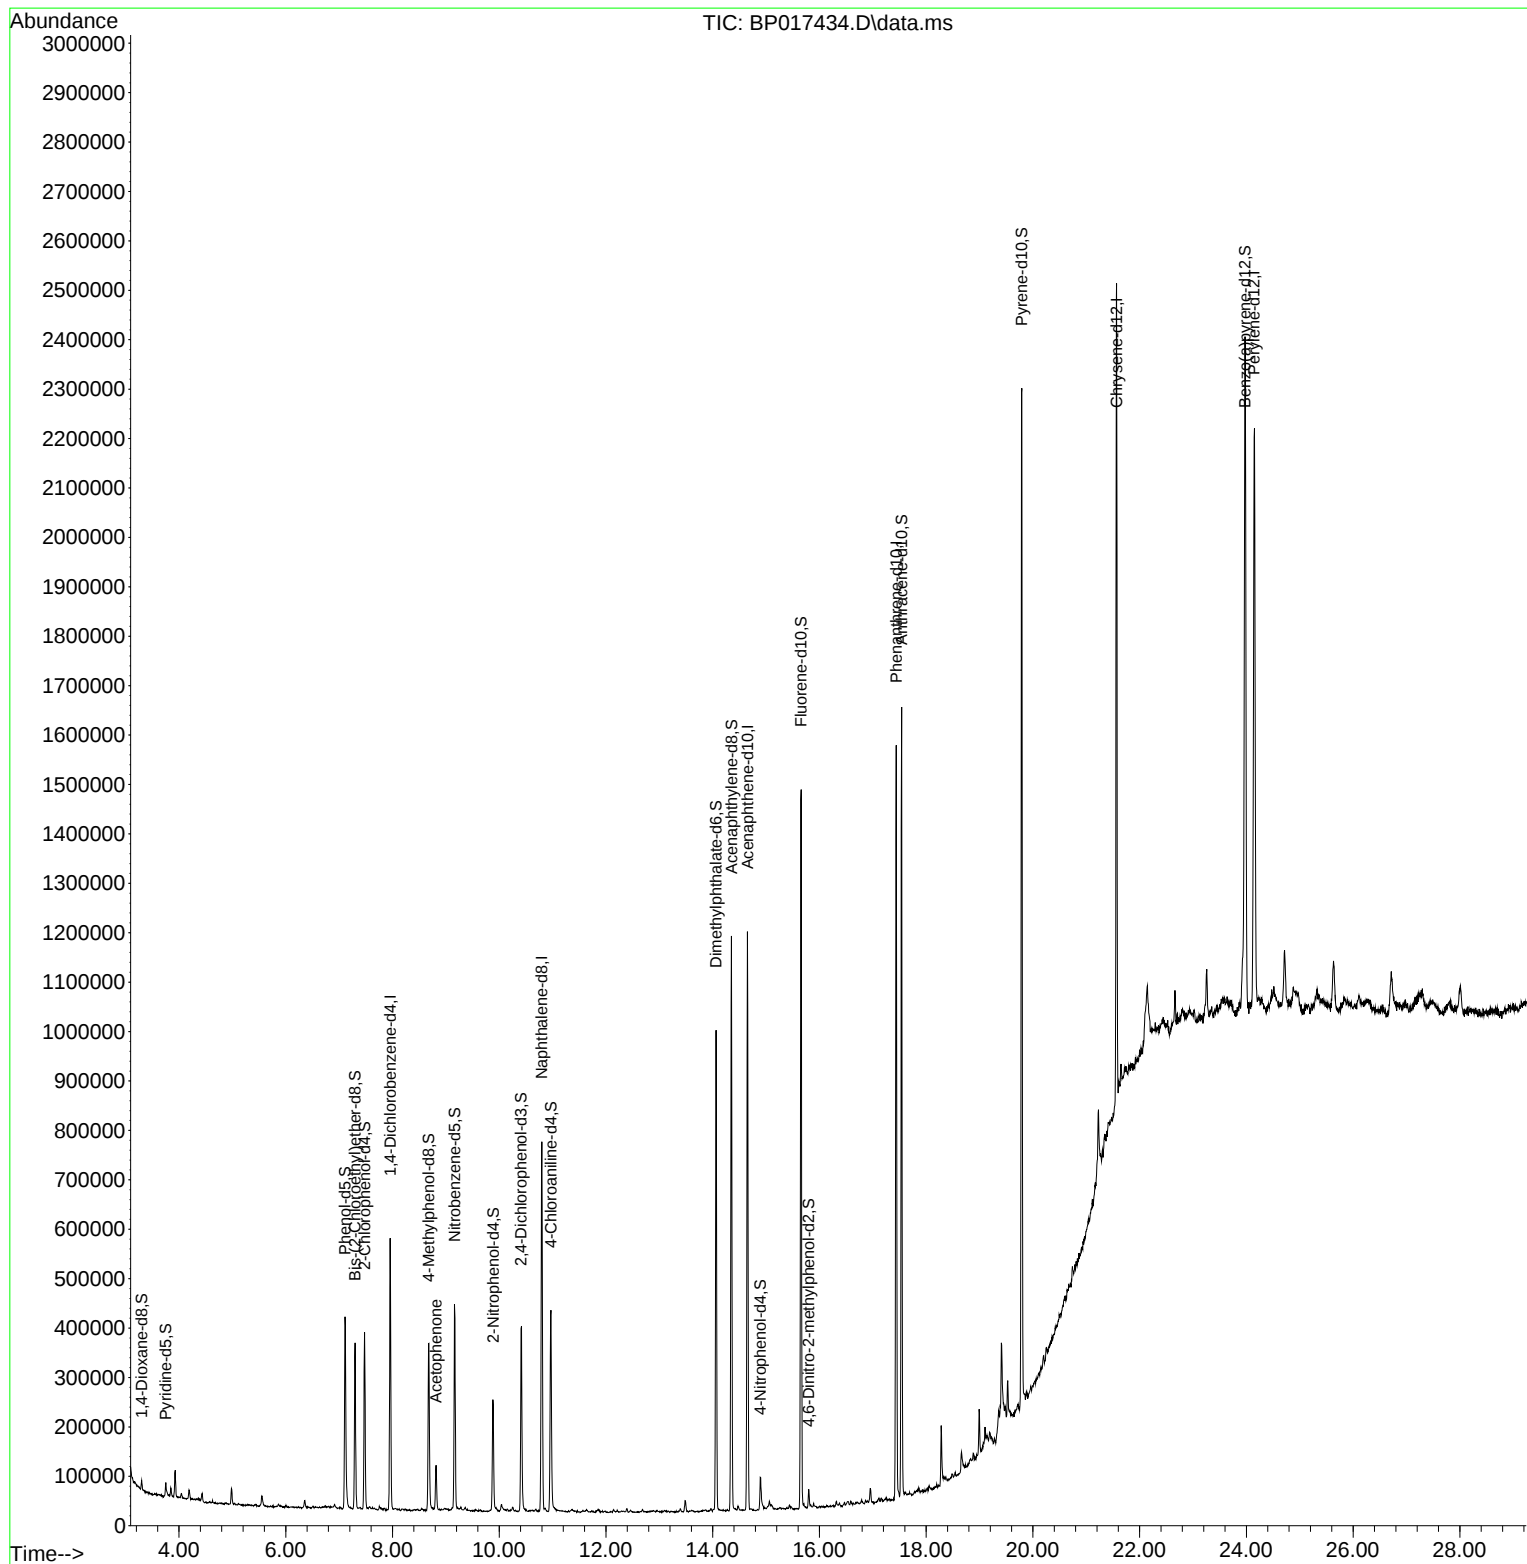

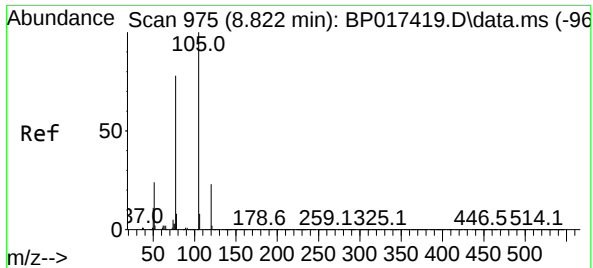

#16
 Acetophenone
 Concen: 3.431 ng/ul
 RT: 8.816 min Scan# 91
 Delta R.T. -0.006 min
 Lab File: BP017434.D
 Acq: 29 Sep 2023 03:07

Instrument :
 BNA_P
 ClientSampleId :
 EZYM3

Tgt Ion:	105	Resp:	48758
Ion	Ratio	Lower	Upper
105	100		
77	80.2	63.6	95.4
51	24.6	19.2	28.8

