

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP092823\
 Data File : BP017412.D
 Acq On : 28 Sep 2023 14:08
 Operator : MA/JU
 Sample : 04417-24 20X
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 EZYF0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP092023.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP017412.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.758	112	114	121	rBV3	14712	25782	1.24%	0.226%
2	4.046	159	163	169	rVB2	11006	16791	0.80%	0.147%
3	5.028	327	330	332	rBV4	3113	4242	0.20%	0.037%
4	5.052	332	334	337	rVB4	3679	2481	0.12%	0.022%
5	5.140	348	349	352	rVB3	2774	2193	0.11%	0.019%
6	5.305	374	377	380	rBV5	2214	2740	0.13%	0.024%
7	5.381	388	390	396	rVB7	1775	3149	0.15%	0.028%
8	5.664	436	438	441	rBV3	2140	2133	0.10%	0.019%
9	6.028	498	500	501	rBV2	2876	2203	0.11%	0.019%
10	6.228	530	534	535	rBV4	2024	2380	0.11%	0.021%
11	6.352	552	555	559	rBV5	2371	3610	0.17%	0.032%
12	6.558	586	590	593	rBV6	2399	3099	0.15%	0.027%
13	6.858	638	641	643	rBV3	2685	3374	0.16%	0.030%
14	7.116	679	685	691	rBV	22976	43009	2.06%	0.377%
15	7.299	708	716	726	rBV	29529	53518	2.56%	0.469%
16	7.475	739	746	754	rBV	22560	43513	2.09%	0.381%
17	7.558	759	760	765	rVB5	2185	2423	0.12%	0.021%
18	7.834	805	807	812	rVB6	1833	2852	0.14%	0.025%
19	7.958	817	828	840	rBV	589308	935347	44.82%	8.196%
20	8.405	902	904	908	rVB4	1751	2137	0.10%	0.019%
21	8.540	924	927	934	rBV9	1986	3974	0.19%	0.035%
22	8.681	945	951	960	rBV2	24261	49801	2.39%	0.436%
23	8.822	973	975	980	rVB6	3254	4086	0.20%	0.036%
24	8.899	985	988	993	rVV7	1783	2426	0.12%	0.021%
25	9.128	1022	1027	1028	rBV5	1975	2691	0.13%	0.024%
26	9.163	1028	1033	1044	rVB2	26228	49634	2.38%	0.435%
27	9.528	1093	1095	1097	rBV3	2043	2301	0.11%	0.020%
28	9.646	1110	1115	1117	rBV6	2485	3608	0.17%	0.032%
29	9.887	1147	1156	1162	rBV6	9606	20145	0.97%	0.177%
30	9.940	1162	1165	1167	rVB4	1911	2127	0.10%	0.019%
31	10.034	1177	1181	1182	rBV4	1931	2994	0.14%	0.026%
32	10.222	1208	1213	1215	rVB6	2430	2464	0.12%	0.022%
33	10.422	1239	1247	1255	rBV8	10202	26184	1.25%	0.229%
34	10.640	1281	1284	1285	rBV3	3247	3278	0.16%	0.029%
35	10.687	1290	1292	1295	rBV3	2382	2298	0.11%	0.020%
36	10.793	1303	1310	1322	rBV	866285	1458773	69.91%	12.783%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP092823\
 Data File : BP017412.D
 Acq On : 28 Sep 2023 14:08
 Operator : MA/JU
 Sample : 04417-24 20X
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 EZYF0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP092023.MA.M
 Title : SVOA CALIBRATION

37	10.869	1322	1323	1329	rVB6	4656	4174	0.20%	0.037%
38	10.975	1336	1341	1353	rVB3	9132	24421	1.17%	0.214%
39	11.504	1427	1431	1432	rBV4	3040	2699	0.13%	0.024%
40	12.146	1536	1540	1543	rBV6	2768	4245	0.20%	0.037%
41	13.393	1747	1752	1753	rBV5	3607	3800	0.18%	0.033%
42	13.487	1760	1768	1773	rBV7	10508	19313	0.93%	0.169%
43	13.569	1777	1782	1786	rVB8	1915	4193	0.20%	0.037%
44	13.934	1842	1844	1847	rBV4	2068	2331	0.11%	0.020%
45	13.957	1847	1848	1852	rBV4	2165	2265	0.11%	0.020%
46	14.063	1860	1866	1872	rBV	62087	89371	4.28%	0.783%
47	14.345	1907	1914	1924	rBV	64196	106507	5.10%	0.933%
48	14.422	1924	1927	1932	rVV7	3616	5578	0.27%	0.049%
49	14.481	1934	1937	1941	rVV6	2407	3465	0.17%	0.030%
50	14.563	1948	1951	1953	rBV4	2385	3063	0.15%	0.027%
51	14.651	1958	1966	1976	rBV	1235189	1774313	85.03%	15.548%
52	14.845	1995	1999	2002	rBV6	2009	3441	0.16%	0.030%
53	15.298	2073	2076	2077	rBV3	3096	2284	0.11%	0.020%
54	15.392	2088	2092	2093	rBV4	3323	4117	0.20%	0.036%
55	15.434	2097	2099	2105	rBV6	4263	7790	0.37%	0.068%
56	15.528	2112	2115	2119	rVB6	2083	2821	0.14%	0.025%
57	15.563	2119	2121	2123	rBV3	2895	2694	0.13%	0.024%
58	15.651	2128	2136	2142	rBV	94754	148026	7.09%	1.297%
59	15.839	2165	2168	2173	rVB7	4917	8082	0.39%	0.071%
60	15.881	2173	2175	2178	rBV4	1993	2148	0.10%	0.019%
61	15.998	2193	2195	2197	rVB2	3521	3106	0.15%	0.027%
62	16.057	2203	2205	2207	rBV3	2669	2839	0.14%	0.025%
63	16.322	2246	2250	2256	rBV7	10569	21308	1.02%	0.187%
64	16.616	2299	2300	2306	rBV6	3609	4596	0.22%	0.040%
65	17.063	2374	2376	2377	rBV2	4102	2529	0.12%	0.022%
66	17.169	2390	2394	2398	rVB6	12156	16973	0.81%	0.149%
67	17.439	2433	2440	2451	rBV	1322071	1880907	90.14%	16.482%
68	17.539	2452	2457	2465	rVV2	79482	131650	6.31%	1.154%
69	19.792	2836	2840	2848	rBV2	126377	212409	10.18%	1.861%
70	21.569	3137	3142	3150	rBV2	1512660	2024132	97.00%	17.737%
71	24.145	3575	3580	3589	rVB2	970191	2086734	100.00%	18.285%




Sum of corrected areas: 11412084

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP092823\
Data File : BP017412.D
Acq On : 28 Sep 2023 14:08
Operator : MA/JU
Sample : 04417-24 20X
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
EZYF0

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP092023.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

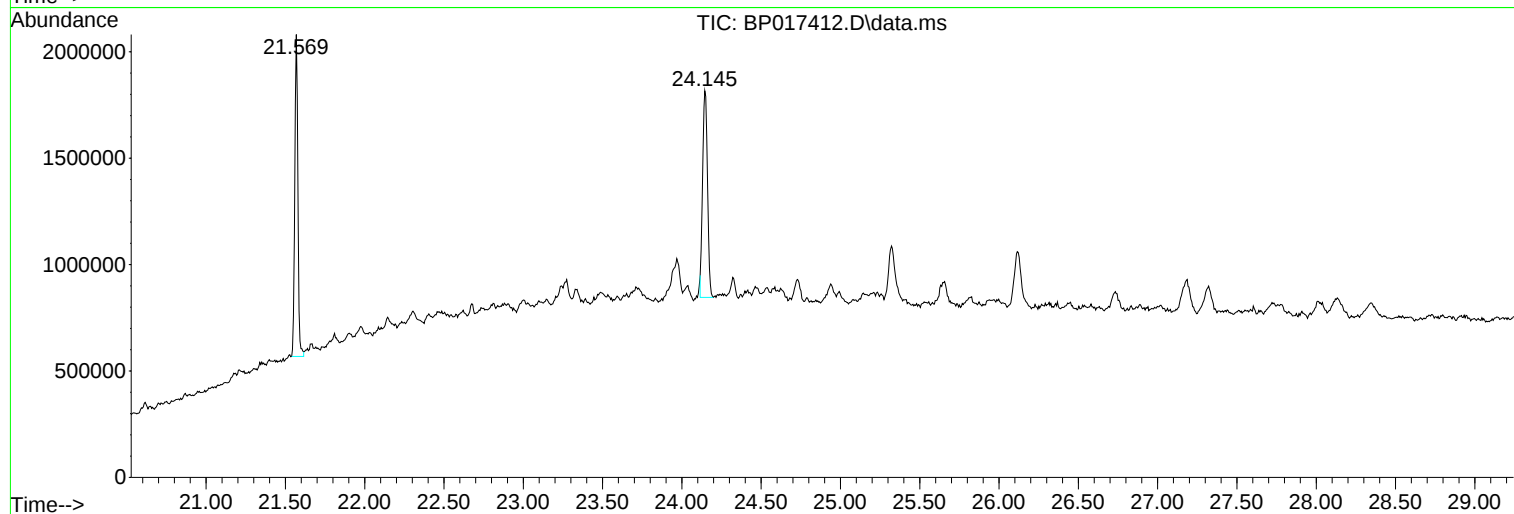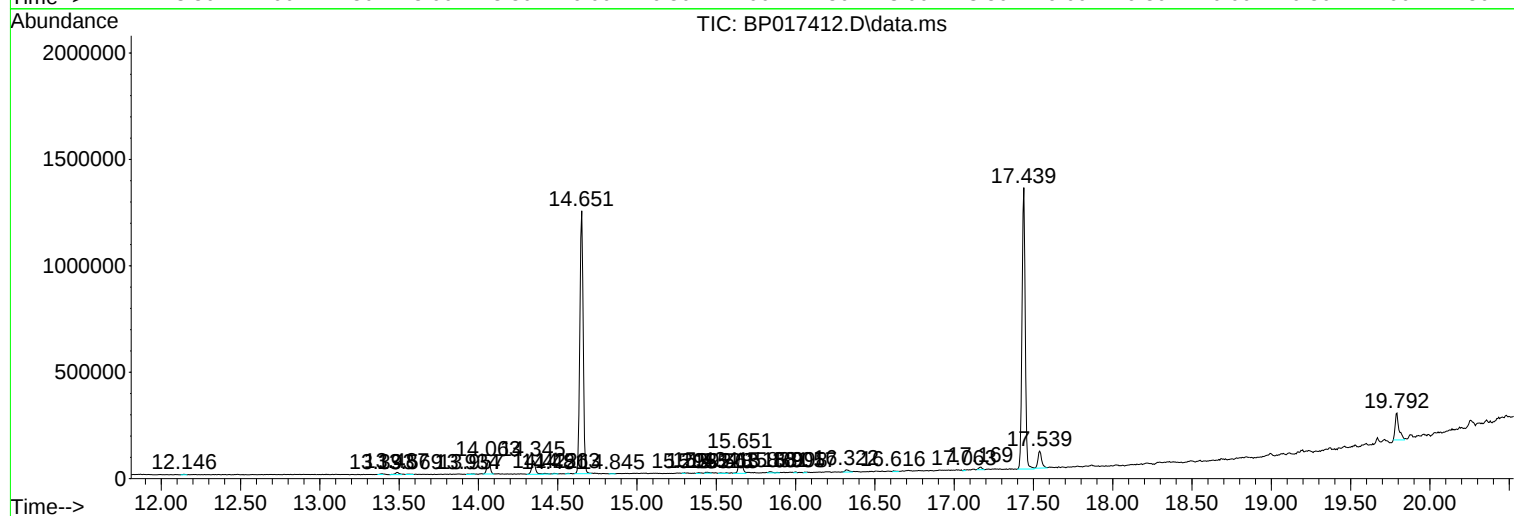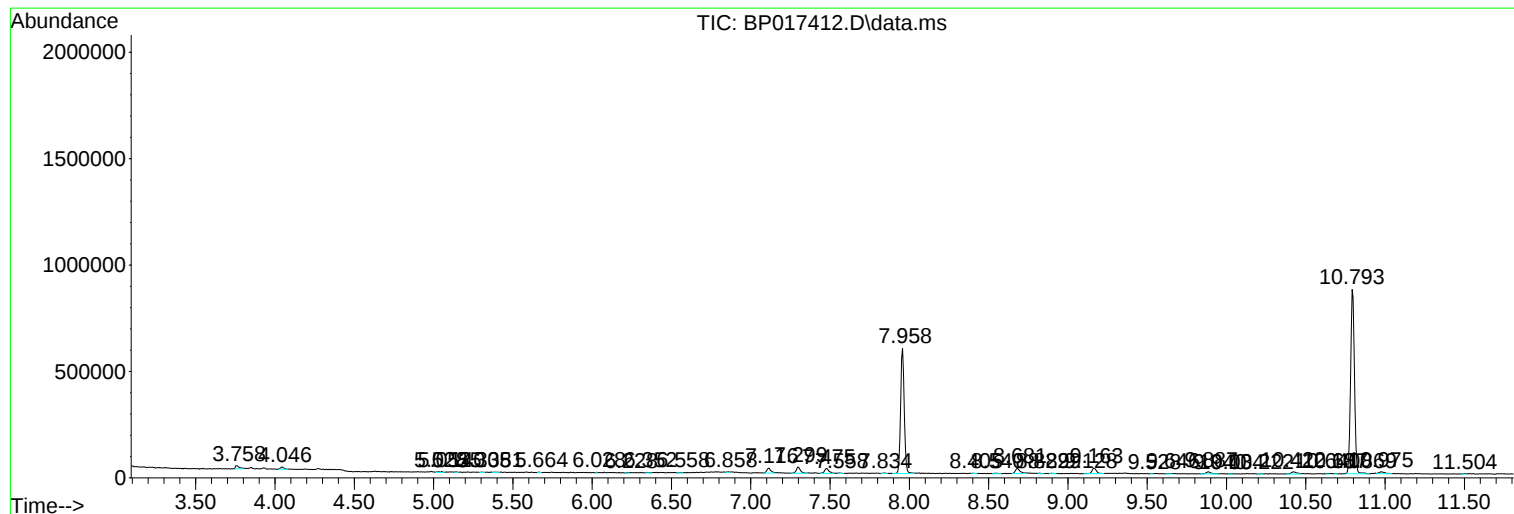

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP092823\
Data File : BP017412.D
Acq On : 28 Sep 2023 14:08
Operator : MA/JU
Sample : 04417-24 20X
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
EZYF0

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP092023.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP092823\
Data File : BP017412.D
Acq On : 28 Sep 2023 14:08
Operator : MA/JU
Sample : 04417-24 20X
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
EZYF0

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP092023.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc