

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP092823\
 Data File : BP017421.D
 Acq On : 28 Sep 2023 19:46
 Operator : MA/JU
 Sample : PB155814BL
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK814

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP092023.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP017421.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.299	33	36	42	rVB	53282	69692	1.27%	0.143%
2	3.734	107	110	127	rBV	653708	976231	17.79%	1.996%
3	7.116	679	685	697	rBV	790546	1269070	23.13%	2.595%
4	7.305	711	717	727	rVB	633731	978432	17.83%	2.001%
5	7.481	740	747	757	rBV	826261	1314924	23.97%	2.689%
6	7.963	823	829	839	rBV	531275	822675	14.99%	1.682%
7	8.687	945	952	963	rBV	941872	1582561	28.85%	3.236%
8	9.169	1027	1034	1042	rBV	749897	1238234	22.57%	2.532%
9	9.887	1148	1156	1168	rBV	618324	1056345	19.25%	2.160%
10	10.422	1239	1247	1258	rBV	966174	1639666	29.89%	3.353%
11	10.804	1305	1312	1321	rVB	740967	1229646	22.41%	2.515%
12	10.969	1332	1340	1355	rBV	958333	1698430	30.96%	3.473%
13	11.828	1477	1486	1488	rBV10	4570	10449	0.19%	0.021%
14	12.398	1578	1583	1589	rBV3	15861	28588	0.52%	0.058%
15	13.492	1764	1769	1775	rBV4	14402	23772	0.43%	0.049%
16	13.610	1785	1789	1795	rBV9	5740	8487	0.15%	0.017%
17	14.069	1858	1867	1877	rBV	1896373	2536828	46.24%	5.188%
18	14.357	1909	1916	1931	rBV2	2022388	3005460	54.78%	6.146%
19	14.657	1960	1967	1975	rBV	1170777	1695570	30.90%	3.468%
20	14.892	2001	2007	2022	rBV	752408	1217731	22.20%	2.490%
21	15.663	2129	2138	2146	rBV	2686219	3775700	68.82%	7.722%
22	15.810	2156	2163	2174	rBV	629572	891535	16.25%	1.823%
23	15.904	2174	2179	2184	rVB5	14349	27467	0.50%	0.056%
24	16.810	2330	2333	2336	rBV5	4003	5689	0.10%	0.012%
25	17.451	2435	2442	2449	rBV	1503277	2173681	39.62%	4.445%
26	17.551	2452	2459	2466	rBV	3114119	4328038	78.89%	8.851%
27	19.804	2836	2842	2847	rBV	3891619	5232023	95.36%	10.700%
28	21.580	3140	3144	3149	rVB	1731804	2169654	39.55%	4.437%
29	23.998	3549	3555	3565	rVB2	2573082	5486409	100.00%	11.220%
30	24.168	3579	3584	3593	rVB	1157511	2404546	43.83%	4.918%




Sum of corrected areas: 48897533

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP092823\
Data File : BP017421.D
Acq On : 28 Sep 2023 19:46
Operator : MA/JU
Sample : PB155814BL
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK814

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP092023.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

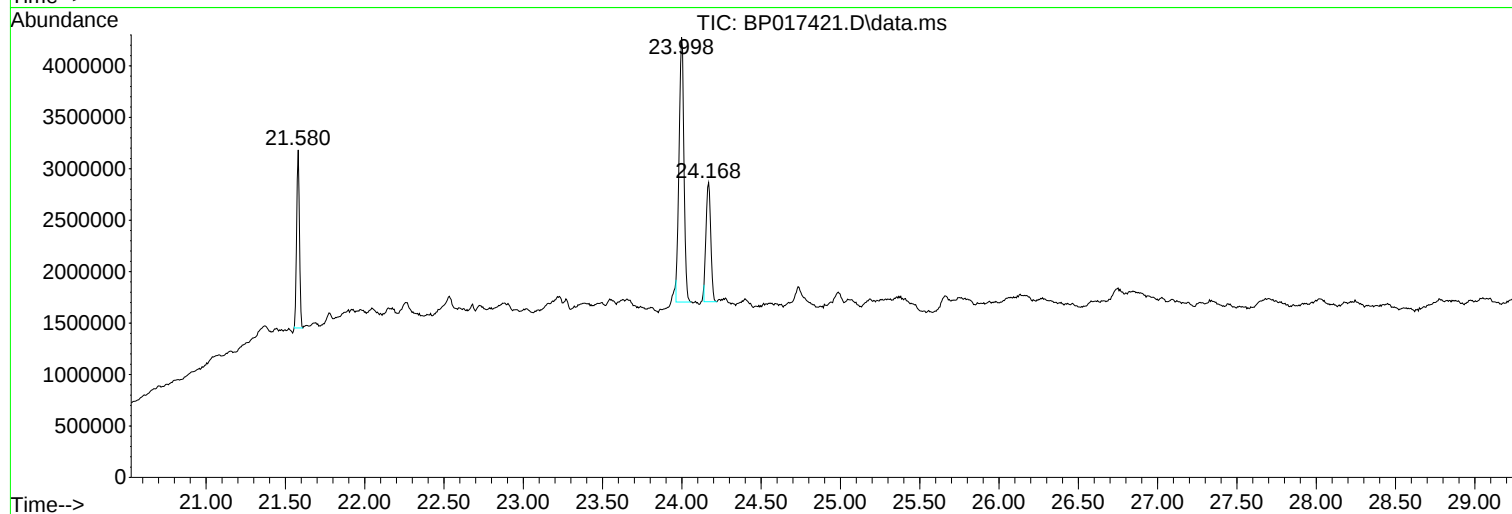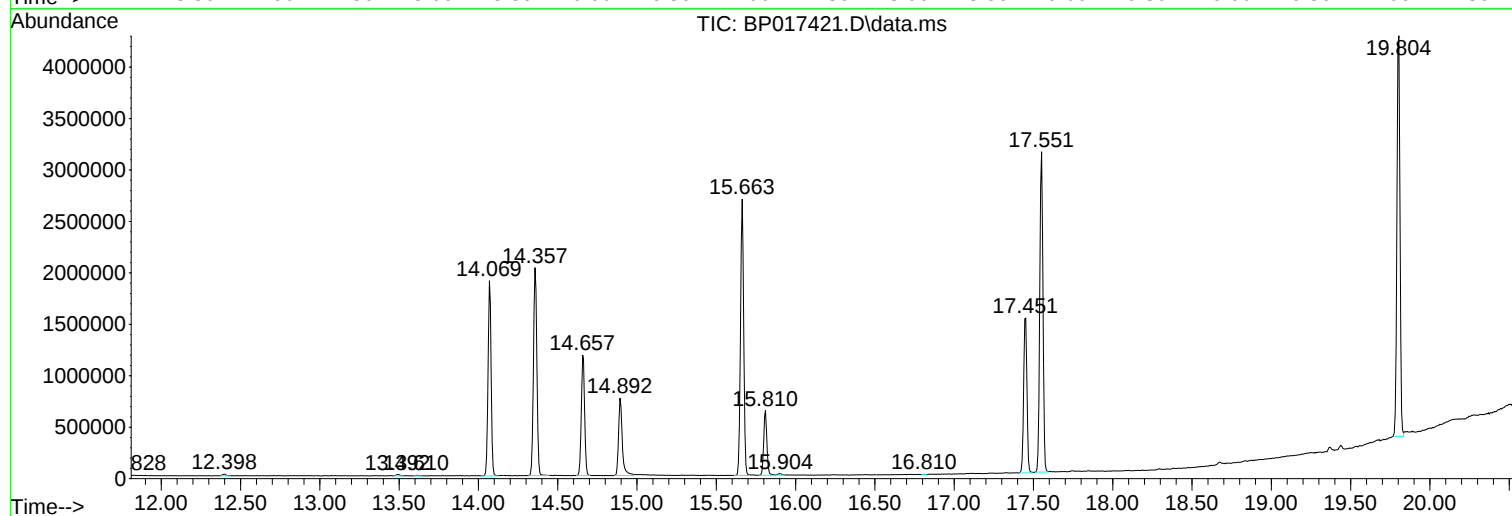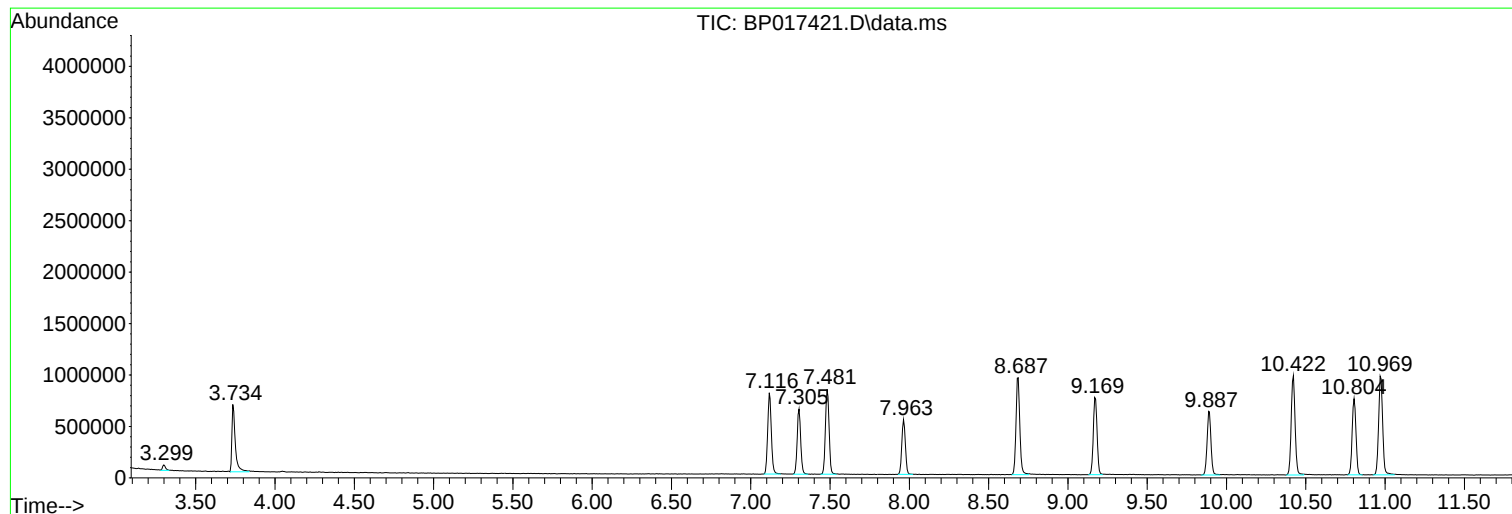

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP092823\
Data File : BP017421.D
Acq On : 28 Sep 2023 19:46
Operator : MA/JU
Sample : PB155814BL
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK814

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP092023.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP092823\
Data File : BP017421.D
Acq On : 28 Sep 2023 19:46
Operator : MA/JU
Sample : PB155814BL
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK814

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP092023.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc