

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP092923\
 Data File : BP017472.D
 Acq On : 30 Sep 2023 06:55
 Operator : MA/JU
 Sample : 04571-08
 Misc :
 ALS Vial : 38 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BBK94

Quant Time: Oct 02 00:56:15 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP092023.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sat Sep 30 04:02:20 2023
 Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.946	152	270493	20.000	ng/u1	0.00
20) Naphthalene-d8	10.787	136	1106900	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.640	164	693141	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.428	188	1586878	20.000	ng/u1	0.00
79) Chrysene-d12	21.557	240	1520980	20.000	ng/u1	0.00
88) Perylene-d12	24.127	264	1683270	20.000	ng/u1	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.299	96	10855	1.648	ng/uL	0.00
4) Pyridine-d5	3.734	84	143676	7.804	ng/u1	0.00
7) Phenol-d5	7.105	99	137091	6.171	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.287	67	178337	13.302	ng/u1	0.00
11) 2-Chlorophenol-d4	7.469	132	167314	9.496	ng/u1	0.00
15) 4-Methylphenol-d8	8.669	113	147573	8.544	ng/u1	0.00
21) Nitrobenzene-d5	9.158	128	118947	14.864	ng/u1	0.00
24) 2-Nitrophenol-d4	9.869	143	86716	9.980	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.399	165	175888	10.714	ng/u1	0.00
31) 4-Chloroaniline-d4	10.957	131	302670	12.728	ng/u1	0.00
46) Dimethylphthalate-d6	14.057	166	770654	15.520	ng/u1	0.00
49) Acenaphthylene-d8	14.340	160	842211	14.747	ng/u1	0.00
54) 4-Nitrophenol-d4	14.887	143	22471	2.598	ng/u1	0.01
60) Fluorene-d10	15.645	176	672190	15.725	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.787	200	19414	2.171	ng/u1	0.00
73) Anthracene-d10	17.528	188	1106559	15.723	ng/u1	0.00
81) Pyrene-d10	19.780	212	1361864	16.558	ng/u1	0.00
92) Benzo(a)pyrene-d12	23.957	264	1270638	15.678	ng/u1	0.00
Target Compounds						
2) 1,4-Dioxane	3.334	88	49705	7.370	ng/uL	94


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP092923\
Data File : BP017472.D
Acq On : 30 Sep 2023 06:55
Operator : MA/JU
Sample : 04571-08
Misc :
ALS Vial : 38 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BBK94

Quant Time: Oct 02 00:56:15 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP092023.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat Sep 30 04:02:20 2023
Response via : Initial Calibration

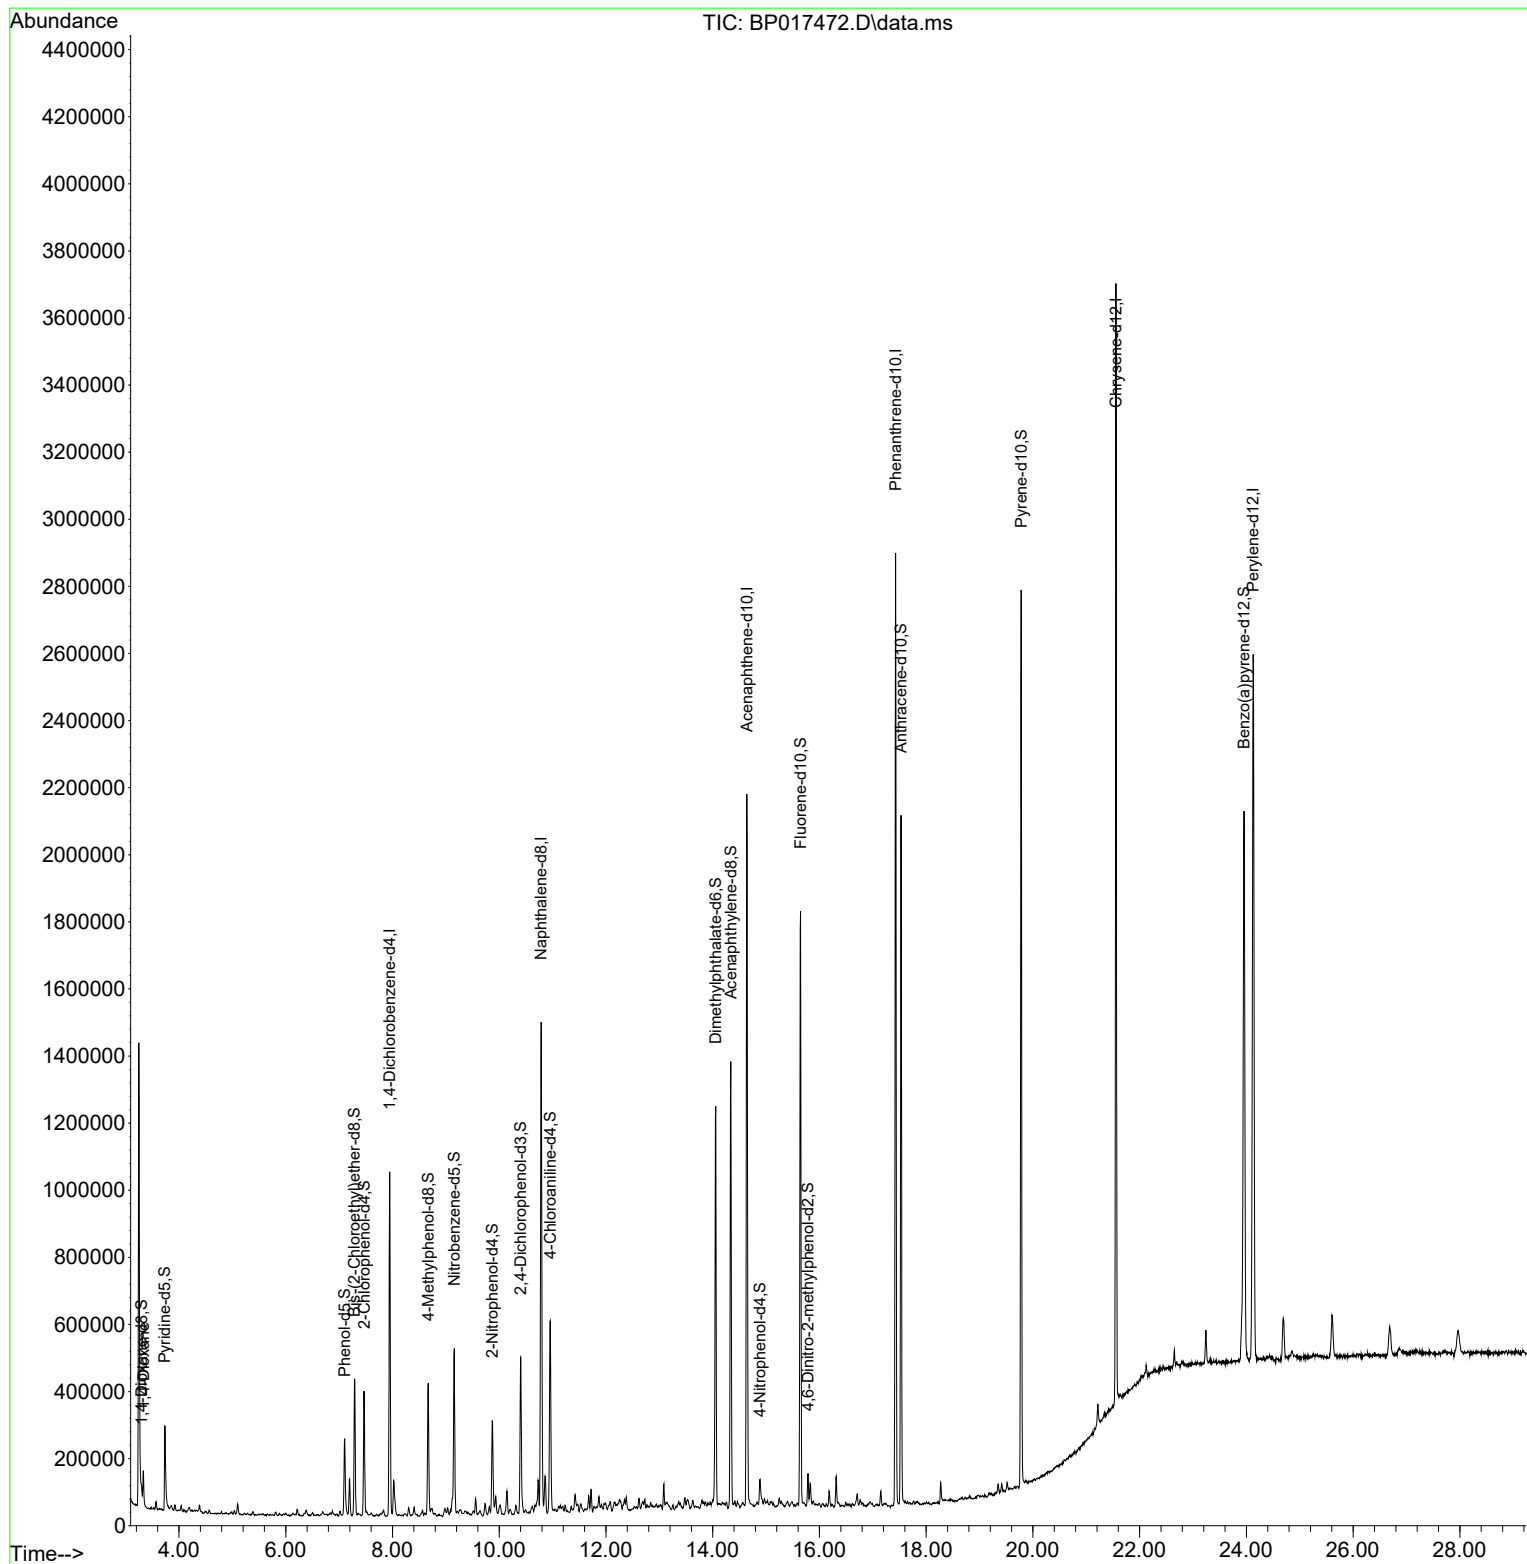

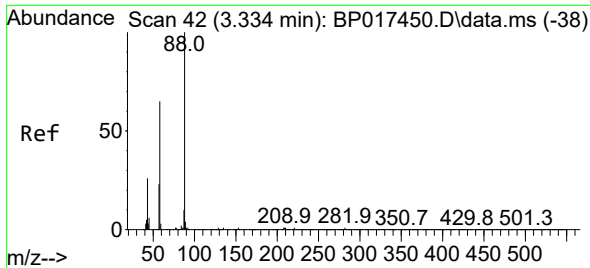

#2
 1,4-Dioxane
 Concen: 7.370 ng/uL
 RT: 3.334 min Scan# 41
 Delta R.T. 0.006 min
 Lab File: BP017472.D
 Acq: 30 Sep 2023 06:55

Instrument :
 BNA_P
 ClientSampleId :
 BBK94

Tgt Ion: 88 Resp: 49705
 Ion Ratio Lower Upper
 88 100
 43 28.3 25.0 37.4
 58 65.0 56.6 84.8

