

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP092923\
 Data File : BP017441.D
 Acq On : 29 Sep 2023 12:14
 Operator : MA/JU
 Sample : 04472-22
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 EZYP5

Quant Time: Sep 29 22:34:19 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP092023.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Sep 29 22:31:03 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.957	152	222075	20.000	ng/ul	0.00
20) Naphthalene-d8	10.799	136	941562	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.651	164	613416	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.439	188	1411646	20.000	ng/ul	0.00
79) Chrysene-d12	21.569	240	1348574	20.000	ng/ul	0.00
88) Perylene-d12	24.145	264	1553668	20.000	ng/ul	-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.299	96	13676	2.529	ng/uL	0.00
4) Pyridine-d5	3.734	84	179652	11.886	ng/ul	0.00
7) Phenol-d5	7.110	99	156063	8.557	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.293	67	361842	32.873	ng/ul	-0.01
11) 2-Chlorophenol-d4	7.475	132	402190	27.803	ng/ul	0.00
15) 4-Methylphenol-d8	8.675	113	278854	19.665	ng/ul	-0.01
21) Nitrobenzene-d5	9.163	128	254274	37.355	ng/ul	0.00
24) 2-Nitrophenol-d4	9.881	143	280990	38.017	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.410	165	458871	32.861	ng/ul	0.00
31) 4-Chloroaniline-d4	10.963	131	655602	32.411	ng/ul	0.00
46) Dimethylphthalate-d6	14.063	166	1600078	36.412	ng/ul	0.00
49) Acenaphthylene-d8	14.351	160	1827131	36.152	ng/ul	0.00
54) 4-Nitrophenol-d4	14.887	143	53119	6.938	ng/ul	0.00
60) Fluorene-d10	15.651	176	1429362	37.783	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.798	200	219871	27.635	ng/ul	0.00
73) Anthracene-d10	17.539	188	2440572	38.982	ng/ul	0.00
81) Pyrene-d10	19.792	212	2907366	39.867	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.980	264	2829123	37.820	ng/ul	0.00
Target Compounds						
					Qvalue	
6) Benzaldehyde	7.116	77	22468	2.414	ng/ul	93


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP092923\
Data File : BP017441.D
Acq On : 29 Sep 2023 12:14
Operator : MA/JU
Sample : 04472-22
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
EZYP5

Quant Time: Sep 29 22:34:19 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP092023.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Sep 29 22:31:03 2023
Response via : Initial Calibration

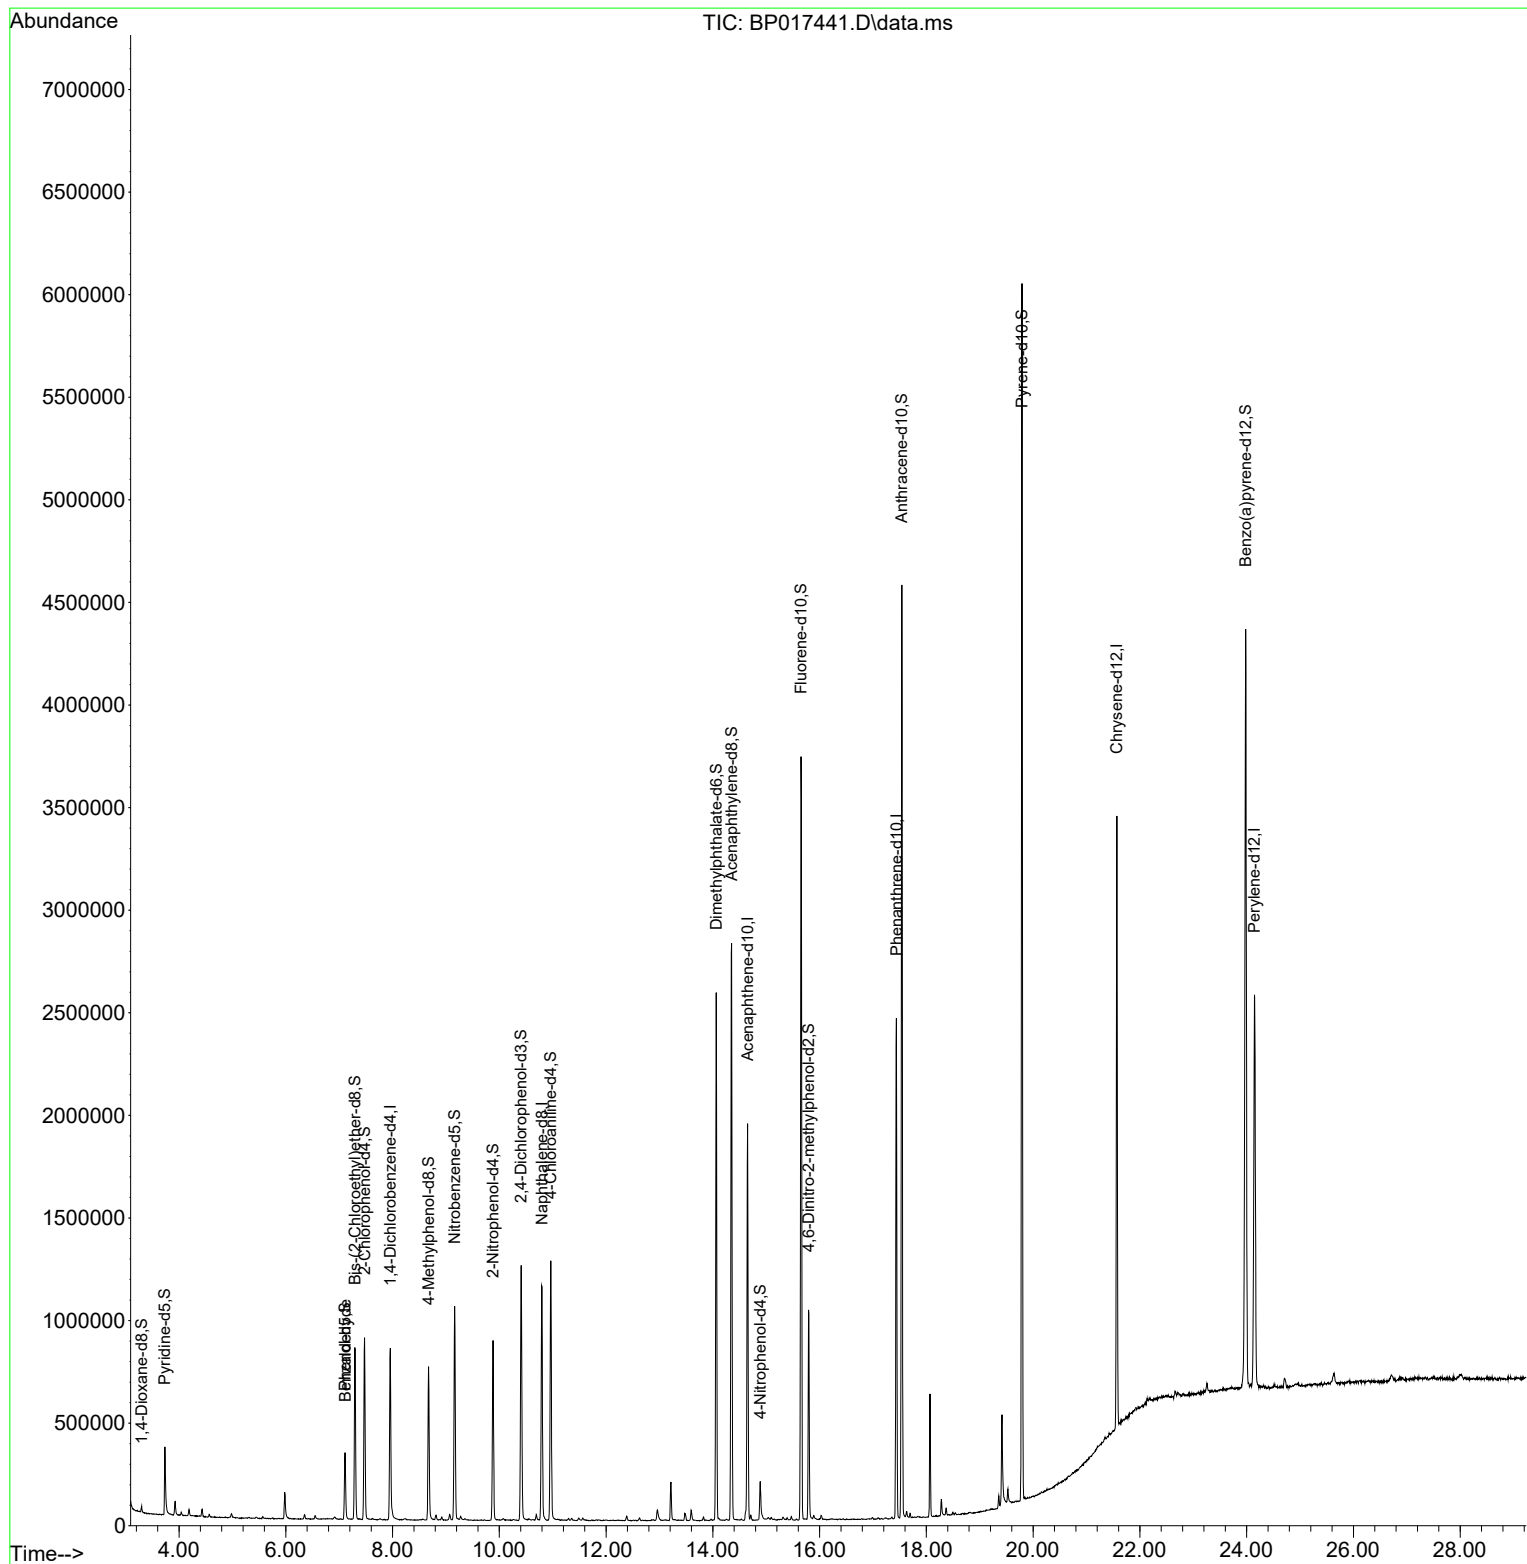

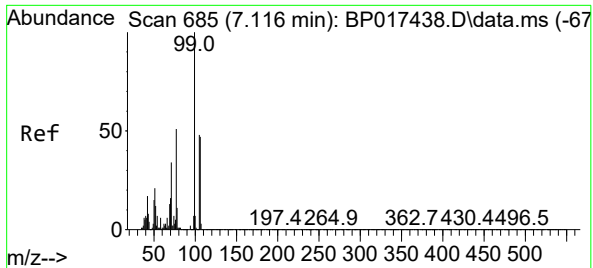

#6
Benzaldehyde
Concen: 2.414 ng/ul
RT: 7.116 min Scan# 61
Delta R.T. -0.000 min
Lab File: BP017441.D
Acq: 29 Sep 2023 12:14

Instrument :
BNA_P
ClientSampleId :
EZYP5

Tgt Ion: 77 Resp: 22468
Ion Ratio Lower Upper
77 100
105 88.4 78.0 117.0
106 87.0 73.2 109.8

