

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP092923\
 Data File : BP017444.D
 Acq On : 29 Sep 2023 13:56
 Operator : MA/JU
 Sample : 04497-07
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BBJC4

Quant Time: Sep 29 22:34:50 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP092023.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Sep 29 22:31:03 2023
 Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.957	152	140981	20.000	ng/ul	0.00
20) Naphthalene-d8	10.793	136	550615	20.000	ng/ul	-0.01
38) Acenaphthene-d10	14.651	164	332529	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.433	188	769954	20.000	ng/ul	-0.01
79) Chrysene-d12	21.569	240	787800	20.000	ng/ul	0.00
88) Perylene-d12	24.145	264	905198	20.000	ng/ul	-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.299	96	10189	2.969	ng/uL	0.00
4) Pyridine-d5	3.734	84	96980	10.107	ng/ul	0.00
7) Phenol-d5	7.110	99	86169	7.442	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.293	67	260327	37.255	ng/ul	-0.01
11) 2-Chlorophenol-d4	7.475	132	266035	28.969	ng/ul	0.00
15) 4-Methylphenol-d8	8.675	113	162702	18.074	ng/ul	-0.01
21) Nitrobenzene-d5	9.163	128	175074	43.982	ng/ul	0.00
24) 2-Nitrophenol-d4	9.881	143	183047	42.350	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.410	165	305159	37.370	ng/ul	0.00
31) 4-Chloroaniline-d4	10.963	131	401866	33.973	ng/ul	0.00
46) Dimethylphthalate-d6	14.063	166	1074317	45.099	ng/ul	0.00
49) Acenaphthylene-d8	14.345	160	1208979	44.127	ng/ul	-0.01
54) 4-Nitrophenol-d4	14.887	143	26392	6.359	ng/ul	0.00
60) Fluorene-d10	15.651	176	959489	46.786	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.792	200	148919	34.316	ng/ul	-0.01
73) Anthracene-d10	17.539	188	1676697	49.101	ng/ul	0.00
81) Pyrene-d10	19.786	212	2094012	49.153	ng/ul	-0.01
92) Benzo(a)pyrene-d12	23.974	264	2092119	48.004	ng/ul	-0.01
Target Compounds						
34) Caprolactam	11.804	113	32481	13.962	ng/ul	Qvalue 98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP092923\
Data File : BP017444.D
Acq On : 29 Sep 2023 13:56
Operator : MA/JU
Sample : 04497-07
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BBJC4

Quant Time: Sep 29 22:34:50 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP092023.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Sep 29 22:31:03 2023
Response via : Initial Calibration

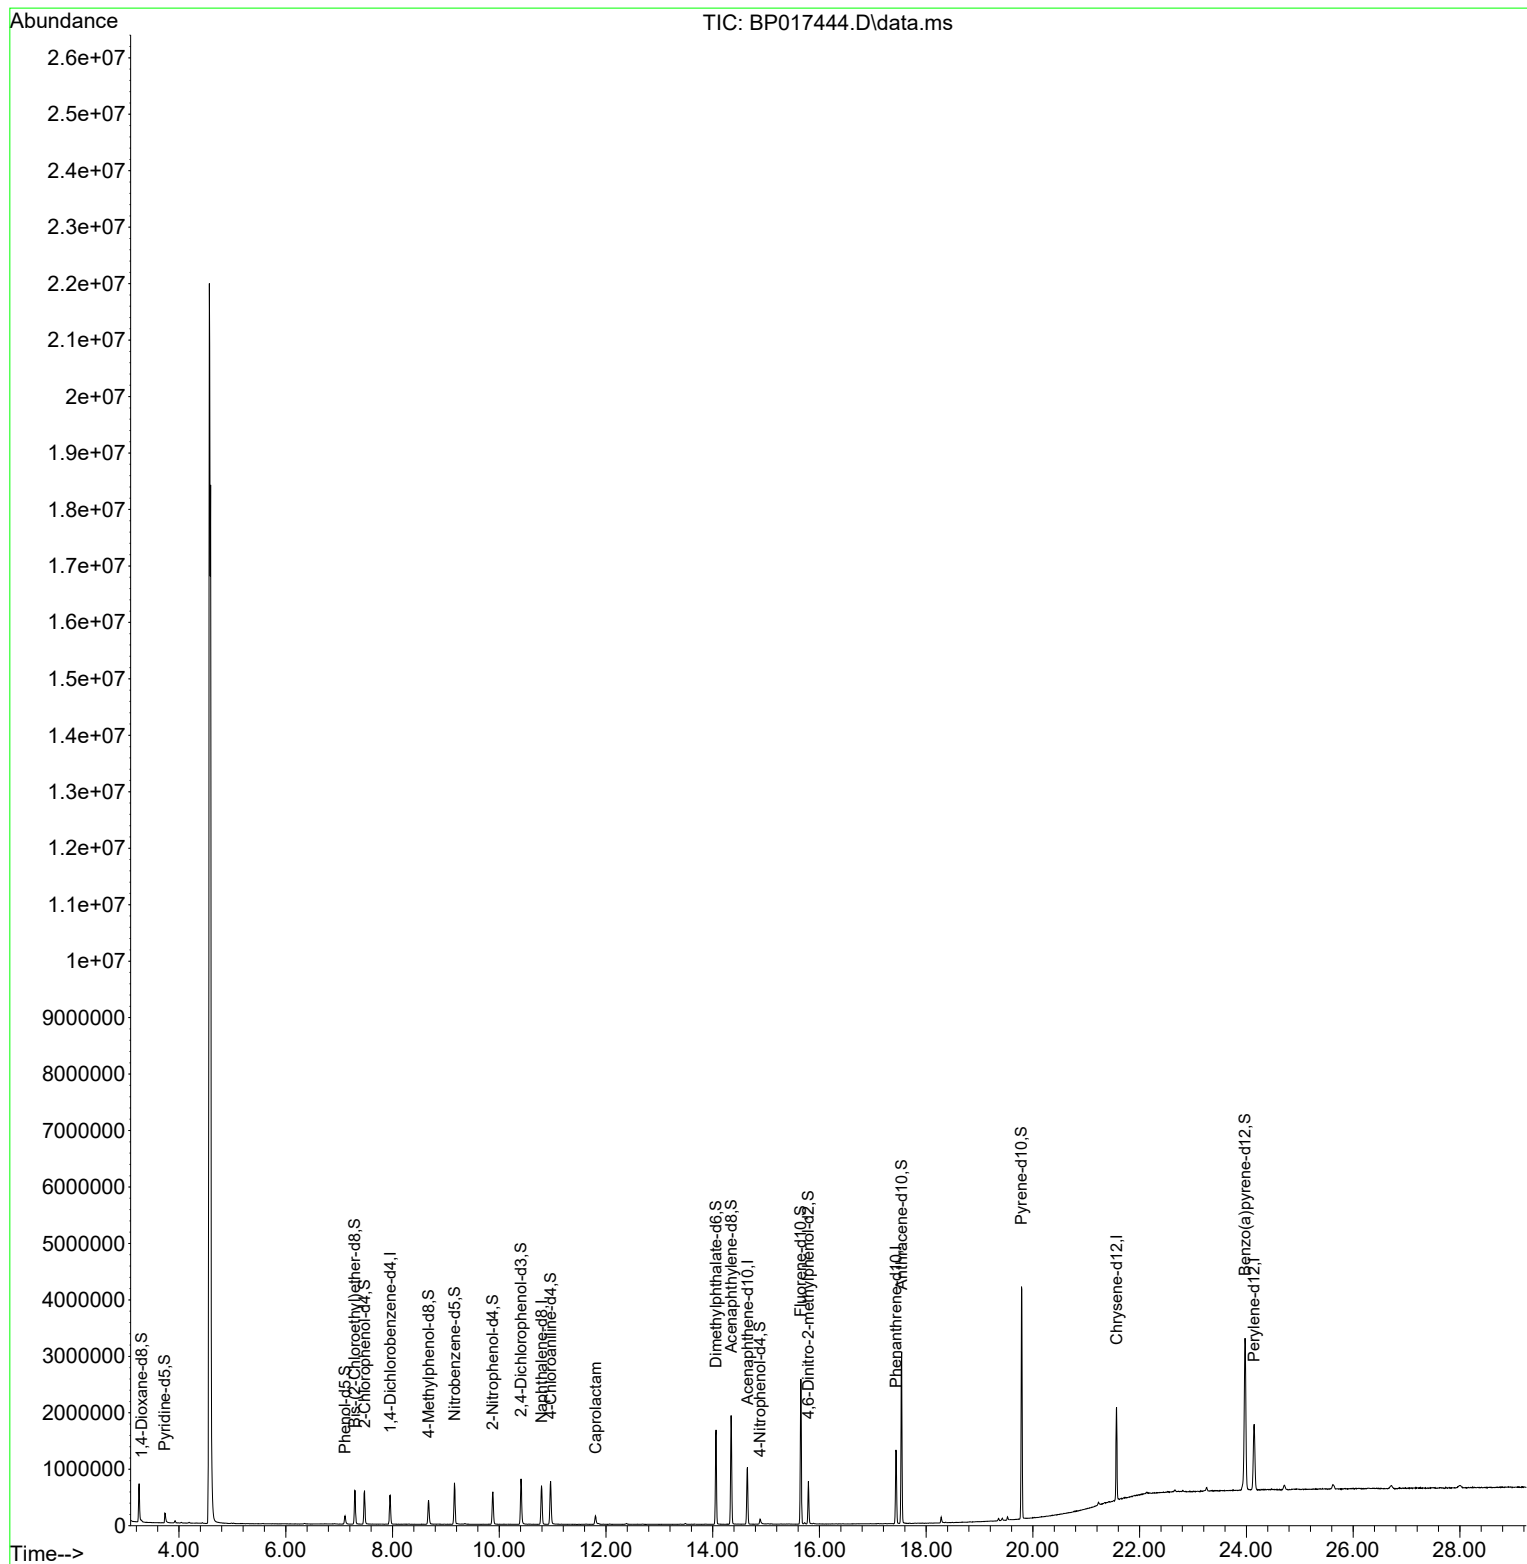

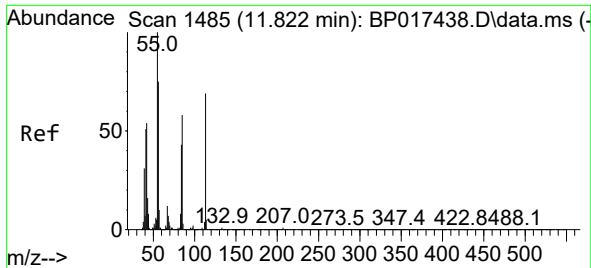

#34
 Caprolactam
 Concen: 13.962 ng/ul
 RT: 11.804 min Scan# 14
 Delta R.T. -0.018 min
 Lab File: BP017444.D
 Acq: 29 Sep 2023 13:56

Instrument :
 BNA_P
 ClientSampleId :
 BBJC4

Tgt Ion:113 Resp: 32481
 Ion Ratio Lower Upper
 113 100
 55 156.7 127.4 191.0
 56 115.1 94.5 141.7

